

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017192.D
 Acq On : 26 Jun 2020 19:22
 Operator : SY/MD
 Sample : L3103-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB	160278	171376	12.98%	1.713%
2	1.579	145	152	162	rBV	112048	122696	9.29%	1.227%
3	2.123	311	321	337	rBV	283499	421992	31.95%	4.219%
4	2.824	537	539	544	rBV6	1386	983	0.07%	0.010%
5	3.045	604	608	609	rBV4	1217	684	0.05%	0.007%
6	3.068	612	615	620	rBV6	1130	944	0.07%	0.009%
7	3.106	624	627	629	rBV3	1077	741	0.06%	0.007%
8	3.158	640	643	645	rBV3	1558	1020	0.08%	0.010%
9	3.222	661	663	666	rBV3	749	547	0.04%	0.005%
10	3.293	681	685	688	rBV3	919	738	0.06%	0.007%
11	3.373	705	710	713	rBV8	1237	1158	0.09%	0.012%
12	3.531	757	759	762	rVB4	1164	662	0.05%	0.007%
13	3.547	762	764	768	rBV3	664	514	0.04%	0.005%
14	3.698	806	811	812	rBV5	1193	879	0.07%	0.009%
15	3.865	857	863	865	rBV5	1212	725	0.05%	0.007%
16	3.907	865	876	894	rBV	91115	240981	18.25%	2.409%
17	4.094	930	934	939	rBV7	1283	1594	0.12%	0.016%
18	4.235	974	978	980	rBV3	1031	727	0.06%	0.007%
19	4.377	1005	1022	1047	rBV	219562	543298	41.14%	5.431%
20	4.637	1102	1103	1105	rBV	1320	637	0.05%	0.006%
21	5.071	1220	1238	1264	rBV2	513304	1320614	100.00%	13.202%
22	5.547	1384	1386	1389	rVB4	844	535	0.04%	0.005%
23	5.640	1403	1415	1445	rBV	425504	854708	64.72%	8.545%
24	6.093	1542	1556	1580	rBV	297419	593691	44.96%	5.935%
25	6.286	1614	1616	1618	rBV3	1427	799	0.06%	0.008%
26	6.309	1620	1623	1627	rBV3	1221	1007	0.08%	0.010%
27	6.373	1640	1643	1645	rBV4	1497	918	0.07%	0.009%
28	6.566	1700	1703	1704	rBV3	1202	545	0.04%	0.005%
29	6.711	1745	1748	1754	rBV8	1798	1624	0.12%	0.016%
30	6.852	1790	1792	1794	rBV3	922	531	0.04%	0.005%
31	6.923	1812	1814	1818	rVB3	1029	512	0.04%	0.005%
32	6.955	1821	1824	1825	rBV3	1012	572	0.04%	0.006%
33	7.007	1828	1840	1862	rBV	167253	300658	22.77%	3.006%
34	7.174	1887	1892	1894	rBV4	1837	1775	0.13%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017192.D
 Acq On : 26 Jun 2020 19:22
 Operator : SY/MD
 Sample : L3103-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.338	1930	1943	1963	rBV	609729	1050411	79.54%	10.501%
36	7.534	2002	2004	2011	rVB8	1395	974	0.07%	0.010%
37	7.640	2028	2037	2052	rBV	123567	204508	15.49%	2.044%
38	7.827	2093	2095	2098	rBV3	1300	731	0.06%	0.007%
39	7.949	2129	2133	2136	rBV5	2044	1919	0.15%	0.019%
40	7.994	2144	2147	2150	rBV5	1363	1068	0.08%	0.011%
41	8.010	2150	2152	2155	rVB4	2182	1122	0.08%	0.011%
42	8.029	2155	2158	2159	rBV3	1106	641	0.05%	0.006%
43	8.055	2164	2166	2168	rBV3	1317	605	0.05%	0.006%
44	8.109	2173	2183	2202	rBV	299568	544786	41.25%	5.446%
45	8.396	2270	2272	2275	rBV5	1580	905	0.07%	0.009%
46	8.698	2362	2366	2370	rBV5	1406	1410	0.11%	0.014%
47	8.756	2380	2384	2388	rVV6	1298	1188	0.09%	0.012%
48	8.804	2396	2399	2401	rBV3	1018	780	0.06%	0.008%
49	8.871	2407	2420	2440	rBV	648213	1047786	79.34%	10.475%
50	9.228	2527	2531	2535	rBV6	1547	1253	0.09%	0.013%
51	9.257	2538	2540	2541	rBV2	981	510	0.04%	0.005%
52	9.347	2565	2568	2573	rBV6	1473	1605	0.12%	0.016%
53	9.396	2581	2583	2586	rVB3	1219	659	0.05%	0.007%
54	9.434	2593	2595	2597	rBV3	1656	964	0.07%	0.010%
55	9.778	2699	2702	2705	rBV4	869	676	0.05%	0.007%
56	9.830	2715	2718	2721	rBV4	1544	984	0.07%	0.010%
57	9.849	2721	2724	2725	rBV3	1404	593	0.04%	0.006%
58	9.949	2752	2755	2757	rBV4	1241	1016	0.08%	0.010%
59	9.965	2757	2760	2764	rVV4	1770	1194	0.09%	0.012%
60	10.084	2794	2797	2802	rVB5	1244	817	0.06%	0.008%
61	10.109	2802	2805	2808	rBV5	1603	1175	0.09%	0.012%
62	10.158	2817	2820	2822	rBV3	1322	820	0.06%	0.008%
63	10.238	2834	2845	2859	rVB	379511	598144	45.29%	5.980%
64	10.354	2876	2881	2882	rBV5	1668	1274	0.10%	0.013%
65	10.659	2972	2976	2977	rBV3	889	578	0.04%	0.006%
66	10.765	3006	3009	3011	rVB4	798	542	0.04%	0.005%
67	10.987	3075	3078	3079	rBV3	1147	554	0.04%	0.006%
68	11.045	3092	3096	3099	rBV3	1291	1086	0.08%	0.011%
69	11.151	3125	3129	3130	rBV4	1457	1084	0.08%	0.011%
70	11.270	3155	3166	3184	rBV	630093	943125	71.42%	9.428%
71	11.424	3212	3214	3217	rBV3	1308	1010	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017192.D
 Acq On : 26 Jun 2020 19:22
 Operator : SY/MD
 Sample : L3103-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3300	rBV	637398	967025	73.23%	9.667%
73	11.823	3336	3338	3340	rBV3	1350	757	0.06%	0.008%
74	11.900	3360	3362	3364	rBV2	1375	826	0.06%	0.008%
75	12.026	3398	3401	3406	rBV6	1321	1236	0.09%	0.012%
76	12.068	3412	3414	3417	rBV2	754	514	0.04%	0.005%
77	12.119	3429	3430	3435	rBV4	1248	1148	0.09%	0.011%
78	12.186	3448	3451	3455	rBV4	1961	1242	0.09%	0.012%
79	12.215	3455	3460	3464	rBV6	1604	1606	0.12%	0.016%
80	12.518	3551	3554	3555	rBV3	1154	662	0.05%	0.007%
81	12.691	3605	3608	3610	rBV4	1057	842	0.06%	0.008%
82	12.736	3620	3622	3626	rVB3	1013	648	0.05%	0.006%
83	12.913	3675	3677	3682	rBV4	933	775	0.06%	0.008%
84	12.965	3691	3693	3696	rBV3	1145	568	0.04%	0.006%
85	13.145	3747	3749	3751	rBV3	1426	655	0.05%	0.007%
86	13.180	3754	3760	3761	rBV3	1549	1174	0.09%	0.012%
87	13.360	3814	3816	3820	rVB4	1262	541	0.04%	0.005%
88	13.688	3914	3918	3920	rBV3	983	649	0.05%	0.006%
89	13.839	3960	3965	3968	rBV5	1477	1382	0.10%	0.014%
90	13.907	3985	3986	3990	rBV2	1264	963	0.07%	0.010%
91	14.141	4057	4059	4061	rBV2	1282	764	0.06%	0.008%
92	14.196	4072	4076	4077	rBV3	885	684	0.05%	0.007%
93	14.334	4114	4119	4120	rBV4	2318	2086	0.16%	0.021%
94	14.466	4158	4160	4162	rBV3	1733	866	0.07%	0.009%
95	14.640	4211	4214	4216	rBV3	1571	911	0.07%	0.009%
96	14.884	4287	4290	4292	rBV3	1334	853	0.06%	0.009%
97	14.964	4311	4315	4318	rBV4	1869	1522	0.12%	0.015%
98	14.981	4318	4320	4321	rBV2	1157	536	0.04%	0.005%
99	15.048	4338	4341	4344	rBV4	1440	1078	0.08%	0.011%
100	15.723	4550	4551	4553	rBV2	1293	545	0.04%	0.005%


Sum of corrected areas: 10002940

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017192.D
Acq On : 26 Jun 2020 19:22
Operator : SY/MD
Sample : L3103-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q23

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

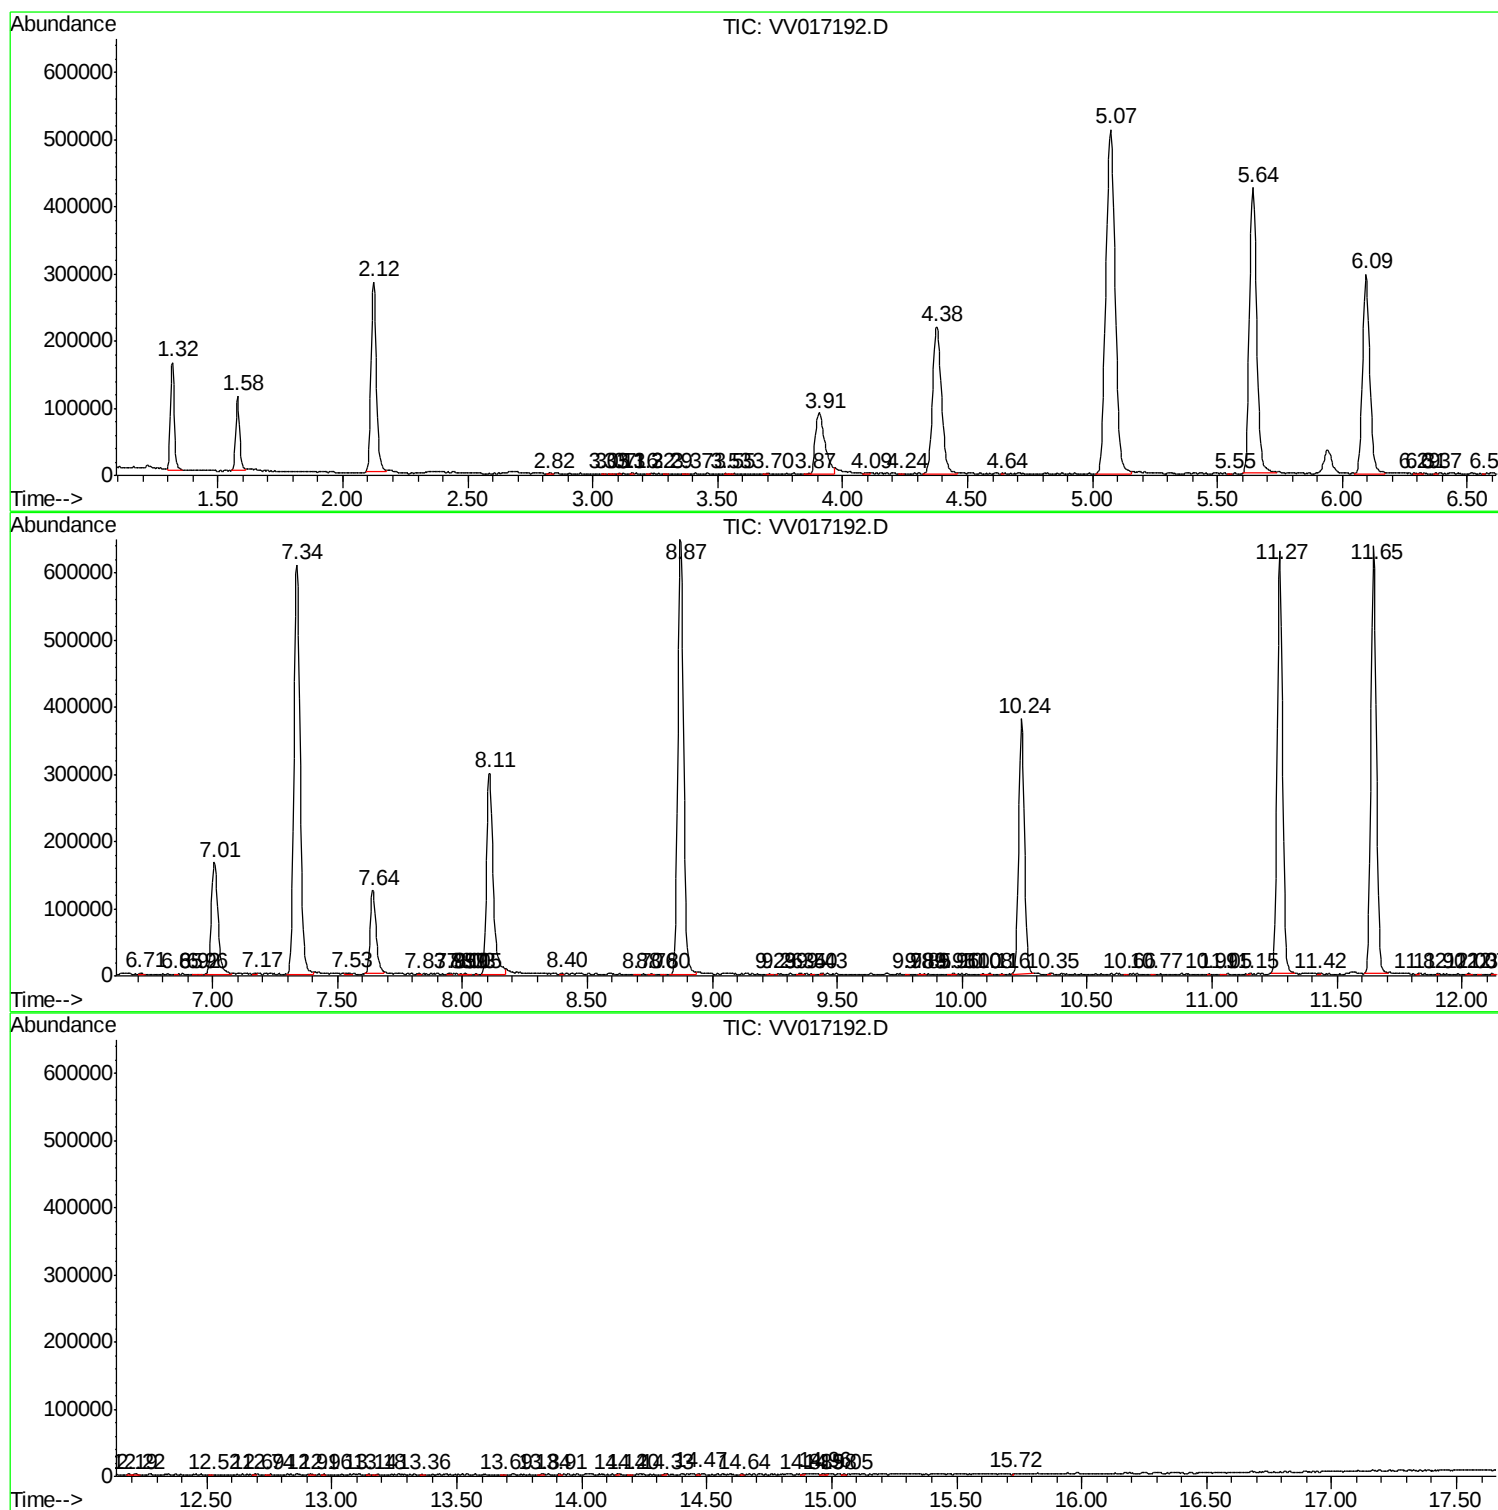

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017192.D
Acq On : 26 Jun 2020 19:22
Operator : SY/MD
Sample : L3103-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q23

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017192.D
Acq On : 26 Jun 2020 19:22
Operator : SY/MD
Sample : L3103-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q23

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc