

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017194.D
 Acq On : 26 Jun 2020 20:09
 Operator : SY/MD
 Sample : L3103-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	82	rVB	158062	165757	12.68%	1.661%
2	1.579	145	152	163	rBV	119868	132078	10.10%	1.323%
3	2.007	283	285	289	rBV4	1617	1263	0.10%	0.013%
4	2.122	312	321	338	rBV	281208	415466	31.78%	4.162%
5	2.521	442	445	446	rBV4	1631	813	0.06%	0.008%
6	2.650	481	485	486	rBV3	1073	752	0.06%	0.008%
7	2.785	524	527	530	rBV4	1381	858	0.07%	0.009%
8	3.055	608	611	613	rBV3	1228	698	0.05%	0.007%
9	3.187	649	652	654	rVB4	1180	670	0.05%	0.007%
10	3.257	672	674	678	rVV4	1623	1330	0.10%	0.013%
11	3.409	716	721	723	rBV5	1367	1059	0.08%	0.011%
12	3.431	723	728	730	rBV4	1202	947	0.07%	0.009%
13	3.508	747	752	755	rBV5	1016	797	0.06%	0.008%
14	3.778	832	836	843	rVB7	1439	1406	0.11%	0.014%
15	3.907	865	876	901	rBV	82349	231251	17.69%	2.317%
16	4.306	997	1000	1003	rBV4	1075	780	0.06%	0.008%
17	4.376	1008	1022	1043	rVV	218388	526389	40.27%	5.273%
18	4.659	1105	1110	1115	rBV9	2106	2495	0.19%	0.025%
19	4.823	1154	1161	1163	rBV7	1370	1455	0.11%	0.015%
20	4.936	1193	1196	1202	rBV6	1247	1244	0.10%	0.012%
21	5.071	1221	1238	1259	rBV3	506975	1307236	100.00%	13.096%
22	5.328	1314	1318	1323	rVV8	2000	1502	0.11%	0.015%
23	5.450	1349	1356	1357	rBV3	1515	1541	0.12%	0.015%
24	5.508	1370	1374	1378	rBV7	1872	1503	0.11%	0.015%
25	5.640	1402	1415	1440	rBV	425543	852362	65.20%	8.539%
26	5.939	1498	1508	1520	rVV8	17391	36726	2.81%	0.368%
27	6.093	1541	1556	1577	rBV	295302	596748	45.65%	5.978%
28	6.277	1610	1613	1618	rBV7	2172	1545	0.12%	0.015%
29	6.331	1625	1630	1635	rBV8	1527	1942	0.15%	0.019%
30	6.608	1714	1716	1719	rVB3	1736	813	0.06%	0.008%
31	6.633	1719	1724	1726	rBV4	2488	1969	0.15%	0.020%
32	6.833	1783	1786	1789	rBV6	1565	1264	0.10%	0.013%
33	6.929	1814	1816	1820	rBV3	1353	894	0.07%	0.009%
34	6.971	1823	1829	1830	rBV4	1431	1084	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017194.D
 Acq On : 26 Jun 2020 20:09
 Operator : SY/MD
 Sample : L3103-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1830	1840	1860	rVV	163416	296152	22.65%	2.967%
36	7.338	1931	1943	1963	rBV	604084	1042024	79.71%	10.439%
37	7.556	2009	2011	2016	rBV4	950	675	0.05%	0.007%
38	7.640	2027	2037	2056	rBV	120132	207880	15.90%	2.083%
39	8.106	2171	2182	2206	rBV	297055	522187	39.95%	5.231%
40	8.318	2246	2248	2251	rBV4	2442	1374	0.11%	0.014%
41	8.363	2258	2262	2263	rBV3	1208	804	0.06%	0.008%
42	8.476	2295	2297	2302	rVB5	1754	1495	0.11%	0.015%
43	8.502	2302	2305	2306	rBV2	1429	895	0.07%	0.009%
44	8.572	2323	2327	2332	rBV6	1112	1274	0.10%	0.013%
45	8.659	2352	2354	2358	rBV4	938	809	0.06%	0.008%
46	8.875	2409	2421	2442	rBV	643603	1037249	79.35%	10.391%
47	9.296	2548	2552	2556	rBV7	1376	1082	0.08%	0.011%
48	9.444	2596	2598	2602	rVB5	962	665	0.05%	0.007%
49	9.466	2602	2605	2609	rVB4	1499	925	0.07%	0.009%
50	9.492	2609	2613	2618	rBV8	1014	1008	0.08%	0.010%
51	9.588	2640	2643	2647	rVB5	1851	1376	0.11%	0.014%
52	9.653	2658	2663	2664	rBV3	1437	1025	0.08%	0.010%
53	9.759	2692	2696	2698	rBV4	1701	1138	0.09%	0.011%
54	9.830	2716	2718	2721	rBV4	1093	788	0.06%	0.008%
55	9.965	2757	2760	2762	rBV3	1574	857	0.07%	0.009%
56	10.000	2767	2771	2775	rVB7	1309	1037	0.08%	0.010%
57	10.042	2780	2784	2785	rBV3	1421	897	0.07%	0.009%
58	10.238	2833	2845	2860	rVV	366602	591688	45.26%	5.928%
59	10.376	2884	2888	2890	rVB3	1307	668	0.05%	0.007%
60	10.402	2894	2896	2899	rBV4	1300	659	0.05%	0.007%
61	10.482	2918	2921	2925	rVB4	2142	1446	0.11%	0.014%
62	10.627	2964	2966	2973	rVB6	1189	944	0.07%	0.009%
63	10.666	2976	2978	2983	rVB4	854	718	0.05%	0.007%
64	10.691	2983	2986	2991	rVB6	1527	1473	0.11%	0.015%
65	10.807	3019	3022	3025	rBV5	1209	922	0.07%	0.009%
66	10.836	3029	3031	3036	rVB4	1454	949	0.07%	0.010%
67	10.862	3036	3039	3042	rBV4	1686	1315	0.10%	0.013%
68	10.971	3069	3073	3076	rVB4	1630	1091	0.08%	0.011%
69	10.990	3076	3079	3083	rBV5	1007	813	0.06%	0.008%
70	11.270	3154	3166	3186	rBV	630438	950726	72.73%	9.524%
71	11.646	3271	3283	3301	rBV	628639	979287	74.91%	9.810%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017194.D
 Acq On : 26 Jun 2020 20:09
 Operator : SY/MD
 Sample : L3103-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.807	3330	3333	3337	rBV4	1211	1210	0.09%	0.012%
73	11.926	3367	3370	3373	rBV4	863	667	0.05%	0.007%
74	12.103	3421	3425	3428	rVB6	1129	877	0.07%	0.009%
75	12.363	3502	3506	3509	rBV4	1314	1641	0.13%	0.016%
76	12.569	3567	3570	3571	rBV3	1279	717	0.05%	0.007%
77	12.765	3629	3631	3635	rBV4	893	679	0.05%	0.007%
78	12.890	3667	3670	3672	rBV3	1284	716	0.05%	0.007%
79	12.987	3696	3700	3701	rBV3	1090	914	0.07%	0.009%
80	13.058	3719	3722	3728	rVB5	1276	1302	0.10%	0.013%
81	13.141	3744	3748	3751	rBV5	1182	1064	0.08%	0.011%
82	13.177	3756	3759	3761	rBV3	1500	1024	0.08%	0.010%
83	13.228	3772	3775	3778	rBV4	1186	994	0.08%	0.010%
84	13.305	3794	3799	3802	rBV6	1415	1211	0.09%	0.012%
85	13.476	3849	3852	3856	rBV6	1140	920	0.07%	0.009%
86	13.878	3973	3977	3978	rBV3	1196	787	0.06%	0.008%
87	13.900	3982	3984	3987	rBV4	1607	882	0.07%	0.009%
88	13.964	4000	4004	4005	rBV2	1369	873	0.07%	0.009%
89	14.241	4088	4090	4093	rBV3	991	784	0.06%	0.008%
90	14.305	4104	4110	4113	rBV5	1267	1516	0.12%	0.015%
91	14.482	4161	4165	4166	rBV4	1451	1185	0.09%	0.012%
92	14.595	4195	4200	4203	rBV5	2046	1582	0.12%	0.016%
93	14.739	4241	4245	4246	rBV3	1626	1178	0.09%	0.012%
94	14.784	4254	4259	4262	rBV5	1507	1129	0.09%	0.011%
95	14.800	4262	4264	4267	rBV4	1732	1058	0.08%	0.011%
96	14.839	4273	4276	4278	rBV3	1243	801	0.06%	0.008%
97	15.032	4334	4336	4340	rBV4	1072	683	0.05%	0.007%
98	15.054	4340	4343	4348	rVB6	1540	1259	0.10%	0.013%
99	15.083	4349	4352	4353	rBV3	1455	841	0.06%	0.008%
100	15.887	4599	4602	4611	rBV3	2459	2610	0.20%	0.026%


Sum of corrected areas: 9982056

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017194.D
Acq On : 26 Jun 2020 20:09
Operator : SY/MD
Sample : L3103-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q62

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

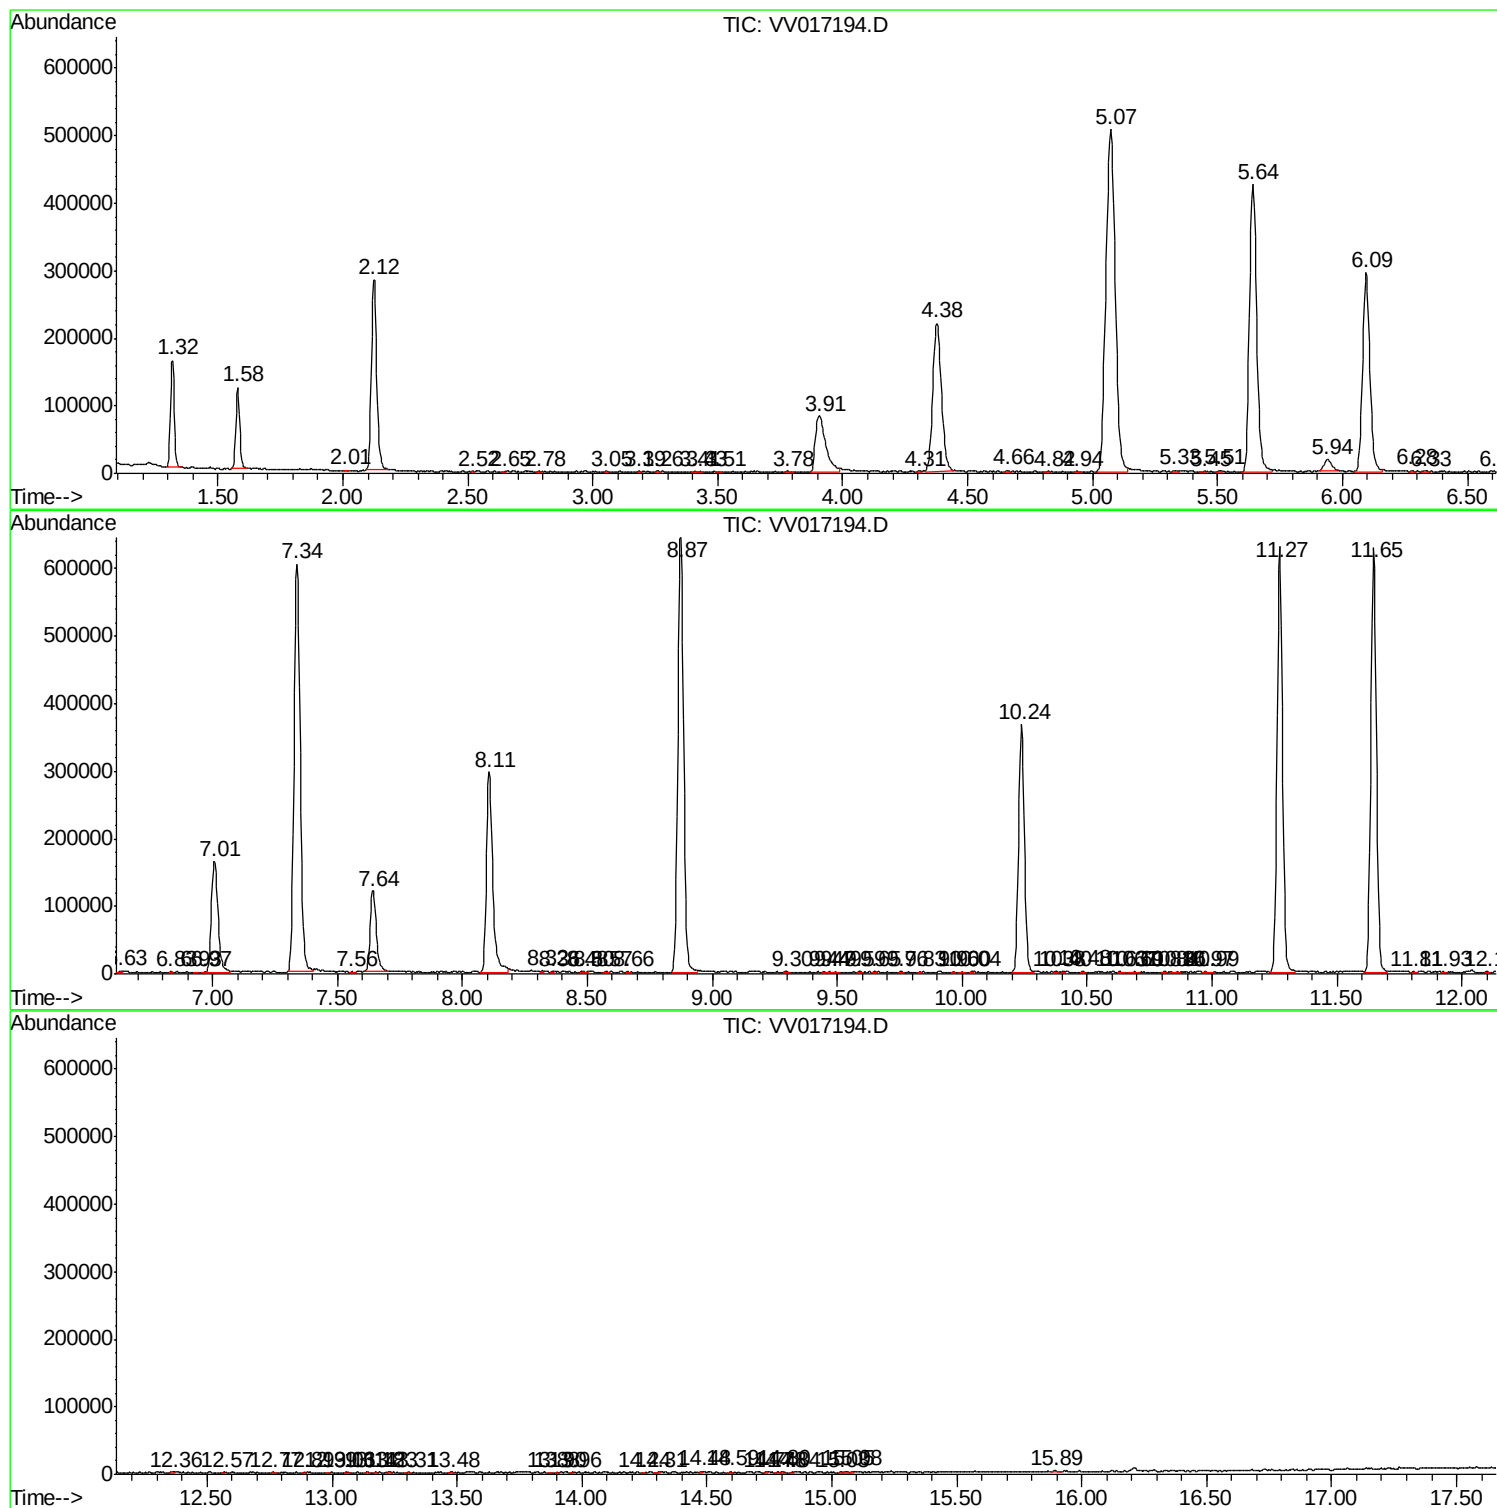

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017194.D
Acq On : 26 Jun 2020 20:09
Operator : SY/MD
Sample : L3103-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q62

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017194.D
Acq On : 26 Jun 2020 20:09
Operator : SY/MD
Sample : L3103-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q62

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc