

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017195.D
 Acq On : 26 Jun 2020 20:32
 Operator : SY/MD
 Sample : L3103-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	165723	174547	13.27%	1.750%
2	1.579	145	152	165	rVB	119615	131242	9.98%	1.316%
3	2.122	312	321	337	rBV	278381	423064	32.17%	4.242%
4	2.280	367	370	371	rBV3	1264	658	0.05%	0.007%
5	2.971	581	585	588	rBV4	837	775	0.06%	0.008%
6	3.161	642	644	646	rBV3	1117	652	0.05%	0.007%
7	3.418	721	724	727	rVB3	1137	740	0.06%	0.007%
8	3.447	730	733	737	rVB5	993	880	0.07%	0.009%
9	3.466	737	739	741	rBV2	1288	663	0.05%	0.007%
10	3.531	754	759	763	rBV8	1064	1098	0.08%	0.011%
11	3.711	810	815	816	rBV5	1021	884	0.07%	0.009%
12	3.907	865	876	902	rBV2	88310	247686	18.83%	2.483%
13	4.312	999	1002	1004	rBV3	1217	634	0.05%	0.006%
14	4.376	1009	1022	1046	rVB2	221510	532179	40.47%	5.336%
15	4.569	1079	1082	1084	rBV4	1046	893	0.07%	0.009%
16	4.910	1184	1188	1190	rVV4	993	795	0.06%	0.008%
17	5.071	1221	1238	1262	rBV2	509402	1315042	100.00%	13.185%
18	5.338	1319	1321	1324	rBV3	1612	884	0.07%	0.009%
19	5.640	1403	1415	1442	rBV	424844	852347	64.82%	8.546%
20	5.868	1484	1486	1490	rVB4	1344	714	0.05%	0.007%
21	5.891	1491	1493	1497	rBV4	1018	767	0.06%	0.008%
22	6.093	1544	1556	1575	rBV	290397	579386	44.06%	5.809%
23	6.334	1627	1631	1633	rBV4	1007	770	0.06%	0.008%
24	6.762	1762	1764	1766	rBV3	1387	783	0.06%	0.008%
25	6.955	1821	1824	1825	rBV3	1605	749	0.06%	0.008%
26	7.006	1831	1840	1861	rVB	162204	286412	21.78%	2.872%
27	7.273	1920	1923	1925	rBV3	871	668	0.05%	0.007%
28	7.338	1931	1943	1962	rBV	613063	1049498	79.81%	10.523%
29	7.640	2027	2037	2058	rBV	118393	208178	15.83%	2.087%
30	7.813	2089	2091	2096	rBV5	1012	734	0.06%	0.007%
31	7.961	2135	2137	2142	rVB4	2122	1411	0.11%	0.014%
32	7.987	2142	2145	2147	rBV3	1955	1375	0.10%	0.014%
33	8.019	2152	2155	2158	rBV4	1149	938	0.07%	0.009%
34	8.039	2158	2161	2163	rBV3	1169	784	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017195.D
 Acq On : 26 Jun 2020 20:32
 Operator : SY/MD
 Sample : L3103-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.106	2172	2182	2213	rBV	309461	543491	41.33%	5.449%
36	8.569	2324	2326	2328	rBV3	1256	799	0.06%	0.008%
37	8.698	2361	2366	2369	rBV5	1702	1708	0.13%	0.017%
38	8.720	2369	2373	2375	rVB4	1056	765	0.06%	0.008%
39	8.871	2408	2420	2439	rBV	638543	1034868	78.69%	10.376%
40	9.080	2481	2485	2487	rBV3	1476	1197	0.09%	0.012%
41	9.125	2496	2499	2501	rBV4	1325	792	0.06%	0.008%
42	9.154	2505	2508	2510	rBV5	1578	1044	0.08%	0.010%
43	9.222	2524	2529	2532	rBV6	1658	1355	0.10%	0.014%
44	9.241	2532	2535	2539	rVV6	1700	1134	0.09%	0.011%
45	9.376	2573	2577	2580	rBV3	1580	1176	0.09%	0.012%
46	9.424	2587	2592	2595	rBV6	1399	1260	0.10%	0.013%
47	9.608	2647	2649	2652	rBV4	1279	823	0.06%	0.008%
48	9.723	2683	2685	2688	rBV4	1275	855	0.07%	0.009%
49	9.829	2713	2718	2720	rBV3	1656	1787	0.14%	0.018%
50	10.029	2776	2780	2781	rBV2	1589	906	0.07%	0.009%
51	10.071	2789	2793	2795	rVV4	967	734	0.06%	0.007%
52	10.090	2797	2799	2804	rVB4	1351	1068	0.08%	0.011%
53	10.138	2812	2814	2818	rBV3	1093	795	0.06%	0.008%
54	10.164	2820	2822	2826	rBV3	961	753	0.06%	0.008%
55	10.238	2832	2845	2865	rVB	386230	600513	45.66%	6.021%
56	10.489	2920	2923	2924	rBV3	1604	874	0.07%	0.009%
57	10.598	2954	2957	2960	rBV5	2219	1762	0.13%	0.018%
58	10.630	2964	2967	2970	rBV4	1505	1132	0.09%	0.011%
59	10.752	3002	3005	3007	rBV4	1263	814	0.06%	0.008%
60	10.791	3014	3017	3019	rBV3	1275	812	0.06%	0.008%
61	10.919	3049	3057	3059	rBV7	1102	1217	0.09%	0.012%
62	11.006	3079	3084	3086	rBV4	1730	1101	0.08%	0.011%
63	11.100	3111	3113	3116	rVB3	1289	699	0.05%	0.007%
64	11.209	3146	3147	3150	rBV3	1178	772	0.06%	0.008%
65	11.270	3155	3166	3187	rVV	622177	947120	72.02%	9.496%
66	11.379	3197	3200	3202	rBV3	1496	944	0.07%	0.009%
67	11.460	3221	3225	3227	rBV3	2117	1556	0.12%	0.016%
68	11.646	3272	3283	3301	rVB	631858	969175	73.70%	9.718%
69	11.823	3336	3338	3339	rBV3	1695	747	0.06%	0.007%
70	12.035	3401	3404	3406	rBV3	1385	934	0.07%	0.009%
71	12.157	3439	3442	3445	rVB3	990	627	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017195.D
 Acq On : 26 Jun 2020 20:32
 Operator : SY/MD
 Sample : L3103-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.180	3445	3449	3451	rBV4	1184	1079	0.08%	0.011%
73	12.331	3492	3496	3497	rBV3	1485	877	0.07%	0.009%
74	12.572	3566	3571	3574	rBV7	1882	2020	0.15%	0.020%
75	12.862	3658	3661	3664	rVB3	1021	638	0.05%	0.006%
76	12.881	3664	3667	3668	rBV3	1818	826	0.06%	0.008%
77	13.051	3718	3720	3726	rVB6	1014	901	0.07%	0.009%
78	13.141	3745	3748	3751	rBV4	1101	654	0.05%	0.007%
79	13.170	3753	3757	3759	rBV4	888	612	0.05%	0.006%
80	13.225	3770	3774	3777	rBV4	870	793	0.06%	0.008%
81	13.501	3857	3860	3866	rBV7	1493	1574	0.12%	0.016%
82	13.566	3878	3880	3882	rBV3	1412	659	0.05%	0.007%
83	13.685	3915	3917	3919	rBV3	897	601	0.05%	0.006%
84	13.775	3941	3945	3949	rBV7	1813	2055	0.16%	0.021%
85	13.816	3955	3958	3960	rBV3	1175	760	0.06%	0.008%
86	14.051	4028	4031	4037	rVB5	1381	1172	0.09%	0.012%
87	14.263	4094	4097	4099	rBV3	1425	809	0.06%	0.008%
88	14.296	4104	4107	4111	rVB5	1371	1069	0.08%	0.011%
89	14.353	4122	4125	4126	rBV	1300	697	0.05%	0.007%
90	14.710	4234	4236	4240	rBV3	1098	631	0.05%	0.006%
91	14.810	4265	4267	4270	rBV3	1012	731	0.06%	0.007%
92	14.884	4288	4290	4293	rBV4	1403	802	0.06%	0.008%
93	14.987	4321	4322	4325	rVV2	1209	599	0.05%	0.006%
94	15.016	4329	4331	4334	rBV3	1304	759	0.06%	0.008%
95	15.051	4339	4342	4343	rBV3	1380	709	0.05%	0.007%
96	15.090	4351	4354	4359	rVB5	2013	1150	0.09%	0.012%
97	15.115	4359	4362	4363	rBV2	1375	890	0.07%	0.009%
98	15.353	4434	4436	4439	rBV3	1252	788	0.06%	0.008%
99	15.485	4475	4477	4480	rBV4	1539	990	0.08%	0.010%
100	15.640	4523	4525	4528	rBV3	1440	635	0.05%	0.006%


Sum of corrected areas: 9973419

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017195.D
Acq On : 26 Jun 2020 20:32
Operator : SY/MD
Sample : L3103-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

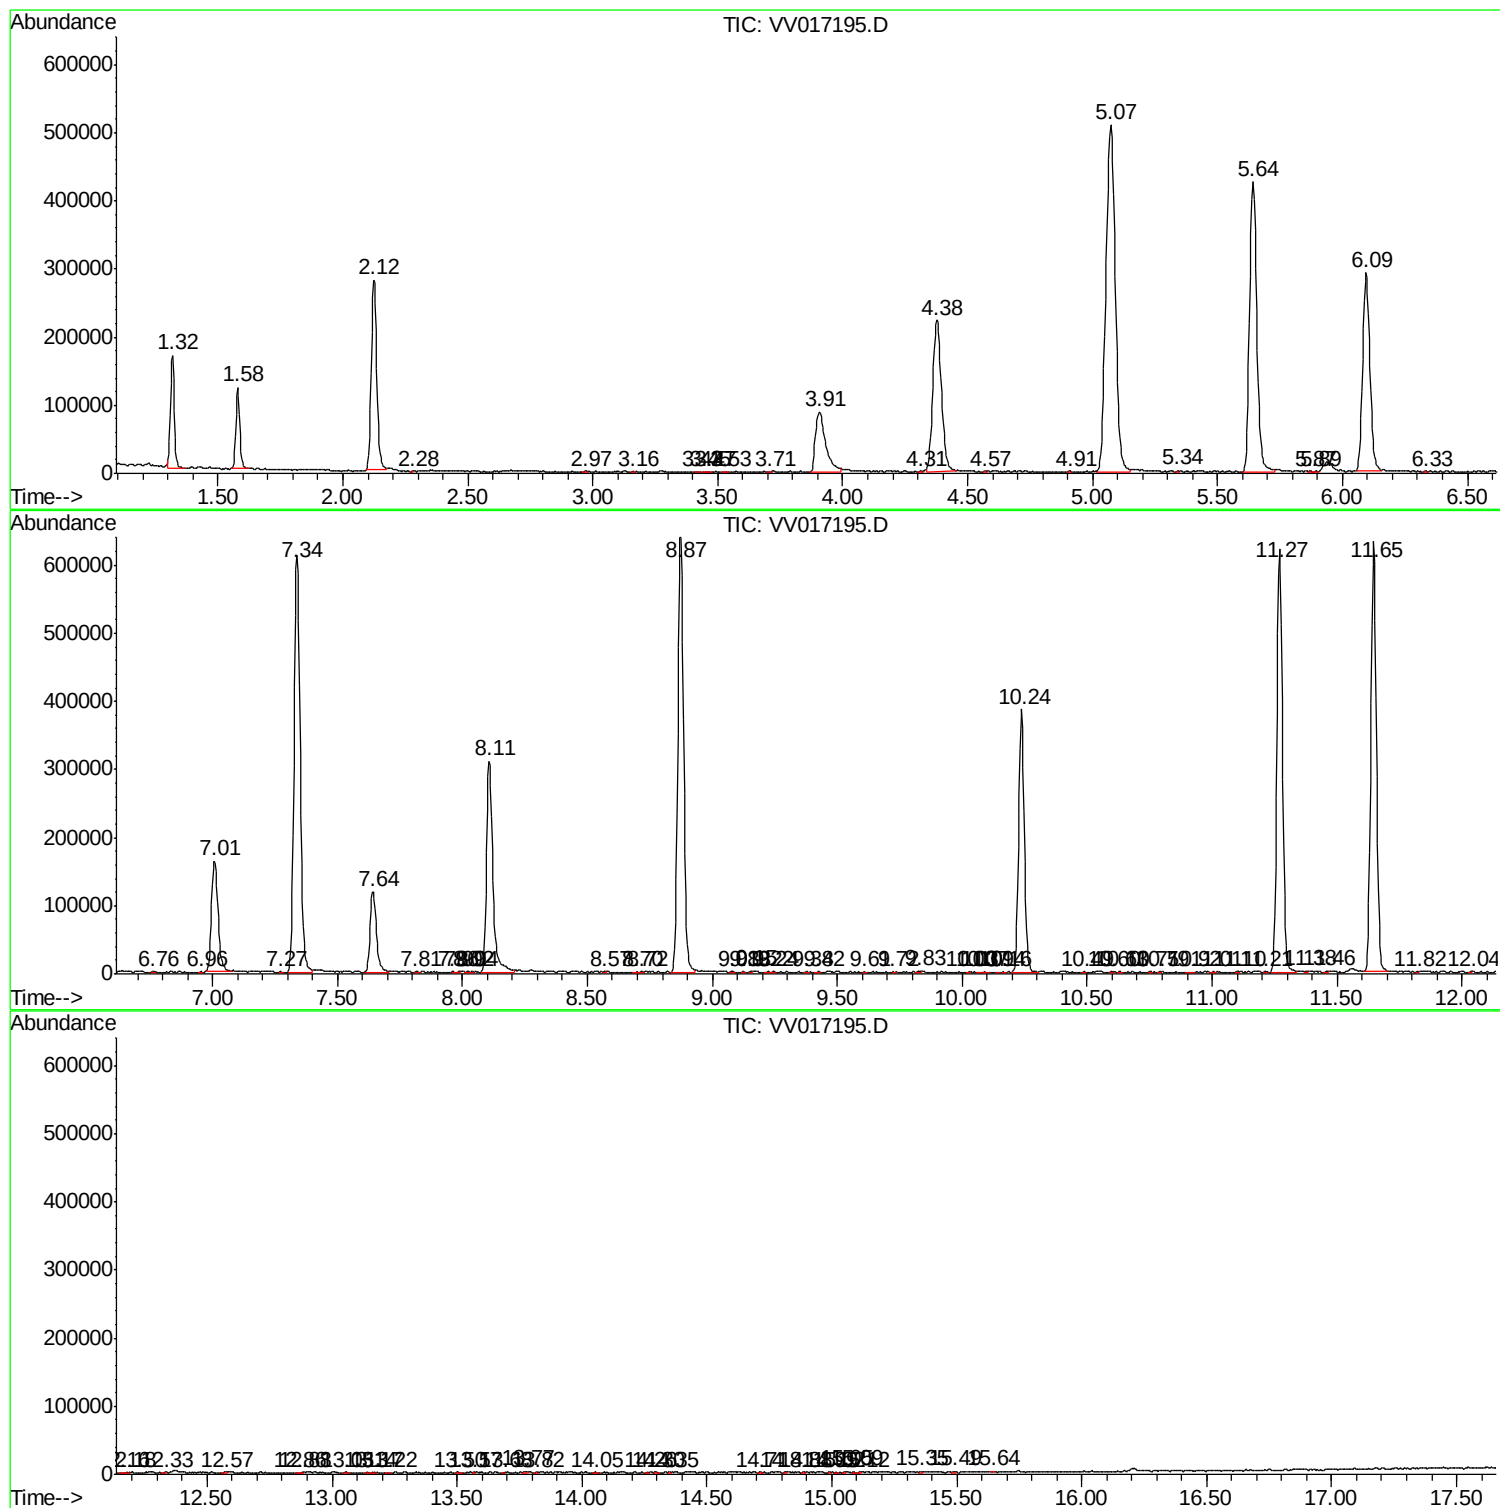

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017195.D
Acq On : 26 Jun 2020 20:32
Operator : SY/MD
Sample : L3103-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017195.D
Acq On : 26 Jun 2020 20:32
Operator : SY/MD
Sample : L3103-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q63

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc