

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017198.D
 Acq On : 26 Jun 2020 21:42
 Operator : SY/MD
 Sample : L3103-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	156432	164630	12.49%	1.638%
2	1.579	145	152	161	rVB	120657	134698	10.22%	1.340%
3	2.123	311	321	340	rBV	281015	425971	32.33%	4.238%
4	2.293	372	374	378	rBV4	1351	1071	0.08%	0.011%
5	2.611	470	473	474	rBV3	1623	850	0.06%	0.008%
6	2.740	511	513	516	rVB3	1247	606	0.05%	0.006%
7	2.762	516	520	521	rBV3	917	650	0.05%	0.006%
8	2.901	560	563	567	rBV5	1682	1480	0.11%	0.015%
9	3.061	610	613	615	rBV2	1294	637	0.05%	0.006%
10	3.216	658	661	663	rBV3	1371	863	0.07%	0.009%
11	3.322	691	694	697	rBV4	1060	811	0.06%	0.008%
12	3.396	712	717	720	rBV8	1242	1260	0.10%	0.013%
13	3.470	736	740	741	rBV3	1606	717	0.05%	0.007%
14	3.653	792	797	799	rVB3	1227	903	0.07%	0.009%
15	3.856	854	860	862	rBV8	1678	1284	0.10%	0.013%
16	3.910	866	877	911	rVV	89237	289058	21.94%	2.876%
17	4.180	959	961	962	rBV2	1148	603	0.05%	0.006%
18	4.377	1009	1022	1045	rVB	213138	521225	39.55%	5.186%
19	4.631	1098	1101	1103	rBV3	943	601	0.05%	0.006%
20	4.669	1109	1113	1116	rBV4	1168	743	0.06%	0.007%
21	4.975	1203	1208	1211	rBV6	1337	1161	0.09%	0.012%
22	5.071	1217	1238	1270	rBV3	509422	1317759	100.00%	13.111%
23	5.309	1308	1312	1317	rBV7	1669	2232	0.17%	0.022%
24	5.422	1345	1347	1350	rBV3	1672	1138	0.09%	0.011%
25	5.479	1363	1365	1367	rBV2	1256	769	0.06%	0.008%
26	5.640	1403	1415	1440	rBV	421479	832351	63.16%	8.281%
27	5.939	1498	1508	1525	rVB4	59887	119574	9.07%	1.190%
28	6.093	1542	1556	1575	rBV2	289997	588635	44.67%	5.857%
29	6.409	1652	1654	1658	rBV4	886	641	0.05%	0.006%
30	6.483	1674	1677	1679	rBV3	1311	775	0.06%	0.008%
31	6.531	1689	1692	1696	rBV5	1467	1227	0.09%	0.012%
32	6.704	1744	1746	1749	rBV4	1168	617	0.05%	0.006%
33	6.762	1759	1764	1768	rBV7	1819	1907	0.14%	0.019%
34	6.897	1805	1806	1811	rVB3	1643	1221	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017198.D
 Acq On : 26 Jun 2020 21:42
 Operator : SY/MD
 Sample : L3103-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.923	1811	1814	1816	rBV2	1201	861	0.07%	0.009%
36	7.007	1829	1840	1859	rBV2	161225	289847	22.00%	2.884%
37	7.122	1874	1876	1879	rVB4	1459	620	0.05%	0.006%
38	7.338	1930	1943	1961	rBV	602594	1027160	77.95%	10.220%
39	7.592	2019	2022	2026	rBV6	1397	1160	0.09%	0.012%
40	7.640	2028	2037	2053	rVV2	116447	197242	14.97%	1.962%
41	7.949	2129	2133	2137	rBV5	2173	2483	0.19%	0.025%
42	8.032	2155	2159	2161	rBV5	1138	852	0.06%	0.008%
43	8.106	2172	2182	2216	rBV	305699	548684	41.64%	5.459%
44	8.499	2300	2304	2305	rBV2	744	621	0.05%	0.006%
45	8.518	2307	2310	2313	rVB4	1081	621	0.05%	0.006%
46	8.563	2321	2324	2326	rBV3	1419	916	0.07%	0.009%
47	8.691	2363	2364	2368	rVB3	1110	624	0.05%	0.006%
48	8.743	2377	2380	2383	rBV4	1534	971	0.07%	0.010%
49	8.872	2409	2420	2438	rBV	629128	1013627	76.92%	10.085%
50	9.068	2478	2481	2486	rBV6	1752	1663	0.13%	0.017%
51	9.592	2641	2644	2647	rBV4	943	679	0.05%	0.007%
52	9.698	2673	2677	2681	rBV6	1566	1170	0.09%	0.012%
53	9.833	2716	2719	2723	rBV5	1384	1061	0.08%	0.011%
54	9.955	2753	2757	2761	rVB7	1112	909	0.07%	0.009%
55	10.158	2817	2820	2822	rBV3	1105	723	0.05%	0.007%
56	10.187	2827	2829	2830	rVV2	1676	693	0.05%	0.007%
57	10.238	2833	2845	2863	rVV	375610	591735	44.90%	5.887%
58	10.386	2888	2891	2892	rBV3	1367	889	0.07%	0.009%
59	10.470	2914	2917	2919	rBV3	910	673	0.05%	0.007%
60	10.797	3015	3019	3023	rBV7	1921	1643	0.12%	0.016%
61	10.826	3026	3028	3033	rBV3	709	711	0.05%	0.007%
62	10.897	3047	3050	3051	rBV2	916	635	0.05%	0.006%
63	11.026	3087	3090	3093	rBV2	1195	797	0.06%	0.008%
64	11.061	3098	3101	3103	rBV3	1051	817	0.06%	0.008%
65	11.122	3117	3120	3122	rBV3	2007	1060	0.08%	0.011%
66	11.270	3153	3166	3181	rBV	615196	939652	71.31%	9.349%
67	11.515	3239	3242	3244	rVB3	1984	1150	0.09%	0.011%
68	11.534	3244	3248	3249	rBV3	1703	1058	0.08%	0.011%
69	11.646	3272	3283	3303	rVB	619605	968384	73.49%	9.635%
70	11.781	3323	3325	3327	rVB3	1552	616	0.05%	0.006%
71	11.936	3369	3373	3375	rBV4	818	629	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017198.D
 Acq On : 26 Jun 2020 21:42
 Operator : SY/MD
 Sample : L3103-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.000	3390	3393	3396	rBV3	822	651	0.05%	0.006%
73	12.016	3396	3398	3401	rBV4	1431	833	0.06%	0.008%
74	12.164	3442	3444	3447	rBV3	1128	617	0.05%	0.006%
75	12.180	3447	3449	3454	rVB5	1374	784	0.06%	0.008%
76	12.373	3506	3509	3510	rBV3	1222	615	0.05%	0.006%
77	12.412	3517	3521	3525	rBV6	1390	1439	0.11%	0.014%
78	12.463	3532	3537	3541	rVB7	1809	2012	0.15%	0.020%
79	12.486	3541	3544	3546	rBV4	1190	810	0.06%	0.008%
80	12.553	3561	3565	3569	rVB7	2055	1804	0.14%	0.018%
81	12.579	3569	3573	3575	rBV3	1295	1019	0.08%	0.010%
82	13.064	3721	3724	3727	rBV3	1250	697	0.05%	0.007%
83	13.096	3732	3734	3737	rBV3	1254	883	0.07%	0.009%
84	13.135	3742	3746	3753	rBV8	1279	1331	0.10%	0.013%
85	13.186	3760	3762	3764	rBV3	1450	776	0.06%	0.008%
86	13.222	3771	3773	3778	rBV4	1043	937	0.07%	0.009%
87	13.476	3849	3852	3855	rBV4	1068	682	0.05%	0.007%
88	13.543	3871	3873	3877	rBV4	1128	910	0.07%	0.009%
89	13.900	3980	3984	3985	rBV4	978	672	0.05%	0.007%
90	13.987	4007	4011	4014	rBV5	1370	1254	0.10%	0.012%
91	14.022	4018	4022	4023	rBV3	1063	689	0.05%	0.007%
92	14.106	4045	4048	4051	rBV4	1133	841	0.06%	0.008%
93	14.122	4051	4053	4056	rVV3	1539	915	0.07%	0.009%
94	14.148	4056	4061	4063	rVB4	1350	990	0.08%	0.010%
95	14.350	4122	4124	4127	rBV4	1213	811	0.06%	0.008%
96	14.482	4163	4165	4168	rVB2	1718	632	0.05%	0.006%
97	14.694	4226	4231	4235	rBV7	1967	1752	0.13%	0.017%
98	14.817	4267	4269	4273	rBV4	1758	1299	0.10%	0.013%
99	14.942	4306	4308	4312	rBV4	1432	1032	0.08%	0.010%
100	15.440	4459	4463	4464	rBV3	1359	951	0.07%	0.009%


Sum of corrected areas: 10050942

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017198.D
Acq On : 26 Jun 2020 21:42
Operator : SY/MD
Sample : L3103-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

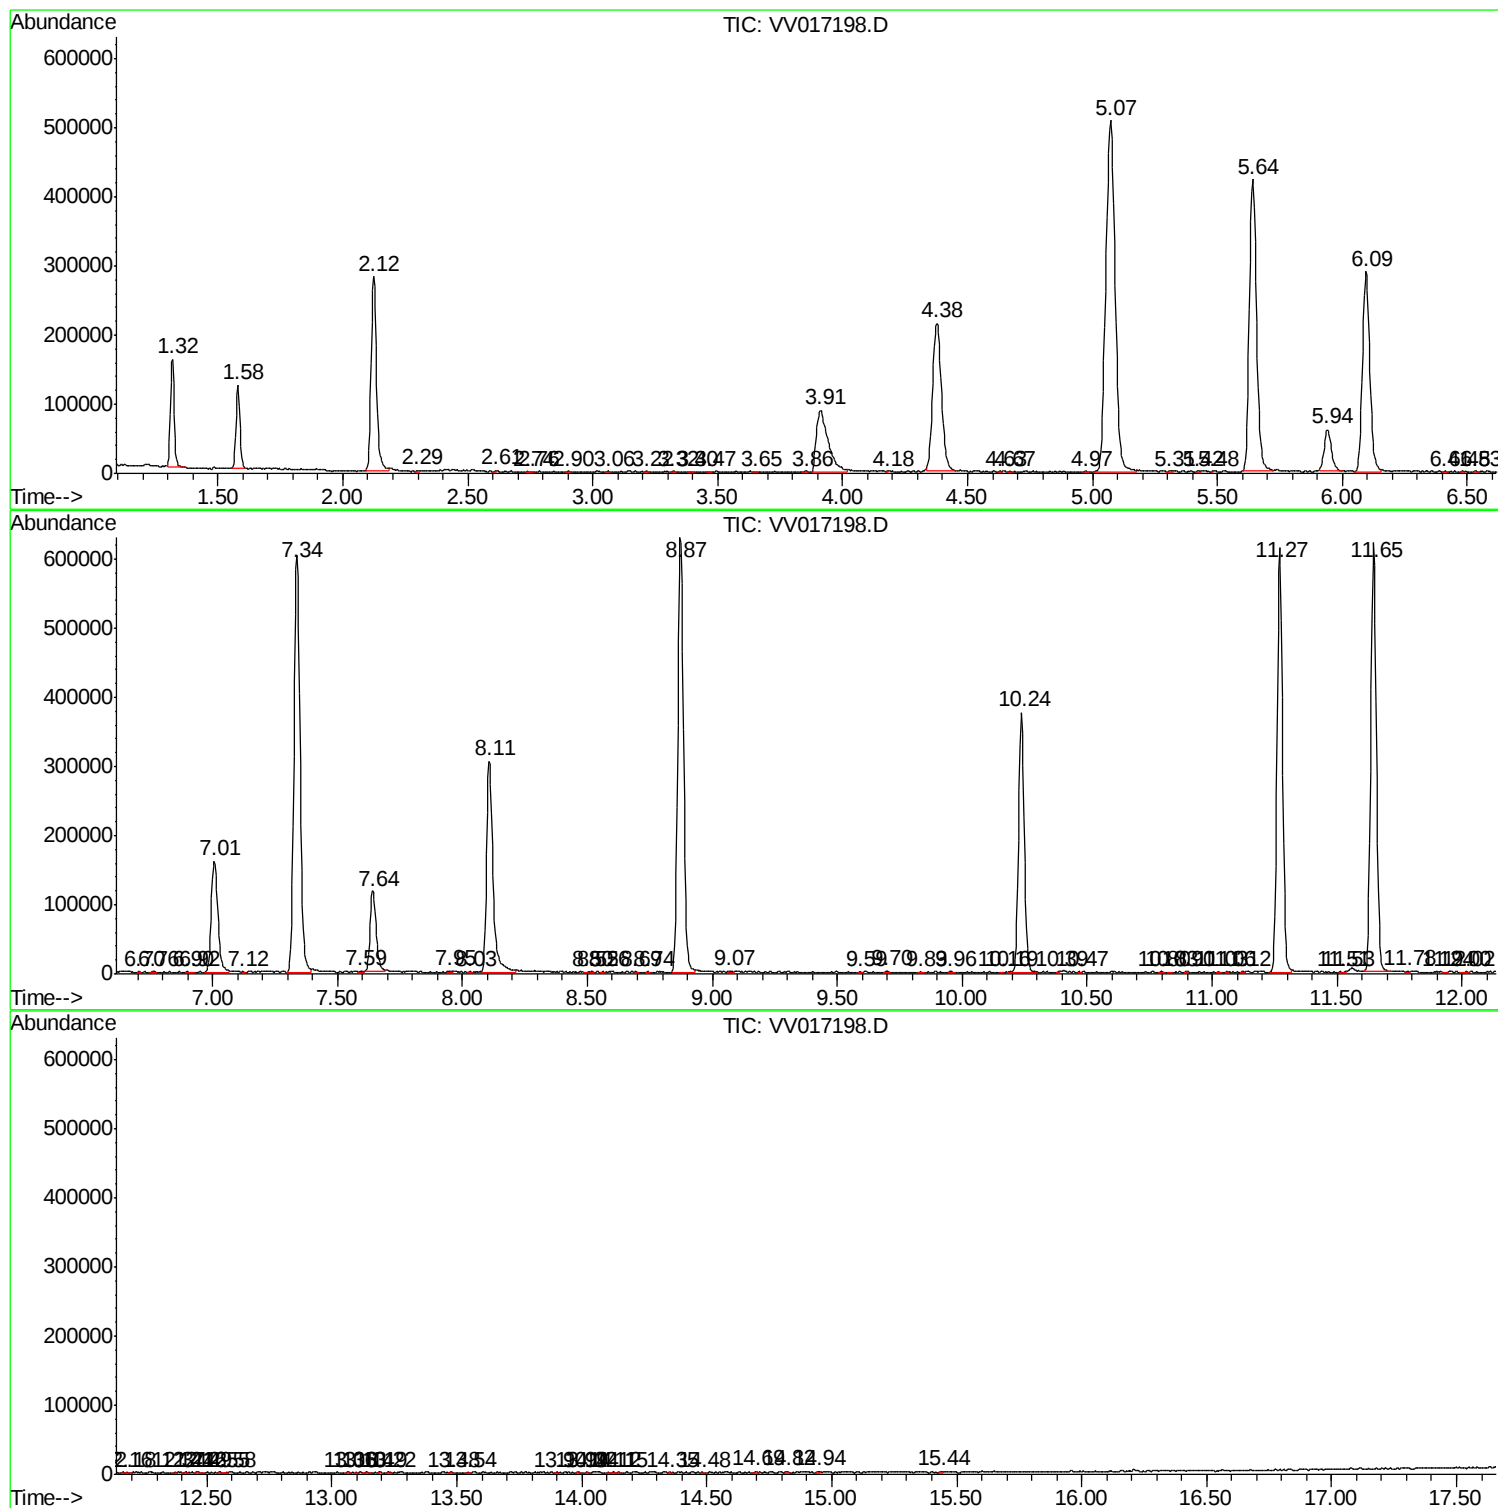

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017198.D
Acq On : 26 Jun 2020 21:42
Operator : SY/MD
Sample : L3103-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q74

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017198.D
Acq On : 26 Jun 2020 21:42
Operator : SY/MD
Sample : L3103-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q74

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
