

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017202.D
 Acq On : 27 Jun 2020 00:24
 Operator : SY/MD
 Sample : L3118-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	84	rVB	163886	169995	13.09%	1.692%
2	1.579	145	152	165	rVB	116725	128934	9.93%	1.283%
3	2.122	312	321	338	rBV	277376	415310	31.97%	4.133%
4	2.730	506	510	519	rVB10	1731	1982	0.15%	0.020%
5	2.788	526	528	531	rBV3	1255	785	0.06%	0.008%
6	2.891	557	560	562	rBV2	1187	809	0.06%	0.008%
7	2.933	569	573	575	rBV4	961	753	0.06%	0.007%
8	3.074	606	617	620	rBV9	1547	2142	0.16%	0.021%
9	3.187	649	652	657	rVV6	1437	1419	0.11%	0.014%
10	3.364	702	707	709	rVB5	1102	925	0.07%	0.009%
11	3.489	740	746	748	rBV4	884	907	0.07%	0.009%
12	3.640	789	793	796	rBV6	1178	810	0.06%	0.008%
13	3.743	823	825	828	rVB3	1719	1019	0.08%	0.010%
14	3.846	853	857	859	rBV3	1170	905	0.07%	0.009%
15	3.907	865	876	901	rBV	88637	250611	19.29%	2.494%
16	4.232	976	977	980	rVB3	1562	668	0.05%	0.007%
17	4.376	1007	1022	1045	rBV	218697	536698	41.32%	5.341%
18	4.547	1074	1075	1079	rVB3	1875	871	0.07%	0.009%
19	4.572	1079	1083	1088	rBV6	1778	2196	0.17%	0.022%
20	4.759	1139	1141	1151	rVB6	2111	1859	0.14%	0.018%
21	4.875	1174	1177	1178	rBV3	1536	996	0.08%	0.010%
22	4.945	1197	1199	1203	rVB3	1486	800	0.06%	0.008%
23	4.978	1207	1209	1213	rVB4	1296	866	0.07%	0.009%
24	5.000	1213	1216	1218	rBV3	1190	786	0.06%	0.008%
25	5.074	1221	1239	1263	rBV2	505696	1298874	100.00%	12.926%
26	5.563	1389	1391	1393	rBV2	1238	598	0.05%	0.006%
27	5.640	1403	1415	1443	rBV	429194	862992	66.44%	8.588%
28	5.929	1496	1505	1515	rBV5	12347	23490	1.81%	0.234%
29	6.093	1543	1556	1578	rVV	291389	590553	45.47%	5.877%
30	6.508	1682	1685	1687	rBV3	1967	1411	0.11%	0.014%
31	6.730	1752	1754	1757	rVB3	1226	665	0.05%	0.007%
32	6.794	1772	1774	1776	rBV3	1344	694	0.05%	0.007%
33	6.830	1782	1785	1786	rBV3	1590	751	0.06%	0.007%
34	6.855	1790	1793	1796	rVV4	966	673	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017202.D
 Acq On : 27 Jun 2020 00:24
 Operator : SY/MD
 Sample : L3118-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.891	1801	1804	1808	rVV5	1303	817	0.06%	0.008%
36	6.929	1813	1816	1818	rBV4	1102	694	0.05%	0.007%
37	7.006	1828	1840	1859	rBV	158552	291323	22.43%	2.899%
38	7.338	1930	1943	1962	rBV	603561	1042387	80.25%	10.373%
39	7.643	2028	2038	2060	rBV	113696	198625	15.29%	1.977%
40	7.849	2099	2102	2105	rVB3	1252	677	0.05%	0.007%
41	7.945	2128	2132	2136	rBV7	1715	1686	0.13%	0.017%
42	8.039	2159	2161	2166	rVB6	1701	1123	0.09%	0.011%
43	8.106	2172	2182	2202	rBV	301189	550196	42.36%	5.475%
44	8.678	2358	2360	2366	rBV4	1637	1563	0.12%	0.016%
45	8.717	2369	2372	2374	rBV3	1761	939	0.07%	0.009%
46	8.772	2386	2389	2392	rVV3	1584	980	0.08%	0.010%
47	8.875	2408	2421	2444	rBV	640075	1053908	81.14%	10.488%
48	9.084	2482	2486	2488	rBV4	1545	1154	0.09%	0.011%
49	9.373	2571	2576	2578	rBV5	1761	1384	0.11%	0.014%
50	9.399	2578	2584	2589	rBV9	1324	1981	0.15%	0.020%
51	9.492	2610	2613	2615	rBV2	922	682	0.05%	0.007%
52	9.569	2635	2637	2641	rBV5	1041	673	0.05%	0.007%
53	9.768	2697	2699	2703	rVB4	1332	800	0.06%	0.008%
54	9.794	2703	2707	2710	rBV2	1367	1198	0.09%	0.012%
55	9.810	2710	2712	2716	rBV5	1508	871	0.07%	0.009%
56	9.913	2742	2744	2747	rVB3	1511	706	0.05%	0.007%
57	10.003	2770	2772	2775	rBV5	930	596	0.05%	0.006%
58	10.045	2778	2785	2787	rBV6	2886	3187	0.25%	0.032%
59	10.238	2833	2845	2861	rVV	374016	588507	45.31%	5.856%
60	10.321	2868	2871	2873	rBV3	1352	861	0.07%	0.009%
61	10.473	2916	2918	2922	rBV4	863	642	0.05%	0.006%
62	10.556	2940	2944	2948	rBV7	1456	1262	0.10%	0.013%
63	10.688	2982	2985	2990	rVB6	1367	901	0.07%	0.009%
64	10.743	2997	3002	3003	rBV4	1088	867	0.07%	0.009%
65	10.919	3055	3057	3061	rBV4	1102	899	0.07%	0.009%
66	11.016	3083	3087	3089	rBV4	1329	921	0.07%	0.009%
67	11.064	3099	3102	3104	rBV3	906	599	0.05%	0.006%
68	11.077	3104	3106	3109	rVV3	1509	632	0.05%	0.006%
69	11.183	3132	3139	3141	rBV4	2665	2686	0.21%	0.027%
70	11.270	3154	3166	3181	rBV	638714	965526	74.34%	9.608%
71	11.521	3240	3244	3246	rBV3	1519	983	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017202.D
 Acq On : 27 Jun 2020 00:24
 Operator : SY/MD
 Sample : L3118-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.556	3248	3255	3270	rVV3	7702	15822	1.22%	0.157%
73	11.646	3271	3283	3298	rVV	639874	977409	75.25%	9.727%
74	11.784	3320	3326	3328	rBV7	1901	1840	0.14%	0.018%
75	11.842	3340	3344	3346	rBV4	1447	1107	0.09%	0.011%
76	12.196	3451	3454	3458	rBV4	1067	805	0.06%	0.008%
77	12.257	3471	3473	3477	rBV5	1529	1034	0.08%	0.010%
78	12.360	3499	3505	3506	rBV5	2201	1920	0.15%	0.019%
79	12.611	3579	3583	3586	rBV5	975	921	0.07%	0.009%
80	12.784	3633	3637	3640	rBV5	1349	1263	0.10%	0.013%
81	12.810	3642	3645	3647	rVV3	1634	794	0.06%	0.008%
82	12.900	3671	3673	3676	rBV5	1241	891	0.07%	0.009%
83	12.942	3682	3686	3687	rBV3	1031	687	0.05%	0.007%
84	12.958	3687	3691	3695	rVV5	1347	1061	0.08%	0.011%
85	13.051	3714	3720	3724	rBV7	1932	2394	0.18%	0.024%
86	13.135	3742	3746	3748	rBV2	1133	985	0.08%	0.010%
87	13.421	3829	3835	3838	rBV6	1420	1625	0.13%	0.016%
88	13.579	3881	3884	3891	rBV6	1104	1004	0.08%	0.010%
89	13.643	3901	3904	3906	rBV3	1519	869	0.07%	0.009%
90	13.733	3929	3932	3934	rBV3	1107	750	0.06%	0.007%
91	13.845	3964	3967	3970	rBV3	1081	816	0.06%	0.008%
92	14.161	4063	4065	4070	rBV6	955	867	0.07%	0.009%
93	14.488	4164	4167	4169	rBV3	1339	751	0.06%	0.007%
94	14.614	4203	4206	4209	rBV5	996	704	0.05%	0.007%
95	14.633	4209	4212	4214	rBV3	971	702	0.05%	0.007%
96	14.897	4289	4294	4295	rBV4	1309	1011	0.08%	0.010%
97	14.919	4299	4301	4305	rBV4	1230	874	0.07%	0.009%
98	14.968	4314	4316	4319	rVB3	1333	729	0.06%	0.007%
99	14.990	4319	4323	4324	rBV3	1117	839	0.06%	0.008%
100	15.096	4353	4356	4358	rBV4	1929	1239	0.10%	0.012%


Sum of corrected areas: 10048896

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017202.D
Acq On : 27 Jun 2020 00:24
Operator : SY/MD
Sample : L3118-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0F81

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

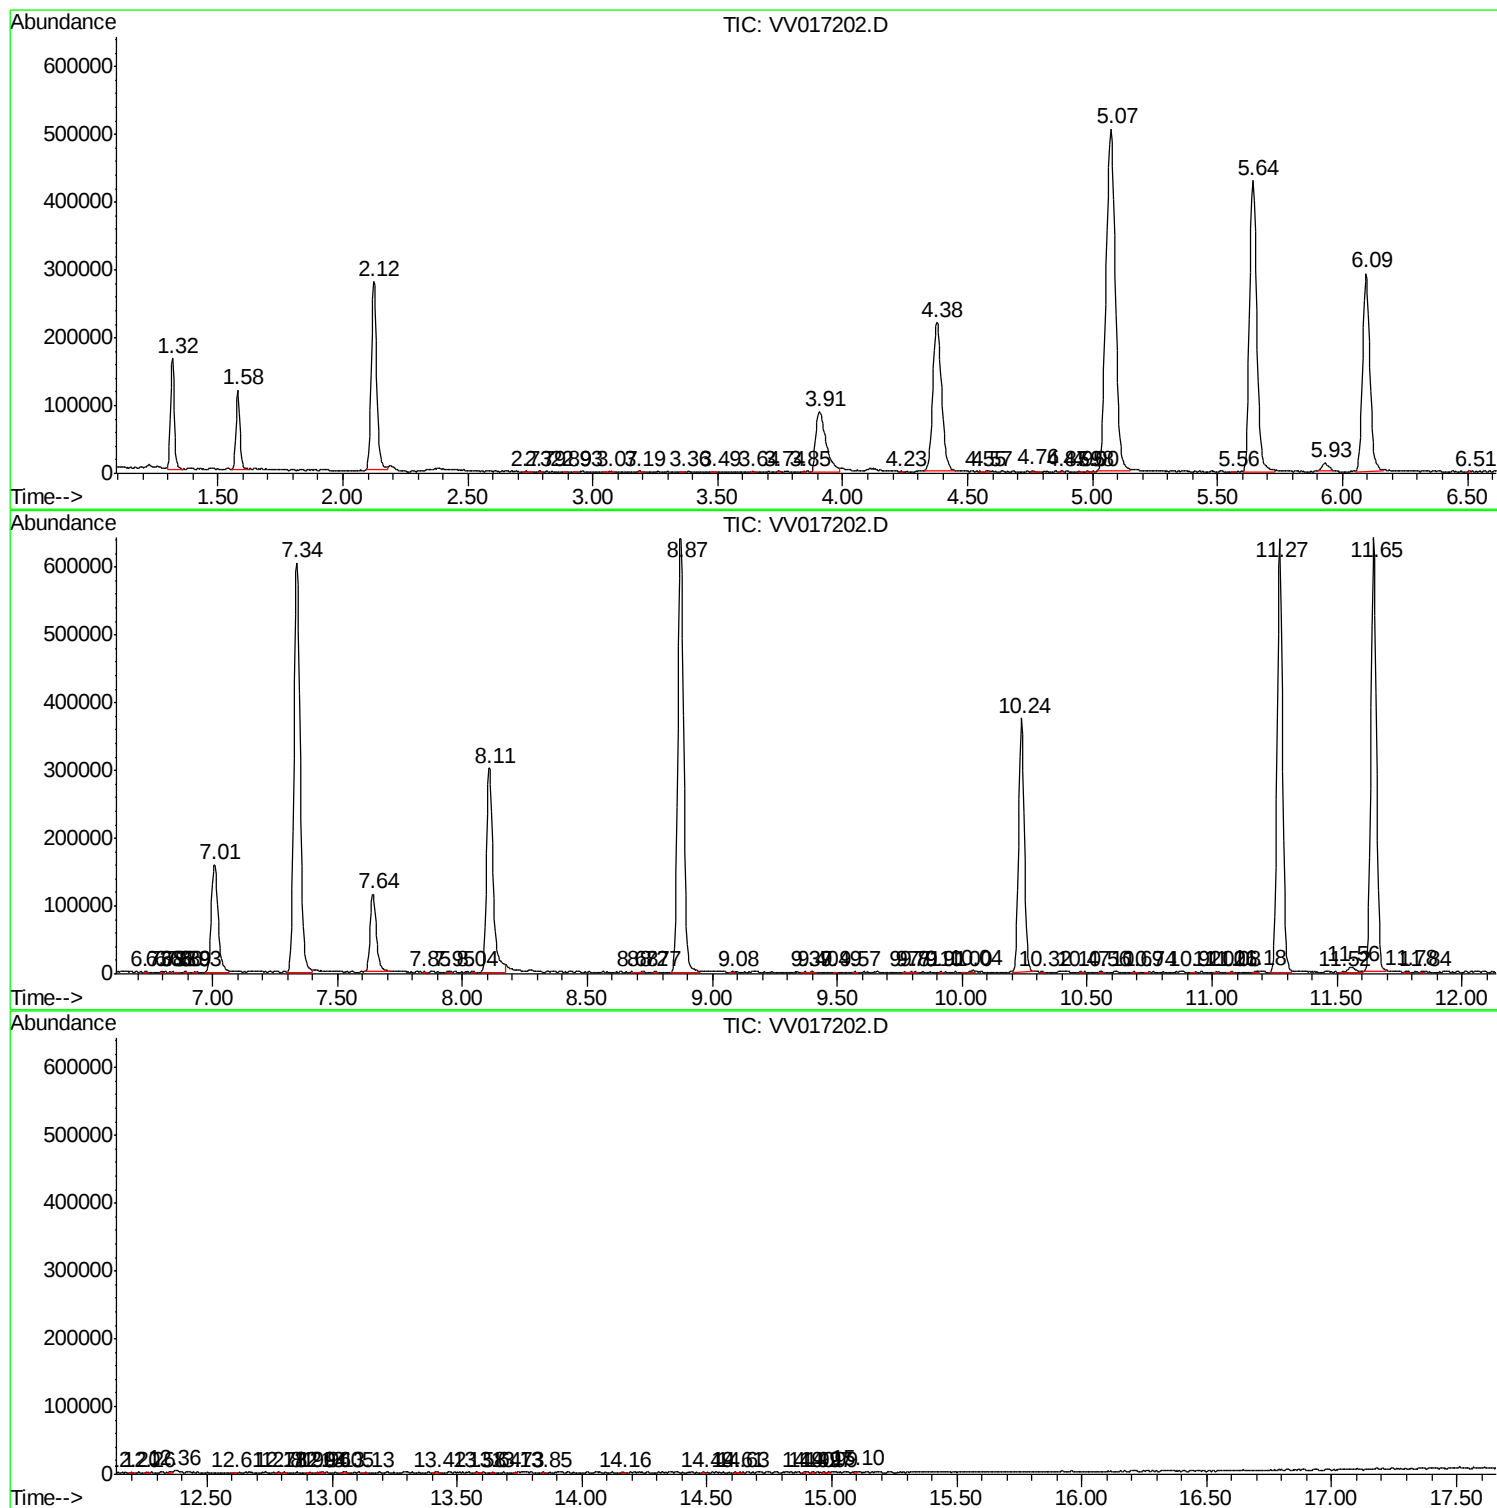

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017202.D
Acq On : 27 Jun 2020 00:24
Operator : SY/MD
Sample : L3118-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F81

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017202.D
Acq On : 27 Jun 2020 00:24
Operator : SY/MD
Sample : L3118-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F81

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc