

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017203.D
 Acq On : 27 Jun 2020 00:47
 Operator : SY/MD
 Sample : L3133-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	80	rVB	157166	159628	12.40%	1.622%
2	1.579	146	152	162	rVB	114745	125502	9.75%	1.276%
3	2.068	300	304	307	rBV4	1224	1181	0.09%	0.012%
4	2.123	310	321	341	rBV	279730	428488	33.29%	4.355%
5	2.357	390	394	396	rBV4	1410	993	0.08%	0.010%
6	2.447	416	422	428	rBV9	1932	2541	0.20%	0.026%
7	2.759	517	519	523	rBV3	1065	812	0.06%	0.008%
8	2.846	542	546	548	rBV5	1582	1083	0.08%	0.011%
9	2.987	588	590	594	rVB3	1401	755	0.06%	0.008%
10	3.032	601	604	606	rBV4	1171	648	0.05%	0.007%
11	3.065	611	614	616	rBV4	1299	763	0.06%	0.008%
12	3.161	641	644	648	rVV3	919	886	0.07%	0.009%
13	3.254	667	673	676	rVB6	1364	1604	0.12%	0.016%
14	3.393	714	716	718	rBV2	1170	673	0.05%	0.007%
15	3.463	733	738	739	rBV3	1311	878	0.07%	0.009%
16	3.553	763	766	769	rBV5	1634	980	0.08%	0.010%
17	3.753	824	828	831	rBV5	1086	1074	0.08%	0.011%
18	3.904	865	875	904	rVV2	88207	245556	19.08%	2.496%
19	4.206	967	969	972	rBV2	996	669	0.05%	0.007%
20	4.376	1003	1022	1045	rBV	228496	564833	43.88%	5.741%
21	4.624	1097	1099	1103	rBV3	1136	657	0.05%	0.007%
22	4.775	1144	1146	1152	rVV7	1737	1210	0.09%	0.012%
23	4.817	1156	1159	1161	rBV3	1408	668	0.05%	0.007%
24	5.071	1216	1238	1262	rBV2	499163	1287188	100.00%	13.082%
25	5.312	1311	1313	1318	rBV4	1249	934	0.07%	0.009%
26	5.470	1359	1362	1364	rBV3	1081	791	0.06%	0.008%
27	5.640	1400	1415	1435	rBV	422944	834898	64.86%	8.486%
28	5.884	1488	1491	1493	rBV4	1469	965	0.07%	0.010%
29	5.926	1497	1504	1520	rVB3	15954	34377	2.67%	0.349%
30	6.093	1543	1556	1577	rVV2	287818	581229	45.15%	5.907%
31	6.338	1628	1632	1634	rVB5	1361	1079	0.08%	0.011%
32	6.351	1634	1636	1639	rBV4	1281	854	0.07%	0.009%
33	6.402	1649	1652	1654	rBV4	1086	698	0.05%	0.007%
34	6.643	1723	1727	1731	rBV7	1421	1672	0.13%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017203.D
 Acq On : 27 Jun 2020 00:47
 Operator : SY/MD
 Sample : L3133-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.724	1748	1752	1753	rBV4	1407	940	0.07%	0.010%
36	6.865	1792	1796	1799	rBV6	1811	1418	0.11%	0.014%
37	6.884	1799	1802	1806	rVV4	1208	930	0.07%	0.009%
38	7.007	1829	1840	1859	rBV	156627	283515	22.03%	2.882%
39	7.338	1927	1943	1963	rBV	596703	1028661	79.92%	10.455%
40	7.640	2027	2037	2058	rBV	115893	201173	15.63%	2.045%
41	7.894	2112	2116	2120	rBV7	977	907	0.07%	0.009%
42	7.920	2122	2124	2129	rVB4	1314	892	0.07%	0.009%
43	7.949	2129	2133	2135	rBV4	1669	1089	0.08%	0.011%
44	8.106	2172	2182	2207	rBV	288163	535003	41.56%	5.438%
45	8.727	2369	2375	2377	rBV5	1582	1344	0.10%	0.014%
46	8.794	2393	2396	2398	rBV4	1376	720	0.06%	0.007%
47	8.871	2409	2420	2440	rBV	628574	1008640	78.36%	10.251%
48	9.145	2502	2505	2508	rBV3	1081	763	0.06%	0.008%
49	9.241	2533	2535	2538	rBV3	985	753	0.06%	0.008%
50	9.293	2545	2551	2554	rVB7	1321	1399	0.11%	0.014%
51	9.363	2570	2573	2576	rBV3	1052	856	0.07%	0.009%
52	9.389	2579	2581	2585	rVB5	1062	725	0.06%	0.007%
53	9.473	2603	2607	2608	rBV3	1498	1051	0.08%	0.011%
54	9.698	2673	2677	2680	rBV3	1420	1065	0.08%	0.011%
55	9.746	2687	2692	2696	rVB6	1796	1812	0.14%	0.018%
56	9.772	2696	2700	2703	rBV5	1033	858	0.07%	0.009%
57	9.810	2708	2712	2716	rVV7	1257	1172	0.09%	0.012%
58	10.048	2781	2786	2790	rBV5	1422	1612	0.13%	0.016%
59	10.106	2800	2804	2805	rVB4	920	662	0.05%	0.007%
60	10.238	2833	2845	2860	rBV	361373	561504	43.62%	5.707%
61	10.338	2874	2876	2881	rBV5	1443	1017	0.08%	0.010%
62	10.447	2908	2910	2912	rBV3	1408	823	0.06%	0.008%
63	10.486	2919	2922	2930	rVB9	1688	1784	0.14%	0.018%
64	10.566	2944	2947	2951	rBV5	1646	1558	0.12%	0.016%
65	10.640	2966	2970	2971	rBV3	1769	920	0.07%	0.009%
66	10.730	2995	2998	3004	rBV4	1038	1033	0.08%	0.010%
67	10.833	3028	3030	3034	rVB4	1283	857	0.07%	0.009%
68	10.858	3034	3038	3039	rBV2	1748	1182	0.09%	0.012%
69	11.270	3154	3166	3182	rBV	607911	924884	71.85%	9.400%
70	11.482	3229	3232	3237	rBV5	1255	1132	0.09%	0.012%
71	11.505	3237	3239	3242	rVV4	1221	678	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017203.D
 Acq On : 27 Jun 2020 00:47
 Operator : SY/MD
 Sample : L3133-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.563	3254	3257	3259	rBV2	1170	686	0.05%	0.007%
73	11.646	3271	3283	3299	rBV	599854	950112	73.81%	9.656%
74	11.871	3351	3353	3357	rBV4	1444	909	0.07%	0.009%
75	12.132	3432	3434	3439	rVV4	1309	870	0.07%	0.009%
76	12.196	3451	3454	3458	rBV3	996	647	0.05%	0.007%
77	12.630	3587	3589	3593	rBV4	982	782	0.06%	0.008%
78	12.810	3641	3645	3648	rBV5	991	854	0.07%	0.009%
79	13.022	3709	3711	3715	rVB4	1482	716	0.06%	0.007%
80	13.058	3716	3722	3724	rBV5	1637	1439	0.11%	0.015%
81	13.350	3811	3813	3816	rBV2	1254	651	0.05%	0.007%
82	13.518	3862	3865	3867	rBV4	1044	815	0.06%	0.008%
83	13.550	3870	3875	3878	rBV6	1293	1307	0.10%	0.013%
84	13.678	3911	3915	3917	rBV4	960	883	0.07%	0.009%
85	13.723	3926	3929	3931	rBV2	1366	818	0.06%	0.008%
86	13.862	3968	3972	3974	rBV4	1025	803	0.06%	0.008%
87	13.926	3990	3992	3996	rVB5	1669	1052	0.08%	0.011%
88	13.984	4008	4010	4012	rBV2	1530	786	0.06%	0.008%
89	14.154	4061	4063	4067	rVB5	1157	748	0.06%	0.008%
90	14.309	4108	4111	4112	rBV2	1516	753	0.06%	0.008%
91	14.373	4129	4131	4133	rBV2	1076	704	0.05%	0.007%
92	14.543	4178	4184	4186	rBV4	1876	1945	0.15%	0.020%
93	14.601	4197	4202	4206	rBV8	1612	1804	0.14%	0.018%
94	14.627	4206	4210	4212	rBV3	1161	920	0.07%	0.009%
95	14.755	4246	4250	4252	rBV3	1587	1343	0.10%	0.014%
96	14.829	4271	4273	4275	rBV4	1364	691	0.05%	0.007%
97	14.990	4320	4323	4325	rBV3	1163	716	0.06%	0.007%
98	15.125	4363	4365	4366	rBV2	1734	769	0.06%	0.008%
99	15.183	4380	4383	4386	rBV5	1487	1080	0.08%	0.011%
100	15.672	4533	4535	4540	rBV5	2042	1411	0.11%	0.014%


Sum of corrected areas: 9839113

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017203.D
Acq On : 27 Jun 2020 00:47
Operator : SY/MD
Sample : L3133-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

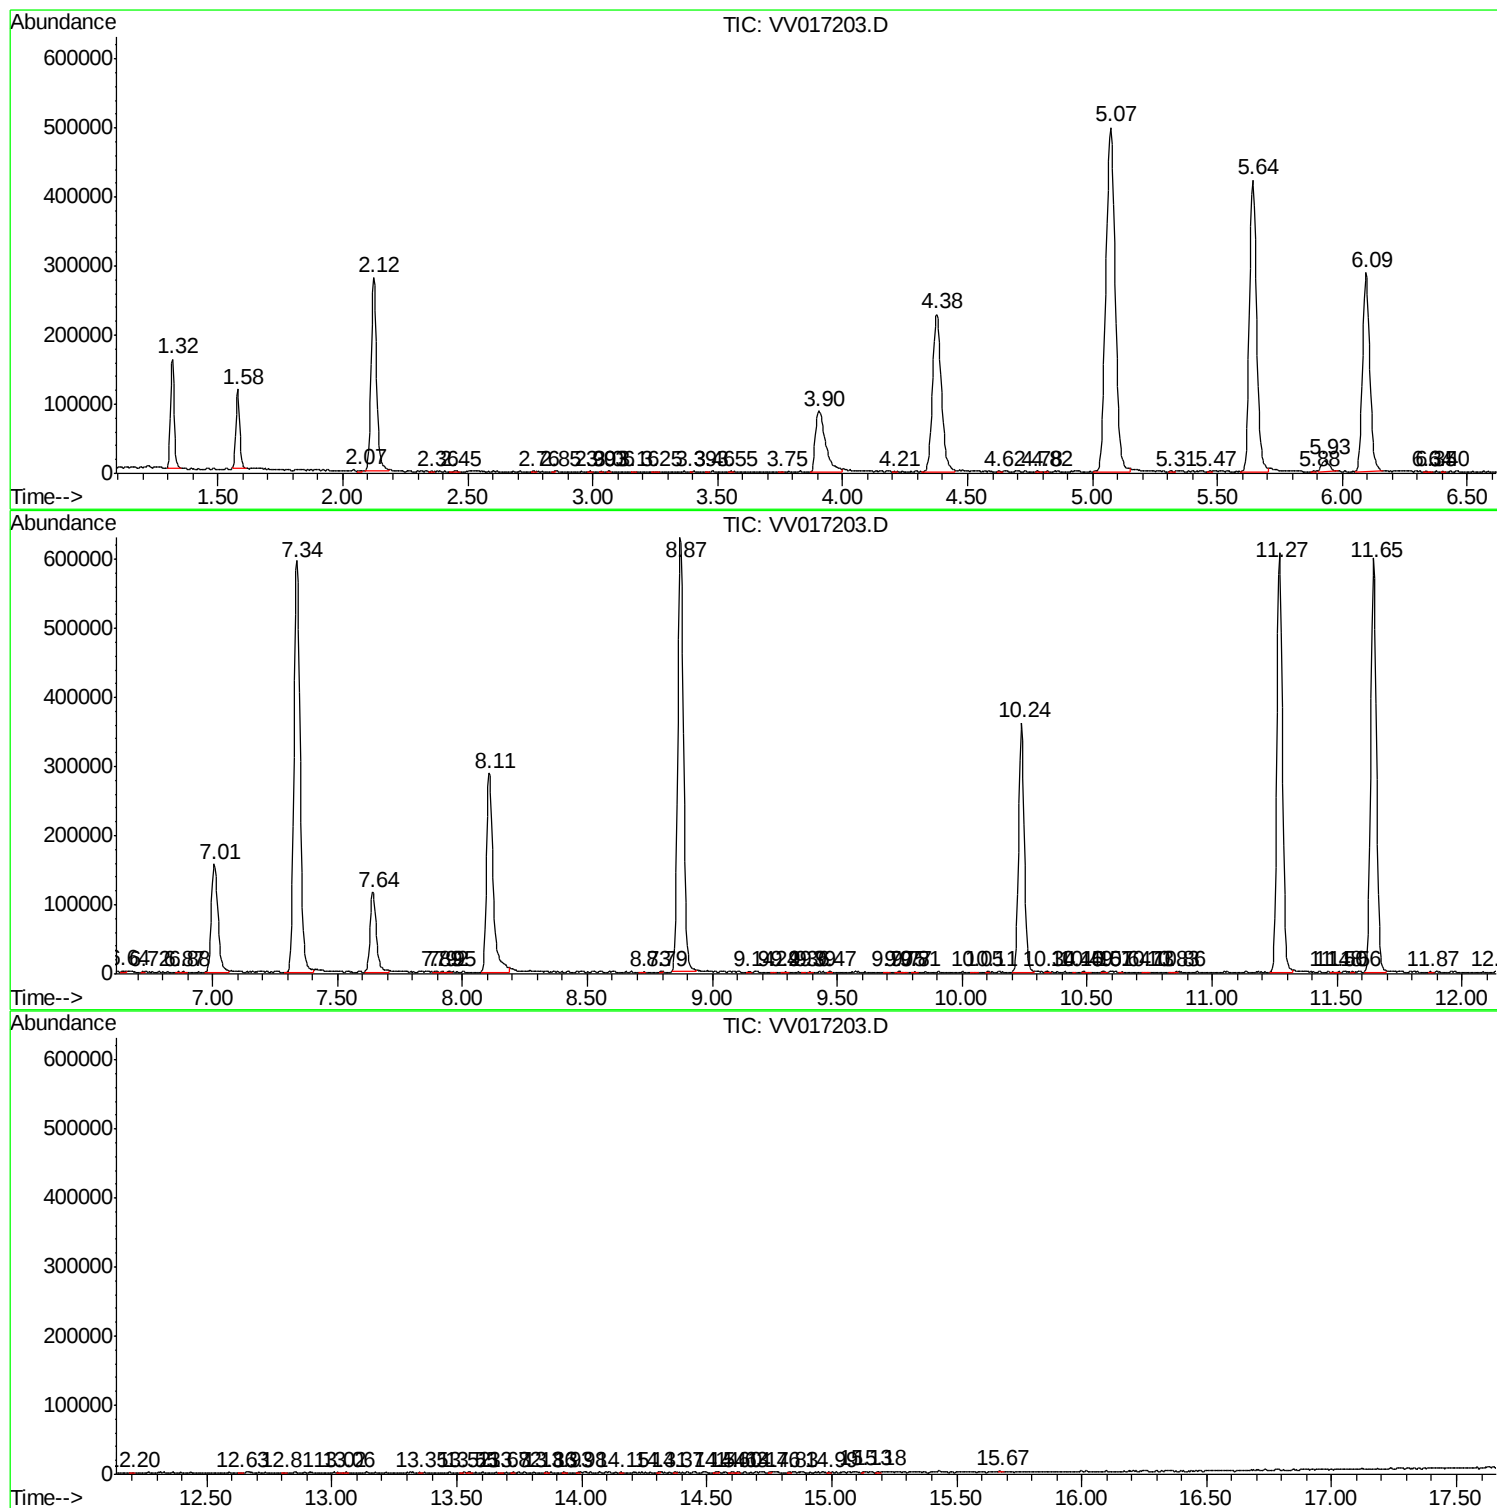

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017203.D
Acq On : 27 Jun 2020 00:47
Operator : SY/MD
Sample : L3133-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017203.D
Acq On : 27 Jun 2020 00:47
Operator : SY/MD
Sample : L3133-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q03

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc