

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017205.D
 Acq On : 27 Jun 2020 01:34
 Operator : SY/MD
 Sample : L3118-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	86	rVB	156021	168615	12.56%	1.647%
2	1.579	145	152	161	rBV	112595	129941	9.68%	1.270%
3	2.122	311	321	339	rBV	288371	436674	32.53%	4.267%
4	2.573	457	461	466	rBV7	1273	1141	0.08%	0.011%
5	2.897	559	562	563	rBV2	987	559	0.04%	0.005%
6	3.180	648	650	655	rVB3	1247	713	0.05%	0.007%
7	3.319	687	693	695	rBV5	1240	972	0.07%	0.009%
8	3.370	707	709	713	rVB4	1125	554	0.04%	0.005%
9	3.585	772	776	778	rBV3	1826	1476	0.11%	0.014%
10	3.608	781	783	787	rVB3	1101	669	0.05%	0.007%
11	3.653	794	797	800	rBV4	1486	886	0.07%	0.009%
12	3.907	862	876	910	rBV2	108057	352532	26.26%	3.444%
13	4.376	1008	1022	1048	rVB	226332	566891	42.23%	5.539%
14	4.933	1190	1195	1196	rBV3	1429	1120	0.08%	0.011%
15	4.962	1200	1204	1206	rBV3	875	640	0.05%	0.006%
16	5.074	1222	1239	1266	rBV2	520647	1342455	100.00%	13.117%
17	5.354	1324	1326	1329	rBV4	1269	727	0.05%	0.007%
18	5.505	1372	1373	1381	rVB7	1482	1497	0.11%	0.015%
19	5.640	1402	1415	1439	rBV	428729	855915	63.76%	8.363%
20	6.093	1543	1556	1578	rBV	304776	607818	45.28%	5.939%
21	6.637	1722	1725	1726	rBV2	1277	797	0.06%	0.008%
22	6.855	1792	1793	1795	rBV2	1152	587	0.04%	0.006%
23	6.900	1804	1807	1809	rBV4	1271	891	0.07%	0.009%
24	6.965	1825	1827	1828	rBV2	1293	582	0.04%	0.006%
25	7.007	1830	1840	1854	rVV2	164916	288918	21.52%	2.823%
26	7.338	1931	1943	1963	rBV	624689	1060993	79.03%	10.367%
27	7.640	2028	2037	2057	rBV	119966	207560	15.46%	2.028%
28	7.907	2118	2120	2123	rBV4	910	565	0.04%	0.006%
29	7.942	2129	2131	2133	rBV2	1117	587	0.04%	0.006%
30	8.000	2144	2149	2151	rBV5	1910	1859	0.14%	0.018%
31	8.013	2151	2153	2156	rVB4	1430	723	0.05%	0.007%
32	8.035	2156	2160	2161	rBV3	1430	939	0.07%	0.009%
33	8.106	2172	2182	2216	rBV	308215	570268	42.48%	5.572%
34	8.871	2408	2420	2444	rVV	644610	1036462	77.21%	10.127%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017205.D
 Acq On : 27 Jun 2020 01:34
 Operator : SY/MD
 Sample : L3118-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	9.161	2507	2510	2516	rVB7	1605	1242	0.09%	0.012%
36	9.248	2533	2537	2541	rBV5	1528	1243	0.09%	0.012%
37	9.341	2564	2566	2569	rVB3	1440	641	0.05%	0.006%
38	9.373	2571	2576	2580	rVB5	1782	1418	0.11%	0.014%
39	9.392	2580	2582	2588	rBV5	1221	1217	0.09%	0.012%
40	9.495	2608	2614	2617	rBV5	1571	1647	0.12%	0.016%
41	9.649	2659	2662	2665	rBV3	1057	792	0.06%	0.008%
42	9.711	2679	2681	2686	rBV5	700	592	0.04%	0.006%
43	9.765	2693	2698	2700	rBV3	1260	985	0.07%	0.010%
44	10.003	2768	2772	2773	rBV4	1197	653	0.05%	0.006%
45	10.039	2780	2783	2784	rBV2	1699	803	0.06%	0.008%
46	10.125	2806	2810	2813	rBV4	916	840	0.06%	0.008%
47	10.164	2819	2822	2825	rBV4	1019	647	0.05%	0.006%
48	10.238	2831	2845	2859	rBV	378423	595578	44.36%	5.819%
49	10.498	2921	2926	2927	rBV5	877	813	0.06%	0.008%
50	10.608	2957	2960	2961	rBV3	1281	663	0.05%	0.006%
51	10.723	2994	2996	2999	rVB5	1376	787	0.06%	0.008%
52	10.759	3004	3007	3012	rBV7	1146	1026	0.08%	0.010%
53	10.813	3018	3024	3028	rBV7	1586	2061	0.15%	0.020%
54	10.862	3037	3039	3040	rBV2	1208	597	0.04%	0.006%
55	10.932	3058	3061	3065	rBV5	1441	1133	0.08%	0.011%
56	10.958	3067	3069	3073	rVB4	1421	989	0.07%	0.010%
57	11.000	3079	3082	3083	rBV2	1135	698	0.05%	0.007%
58	11.077	3102	3106	3107	rBV3	1444	999	0.07%	0.010%
59	11.270	3155	3166	3182	rBV	633033	952031	70.92%	9.302%
60	11.370	3195	3197	3201	rBV4	1403	914	0.07%	0.009%
61	11.415	3208	3211	3214	rBV4	1242	810	0.06%	0.008%
62	11.453	3220	3223	3225	rBV4	1399	575	0.04%	0.006%
63	11.469	3226	3228	3232	rBV4	1658	1028	0.08%	0.010%
64	11.646	3272	3283	3301	rVB	637457	985756	73.43%	9.631%
65	11.858	3345	3349	3350	rBV4	1142	742	0.06%	0.007%
66	11.955	3376	3379	3382	rBV4	1078	788	0.06%	0.008%
67	12.003	3392	3394	3396	rVB3	1417	640	0.05%	0.006%
68	12.074	3414	3416	3422	rVB4	1113	812	0.06%	0.008%
69	12.141	3434	3437	3442	rBV8	1495	1812	0.13%	0.018%
70	12.264	3473	3475	3479	rVB3	1655	1071	0.08%	0.010%
71	12.299	3484	3486	3488	rVB3	1606	625	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017205.D
 Acq On : 27 Jun 2020 01:34
 Operator : SY/MD
 Sample : L3118-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.405	3515	3519	3523	rBV6	1237	1072	0.08%	0.010%
73	12.428	3523	3526	3529	rBV4	1232	914	0.07%	0.009%
74	12.489	3542	3545	3547	rBV3	1659	992	0.07%	0.010%
75	12.601	3576	3580	3584	rBV6	1027	859	0.06%	0.008%
76	12.627	3584	3588	3592	rVV7	1378	1132	0.08%	0.011%
77	12.688	3604	3607	3612	rBV5	1549	1334	0.10%	0.013%
78	12.807	3641	3644	3645	rBV2	1460	838	0.06%	0.008%
79	12.984	3696	3699	3701	rVB3	1427	645	0.05%	0.006%
80	13.096	3731	3734	3735	rBV4	1131	661	0.05%	0.006%
81	13.138	3742	3747	3752	rBV9	1209	1389	0.10%	0.014%
82	13.270	3784	3788	3790	rBV3	1127	870	0.06%	0.009%
83	13.363	3813	3817	3819	rBV4	700	542	0.04%	0.005%
84	13.382	3819	3823	3824	rBV4	1106	955	0.07%	0.009%
85	13.569	3878	3881	3882	rBV2	1146	666	0.05%	0.007%
86	13.595	3886	3889	3891	rVB5	1100	637	0.05%	0.006%
87	13.608	3891	3893	3897	rBV4	1024	742	0.06%	0.007%
88	13.656	3906	3908	3909	rBV2	1471	670	0.05%	0.007%
89	13.749	3932	3937	3941	rBV6	1693	1772	0.13%	0.017%
90	14.189	4071	4074	4081	rVB8	1449	1362	0.10%	0.013%
91	14.308	4108	4111	4114	rBV4	1303	862	0.06%	0.008%
92	14.463	4156	4159	4161	rVB3	1493	853	0.06%	0.008%
93	14.482	4161	4165	4166	rBV4	816	582	0.04%	0.006%
94	14.537	4179	4182	4186	rVB4	1105	834	0.06%	0.008%
95	14.990	4321	4323	4325	rBV2	1510	645	0.05%	0.006%
96	15.115	4360	4362	4365	rBV3	1584	1020	0.08%	0.010%
97	15.157	4373	4375	4379	rVB3	1169	723	0.05%	0.007%
98	15.263	4406	4408	4410	rBV3	1371	677	0.05%	0.007%
99	15.408	4450	4453	4455	rBV4	992	681	0.05%	0.007%
100	15.550	4496	4497	4502	rVB5	1533	615	0.05%	0.006%


Sum of corrected areas: 10234738

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017205.D
Acq On : 27 Jun 2020 01:34
Operator : SY/MD
Sample : L3118-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

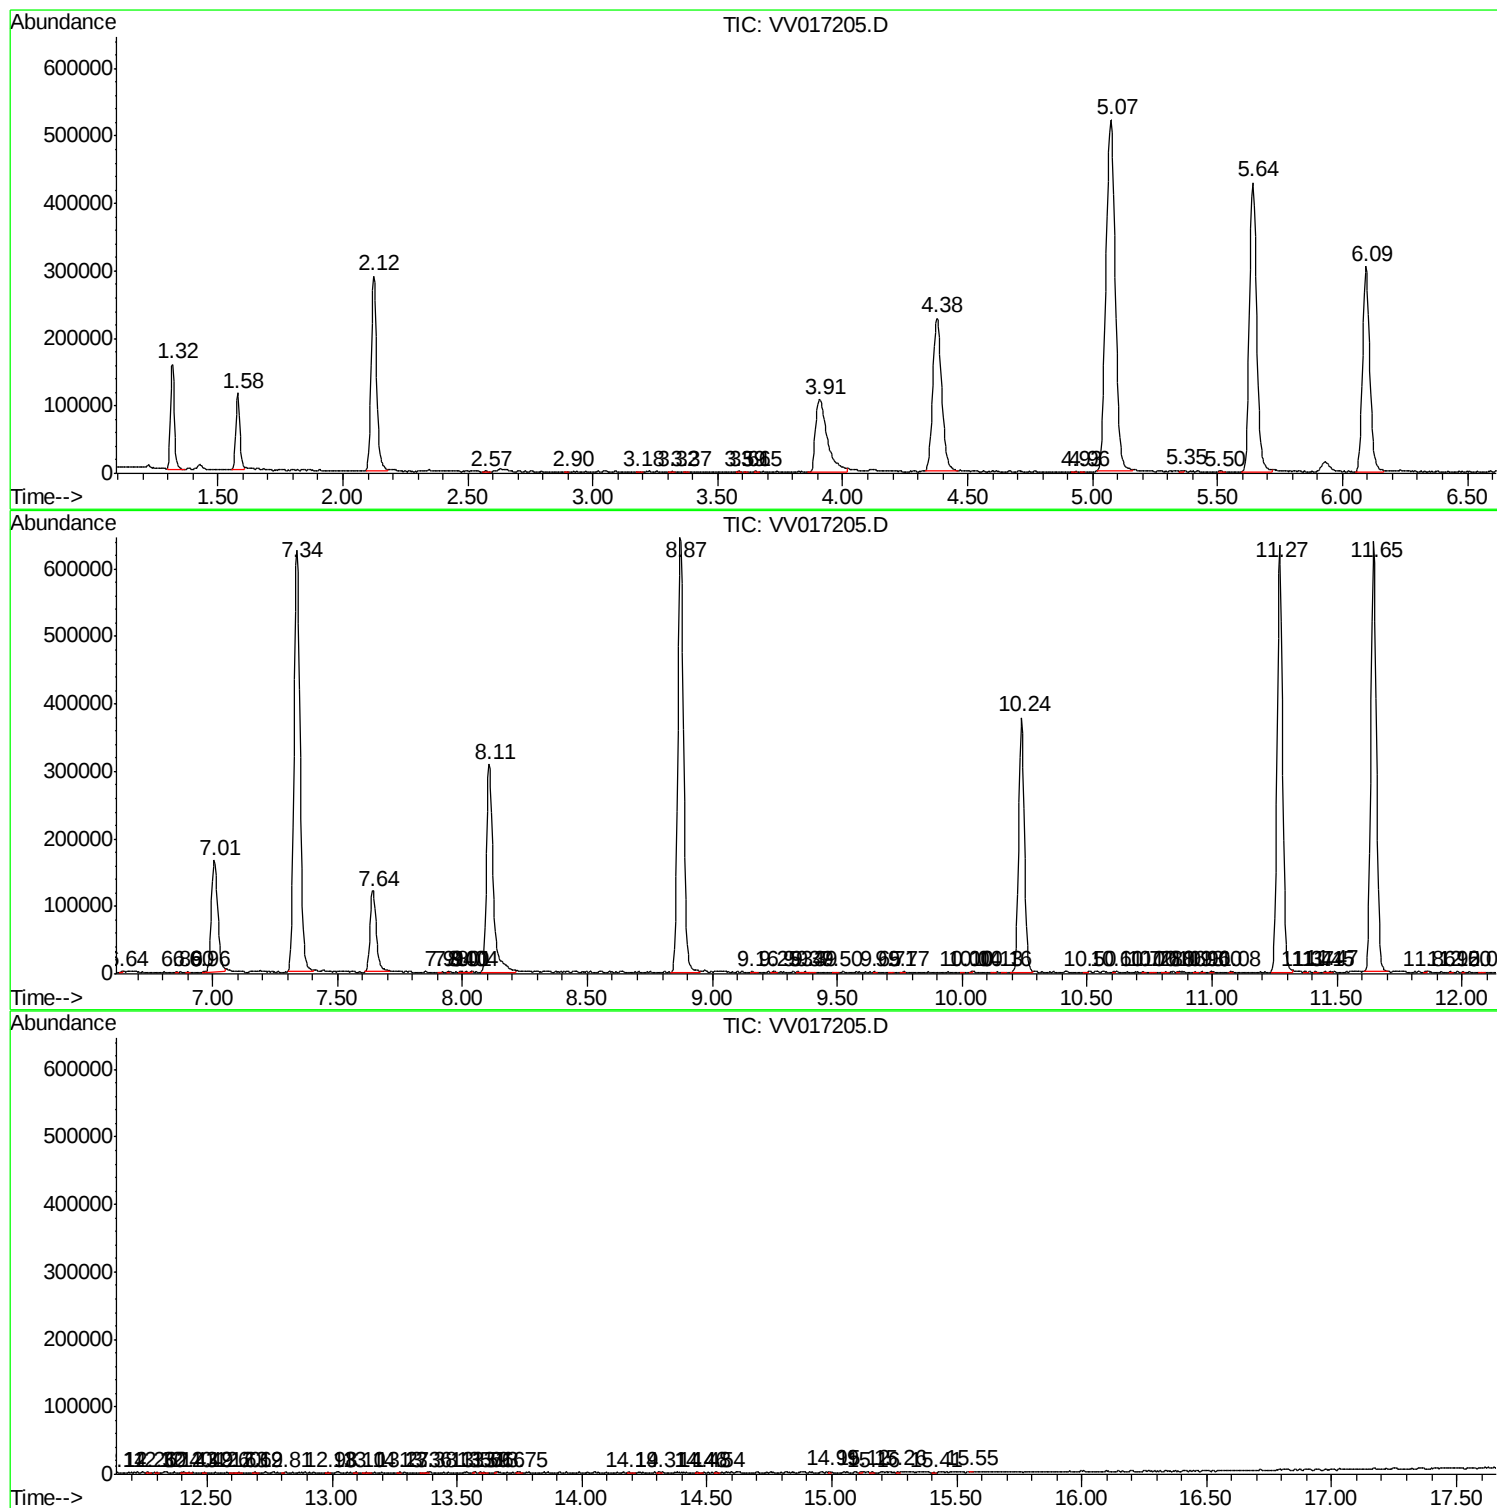

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017205.D
Acq On : 27 Jun 2020 01:34
Operator : SY/MD
Sample : L3118-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F58

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017205.D
Acq On : 27 Jun 2020 01:34
Operator : SY/MD
Sample : L3118-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F58

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc