

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017206.D
 Acq On : 27 Jun 2020 01:57
 Operator : SY/MD
 Sample : L3118-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	152655	158899	12.25%	1.593%
2	1.579	145	152	161	rBV	108395	123079	9.49%	1.234%
3	2.122	311	321	338	rBV	278334	418421	32.25%	4.195%
4	2.261	362	364	367	rVB4	1403	637	0.05%	0.006%
5	2.598	467	469	473	rBV3	1289	1107	0.09%	0.011%
6	2.756	514	518	519	rBV3	1427	974	0.08%	0.010%
7	2.839	542	544	547	rVB2	1526	1057	0.08%	0.011%
8	2.865	547	552	555	rBV5	851	895	0.07%	0.009%
9	2.913	564	567	568	rBV3	1548	932	0.07%	0.009%
10	2.949	576	578	581	rBV3	971	571	0.04%	0.006%
11	3.036	603	605	608	rBV3	920	513	0.04%	0.005%
12	3.077	616	618	624	rBV7	1279	1024	0.08%	0.010%
13	3.228	663	665	668	rBV3	1032	550	0.04%	0.006%
14	3.299	684	687	689	rBV3	1296	958	0.07%	0.010%
15	3.325	693	695	697	rBV2	1316	670	0.05%	0.007%
16	3.373	708	710	713	rVB3	884	531	0.04%	0.005%
17	3.399	713	718	719	rBV3	873	772	0.06%	0.008%
18	3.428	725	727	730	rVB4	1271	754	0.06%	0.008%
19	3.486	743	745	749	rBV4	1053	670	0.05%	0.007%
20	3.669	799	802	804	rBV3	1098	708	0.05%	0.007%
21	3.701	810	812	815	rBV3	919	665	0.05%	0.007%
22	3.798	838	842	844	rBV3	1118	808	0.06%	0.008%
23	3.907	862	876	912	rBV2	103451	336715	25.95%	3.376%
24	4.376	1006	1022	1047	rBV	221069	564239	43.49%	5.656%
25	4.618	1095	1097	1099	rVB4	1464	635	0.05%	0.006%
26	4.746	1131	1137	1141	rBV7	1374	1911	0.15%	0.019%
27	4.781	1145	1148	1150	rVV3	928	523	0.04%	0.005%
28	4.994	1210	1214	1216	rBV3	1486	1251	0.10%	0.013%
29	5.013	1216	1220	1221	rVV3	1951	1088	0.08%	0.011%
30	5.071	1221	1238	1264	rVV2	505033	1297391	100.00%	13.006%
31	5.322	1313	1316	1321	rBV7	1738	1884	0.15%	0.019%
32	5.473	1360	1363	1366	rBV4	1408	1041	0.08%	0.010%
33	5.524	1376	1379	1381	rBV3	1567	991	0.08%	0.010%
34	5.640	1402	1415	1438	rBV	425235	852602	65.72%	8.547%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017206.D
 Acq On : 27 Jun 2020 01:57
 Operator : SY/MD
 Sample : L3118-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.093	1542	1556	1577	rBV	291877	585347	45.12%	5.868%
36	6.270	1607	1611	1616	rVB6	1132	1121	0.09%	0.011%
37	6.309	1621	1623	1625	rBV2	1133	591	0.05%	0.006%
38	6.376	1641	1644	1649	rBV5	1371	1494	0.12%	0.015%
39	6.958	1823	1825	1828	rBV4	1489	973	0.07%	0.010%
40	7.006	1830	1840	1855	rVV	160660	282530	21.78%	2.832%
41	7.174	1889	1892	1897	rBV5	1720	1422	0.11%	0.014%
42	7.289	1923	1928	1930	rBV4	1709	1348	0.10%	0.014%
43	7.338	1931	1943	1964	rVV	596099	1022016	78.77%	10.246%
44	7.592	2019	2022	2023	rBV2	1057	573	0.04%	0.006%
45	7.640	2028	2037	2052	rVV2	115889	197942	15.26%	1.984%
46	7.949	2129	2133	2134	rBV2	1182	678	0.05%	0.007%
47	7.997	2143	2148	2153	rBV7	1536	1707	0.13%	0.017%
48	8.032	2157	2159	2164	rBV6	1194	891	0.07%	0.009%
49	8.061	2166	2168	2170	rBV3	977	507	0.04%	0.005%
50	8.106	2173	2182	2207	rBV	294374	538923	41.54%	5.403%
51	8.585	2328	2331	2334	rBV3	1205	721	0.06%	0.007%
52	8.768	2384	2388	2391	rBV4	1501	1411	0.11%	0.014%
53	8.875	2404	2421	2444	rBV	626571	1024091	78.93%	10.266%
54	9.093	2487	2489	2492	rBV3	1518	933	0.07%	0.009%
55	9.231	2530	2532	2535	rBV3	1074	769	0.06%	0.008%
56	9.347	2565	2568	2570	rBV4	1361	794	0.06%	0.008%
57	9.540	2626	2628	2632	rVB4	1391	895	0.07%	0.009%
58	9.569	2632	2637	2640	rBV7	1919	1447	0.11%	0.015%
59	9.592	2640	2644	2646	rBV3	1362	880	0.07%	0.009%
60	9.701	2676	2678	2681	rVB2	1808	959	0.07%	0.010%
61	9.723	2681	2685	2687	rBV5	1445	1088	0.08%	0.011%
62	9.945	2748	2754	2755	rBV5	979	789	0.06%	0.008%
63	10.039	2779	2783	2787	rBV7	1395	1461	0.11%	0.015%
64	10.067	2789	2792	2795	rVB3	1579	1089	0.08%	0.011%
65	10.087	2795	2798	2799	rBV3	1280	527	0.04%	0.005%
66	10.238	2831	2845	2858	rBV	363825	575876	44.39%	5.773%
67	10.411	2896	2899	2905	rBV8	1369	1419	0.11%	0.014%
68	10.543	2936	2940	2942	rBV4	1696	933	0.07%	0.009%
69	10.743	2998	3002	3005	rVB6	1297	1032	0.08%	0.010%
70	10.846	3030	3034	3037	rBV4	1314	1030	0.08%	0.010%
71	10.923	3056	3058	3064	rVV7	978	851	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017206.D
 Acq On : 27 Jun 2020 01:57
 Operator : SY/MD
 Sample : L3118-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.987	3075	3078	3079	rBV3	1364	696	0.05%	0.007%
73	11.083	3104	3108	3114	rBV8	1663	1799	0.14%	0.018%
74	11.183	3136	3139	3141	rBV3	1394	872	0.07%	0.009%
75	11.270	3153	3166	3188	rBV	608291	939958	72.45%	9.423%
76	11.411	3208	3210	3214	rBV3	988	633	0.05%	0.006%
77	11.646	3272	3283	3301	rVB	622082	977782	75.37%	9.802%
78	11.865	3350	3351	3356	rBV4	811	714	0.06%	0.007%
79	12.038	3402	3405	3408	rBV5	1251	904	0.07%	0.009%
80	12.241	3465	3468	3470	rBV4	1332	887	0.07%	0.009%
81	12.575	3568	3572	3576	rBV6	1422	1269	0.10%	0.013%
82	12.662	3595	3599	3601	rBV5	1624	1458	0.11%	0.015%
83	12.733	3617	3621	3623	rBV4	1275	999	0.08%	0.010%
84	12.929	3678	3682	3686	rBV5	1101	1044	0.08%	0.010%
85	12.958	3690	3691	3693	rBV2	1040	525	0.04%	0.005%
86	13.148	3748	3750	3752	rBV2	920	517	0.04%	0.005%
87	13.235	3773	3777	3779	rBV3	1089	957	0.07%	0.010%
88	13.357	3812	3815	3818	rBV3	880	602	0.05%	0.006%
89	13.402	3826	3829	3832	rBV5	1468	909	0.07%	0.009%
90	13.463	3845	3848	3850	rBV3	1647	1128	0.09%	0.011%
91	13.501	3857	3860	3864	rBV3	1268	949	0.07%	0.010%
92	13.595	3887	3889	3891	rBV3	1124	632	0.05%	0.006%
93	13.694	3918	3920	3924	rVB4	1061	545	0.04%	0.005%
94	13.890	3978	3981	3985	rBV4	1343	980	0.08%	0.010%
95	14.003	4013	4016	4018	rBV2	1129	648	0.05%	0.006%
96	14.144	4056	4060	4064	rVB7	1642	1335	0.10%	0.013%
97	14.164	4064	4066	4068	rBV2	1158	573	0.04%	0.006%
98	14.411	4141	4143	4146	rBV3	1551	1043	0.08%	0.010%
99	14.868	4280	4285	4289	rBV6	1476	1708	0.13%	0.017%
100	15.022	4331	4333	4337	rBV4	1114	663	0.05%	0.007%


Sum of corrected areas: 9975253

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017206.D
Acq On : 27 Jun 2020 01:57
Operator : SY/MD
Sample : L3118-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

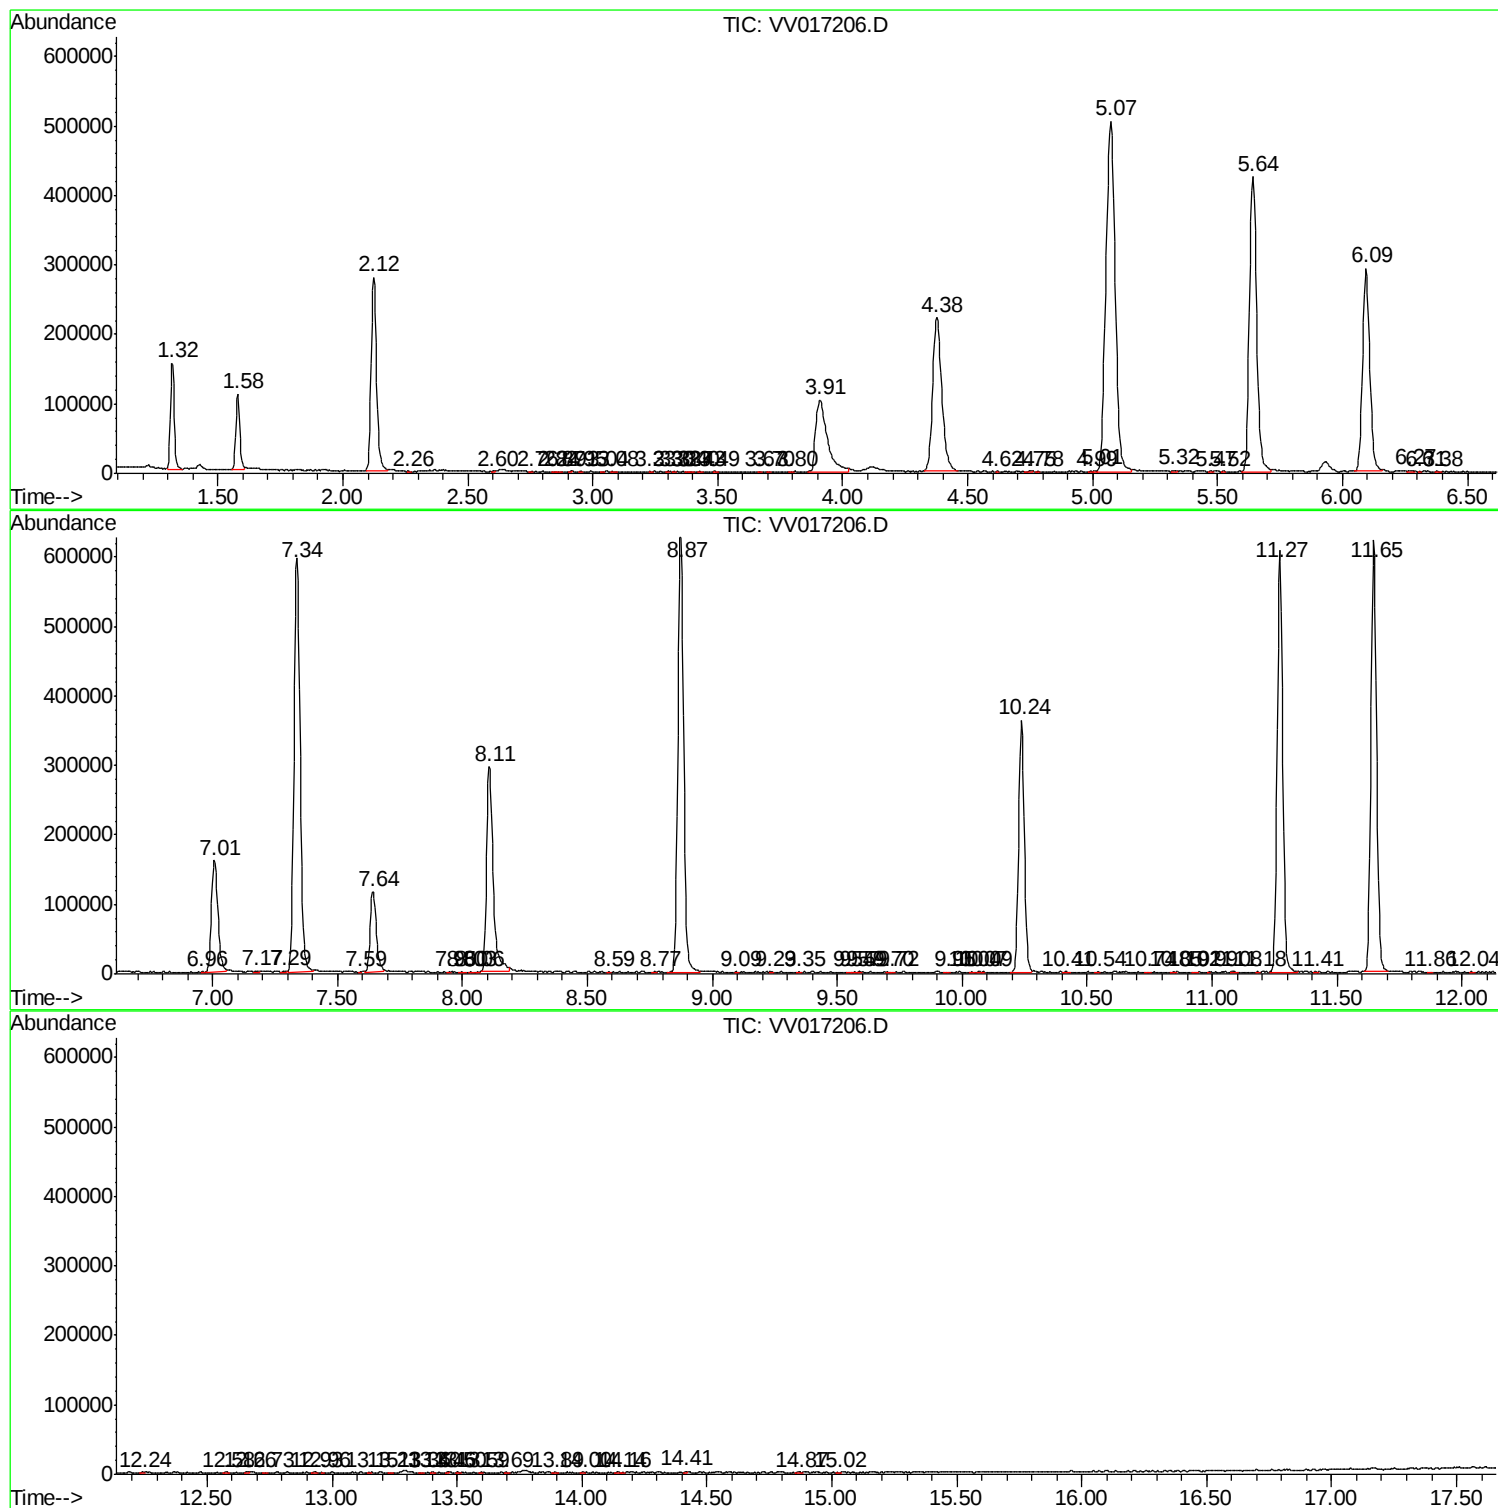

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017206.D
Acq On : 27 Jun 2020 01:57
Operator : SY/MD
Sample : L3118-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F77

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017206.D
Acq On : 27 Jun 2020 01:57
Operator : SY/MD
Sample : L3118-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F77

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc