

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017209.D
 Acq On : 27 Jun 2020 03:07
 Operator : SY/MD
 Sample : L3132-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	82	rVB	156130	159550	12.40%	1.588%
2	1.579	145	152	161	rBV	117268	128021	9.95%	1.274%
3	2.122	311	321	338	rBV	272544	410299	31.89%	4.083%
4	2.280	367	370	371	rBV2	1522	643	0.05%	0.006%
5	2.781	522	526	528	rBV3	1001	744	0.06%	0.007%
6	2.894	558	561	562	rBV3	1090	613	0.05%	0.006%
7	2.929	570	572	576	rBV4	1359	947	0.07%	0.009%
8	3.035	604	605	607	rBV	1088	576	0.04%	0.006%
9	3.097	620	624	627	rBV5	978	883	0.07%	0.009%
10	3.380	710	712	715	rBV4	1017	621	0.05%	0.006%
11	3.582	772	775	777	rBV3	1462	840	0.07%	0.008%
12	3.608	777	783	785	rBV5	774	728	0.06%	0.007%
13	3.624	785	788	790	rBV4	959	693	0.05%	0.007%
14	3.675	801	804	808	rVB3	1007	642	0.05%	0.006%
15	3.794	837	841	844	rBV4	1209	980	0.08%	0.010%
16	3.859	858	861	863	rBV4	1597	784	0.06%	0.008%
17	3.907	865	876	906	rBV	85931	248852	19.34%	2.476%
18	4.376	1009	1022	1050	rVB	213539	519753	40.39%	5.172%
19	4.540	1071	1073	1077	rVB4	1396	962	0.07%	0.010%
20	4.611	1092	1095	1099	rVB4	1624	1046	0.08%	0.010%
21	4.640	1099	1104	1107	rBV6	1222	1187	0.09%	0.012%
22	4.814	1153	1158	1159	rBV5	978	811	0.06%	0.008%
23	4.846	1165	1168	1171	rBV5	1071	848	0.07%	0.008%
24	5.071	1220	1238	1268	rBV2	489827	1286743	100.00%	12.803%
25	5.328	1312	1318	1323	rBV9	2357	2808	0.22%	0.028%
26	5.418	1344	1346	1351	rVB5	1769	952	0.07%	0.009%
27	5.640	1402	1415	1439	rVV	428107	855569	66.49%	8.513%
28	5.939	1497	1508	1525	rVB	13870	35547	2.76%	0.354%
29	6.093	1542	1556	1576	rBV	288395	578820	44.98%	5.759%
30	6.424	1655	1659	1665	rBV4	1103	1320	0.10%	0.013%
31	6.521	1684	1689	1693	rBV7	1268	1581	0.12%	0.016%
32	6.553	1697	1699	1702	rBV4	978	707	0.05%	0.007%
33	6.727	1751	1753	1757	rVB4	1660	915	0.07%	0.009%
34	6.804	1772	1777	1780	rBV7	1066	1169	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017209.D
 Acq On : 27 Jun 2020 03:07
 Operator : SY/MD
 Sample : L3132-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.878	1798	1800	1802	rVB3	1380	610	0.05%	0.006%
36	6.932	1814	1817	1819	rBV3	1266	1042	0.08%	0.010%
37	6.952	1820	1823	1826	rVV4	1907	1208	0.09%	0.012%
38	7.006	1830	1840	1857	rVV2	154729	279951	21.76%	2.786%
39	7.338	1931	1943	1962	rBV	587862	1014008	78.80%	10.090%
40	7.601	2022	2025	2026	rBV3	1349	732	0.06%	0.007%
41	7.643	2028	2038	2052	rVV	112617	192992	15.00%	1.920%
42	7.791	2081	2084	2085	rBV2	1355	784	0.06%	0.008%
43	7.836	2095	2098	2100	rBV2	1144	671	0.05%	0.007%
44	7.997	2137	2148	2167	rVB2	111984	196255	15.25%	1.953%
45	8.109	2171	2183	2200	rBV	287947	524821	40.79%	5.222%
46	8.723	2371	2374	2375	rBV3	2312	1070	0.08%	0.011%
47	8.807	2396	2400	2403	rBV4	1116	1065	0.08%	0.011%
48	8.871	2409	2420	2443	rBV	641688	1032297	80.23%	10.272%
49	9.132	2498	2501	2502	rBV2	1199	802	0.06%	0.008%
50	9.174	2510	2514	2518	rVB5	1224	779	0.06%	0.008%
51	9.492	2610	2613	2617	rBV3	1440	766	0.06%	0.008%
52	9.514	2617	2620	2627	rBV7	1250	1431	0.11%	0.014%
53	9.582	2638	2641	2644	rBV5	1126	703	0.05%	0.007%
54	9.659	2662	2665	2671	rVB5	1536	1344	0.10%	0.013%
55	9.749	2688	2693	2696	rBV4	1370	1564	0.12%	0.016%
56	9.823	2713	2716	2721	rBV4	1401	1054	0.08%	0.010%
57	9.997	2768	2770	2776	rVB7	1240	707	0.05%	0.007%
58	10.055	2785	2788	2790	rBV3	1118	651	0.05%	0.006%
59	10.193	2829	2831	2833	rBV2	1195	689	0.05%	0.007%
60	10.238	2833	2845	2865	rVB	374657	576523	44.80%	5.737%
61	10.447	2907	2910	2912	rBV4	1517	731	0.06%	0.007%
62	10.730	2992	2998	3000	rBV5	1377	1405	0.11%	0.014%
63	10.874	3038	3043	3046	rBV5	1184	1367	0.11%	0.014%
64	10.919	3056	3057	3061	rVB4	1319	727	0.06%	0.007%
65	10.942	3061	3064	3067	rBV5	649	598	0.05%	0.006%
66	11.148	3125	3128	3133	rVB5	1679	1407	0.11%	0.014%
67	11.177	3133	3137	3139	rBV4	1459	1233	0.10%	0.012%
68	11.225	3148	3152	3155	rBV6	1027	948	0.07%	0.009%
69	11.270	3155	3166	3186	rVV	622264	959561	74.57%	9.548%
70	11.505	3235	3239	3241	rVB3	837	582	0.05%	0.006%
71	11.646	3268	3283	3301	rBV	606815	965807	75.06%	9.610%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017209.D
 Acq On : 27 Jun 2020 03:07
 Operator : SY/MD
 Sample : L3132-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.829	3337	3340	3344	rBV5	1666	1201	0.09%	0.012%
73	11.871	3350	3353	3356	rBV3	1514	849	0.07%	0.008%
74	11.974	3383	3385	3388	rBV3	1560	968	0.08%	0.010%
75	12.302	3483	3487	3490	rVB3	1103	841	0.07%	0.008%
76	12.370	3505	3508	3510	rBV3	1392	918	0.07%	0.009%
77	12.501	3545	3549	3550	rBV2	1917	1059	0.08%	0.011%
78	12.588	3572	3576	3578	rBV4	886	735	0.06%	0.007%
79	12.656	3594	3597	3601	rBV5	1679	1283	0.10%	0.013%
80	12.794	3635	3640	3641	rBV3	1204	972	0.08%	0.010%
81	12.942	3684	3686	3692	rVB5	1149	884	0.07%	0.009%
82	13.009	3704	3707	3711	rBV4	936	752	0.06%	0.007%
83	13.138	3743	3747	3749	rBV3	835	624	0.05%	0.006%
84	13.289	3787	3794	3803	rVB3	5878	8894	0.69%	0.088%
85	13.357	3813	3815	3819	rBV4	824	708	0.06%	0.007%
86	13.424	3833	3836	3838	rBV3	1505	986	0.08%	0.010%
87	13.550	3873	3875	3881	rVB5	1451	1194	0.09%	0.012%
88	13.620	3893	3897	3900	rBV4	1649	1109	0.09%	0.011%
89	13.652	3904	3907	3910	rBV5	876	670	0.05%	0.007%
90	13.710	3921	3925	3927	rBV4	892	678	0.05%	0.007%
91	14.080	4037	4040	4043	rBV5	936	885	0.07%	0.009%
92	14.128	4053	4055	4058	rVB3	1292	661	0.05%	0.007%
93	14.167	4065	4067	4071	rBV4	1010	644	0.05%	0.006%
94	14.392	4134	4137	4139	rBV2	1072	803	0.06%	0.008%
95	14.726	4237	4241	4243	rBV3	1074	877	0.07%	0.009%
96	14.897	4291	4294	4299	rVB5	1843	1380	0.11%	0.014%
97	15.244	4400	4402	4404	rBV3	1404	727	0.06%	0.007%
98	15.369	4439	4441	4444	rVB3	1278	664	0.05%	0.007%
99	15.585	4505	4508	4510	rBV3	1580	970	0.08%	0.010%
100	15.694	4540	4542	4546	rBV5	1517	1016	0.08%	0.010%


Sum of corrected areas: 10049991

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017209.D
Acq On : 27 Jun 2020 03:07
Operator : SY/MD
Sample : L3132-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

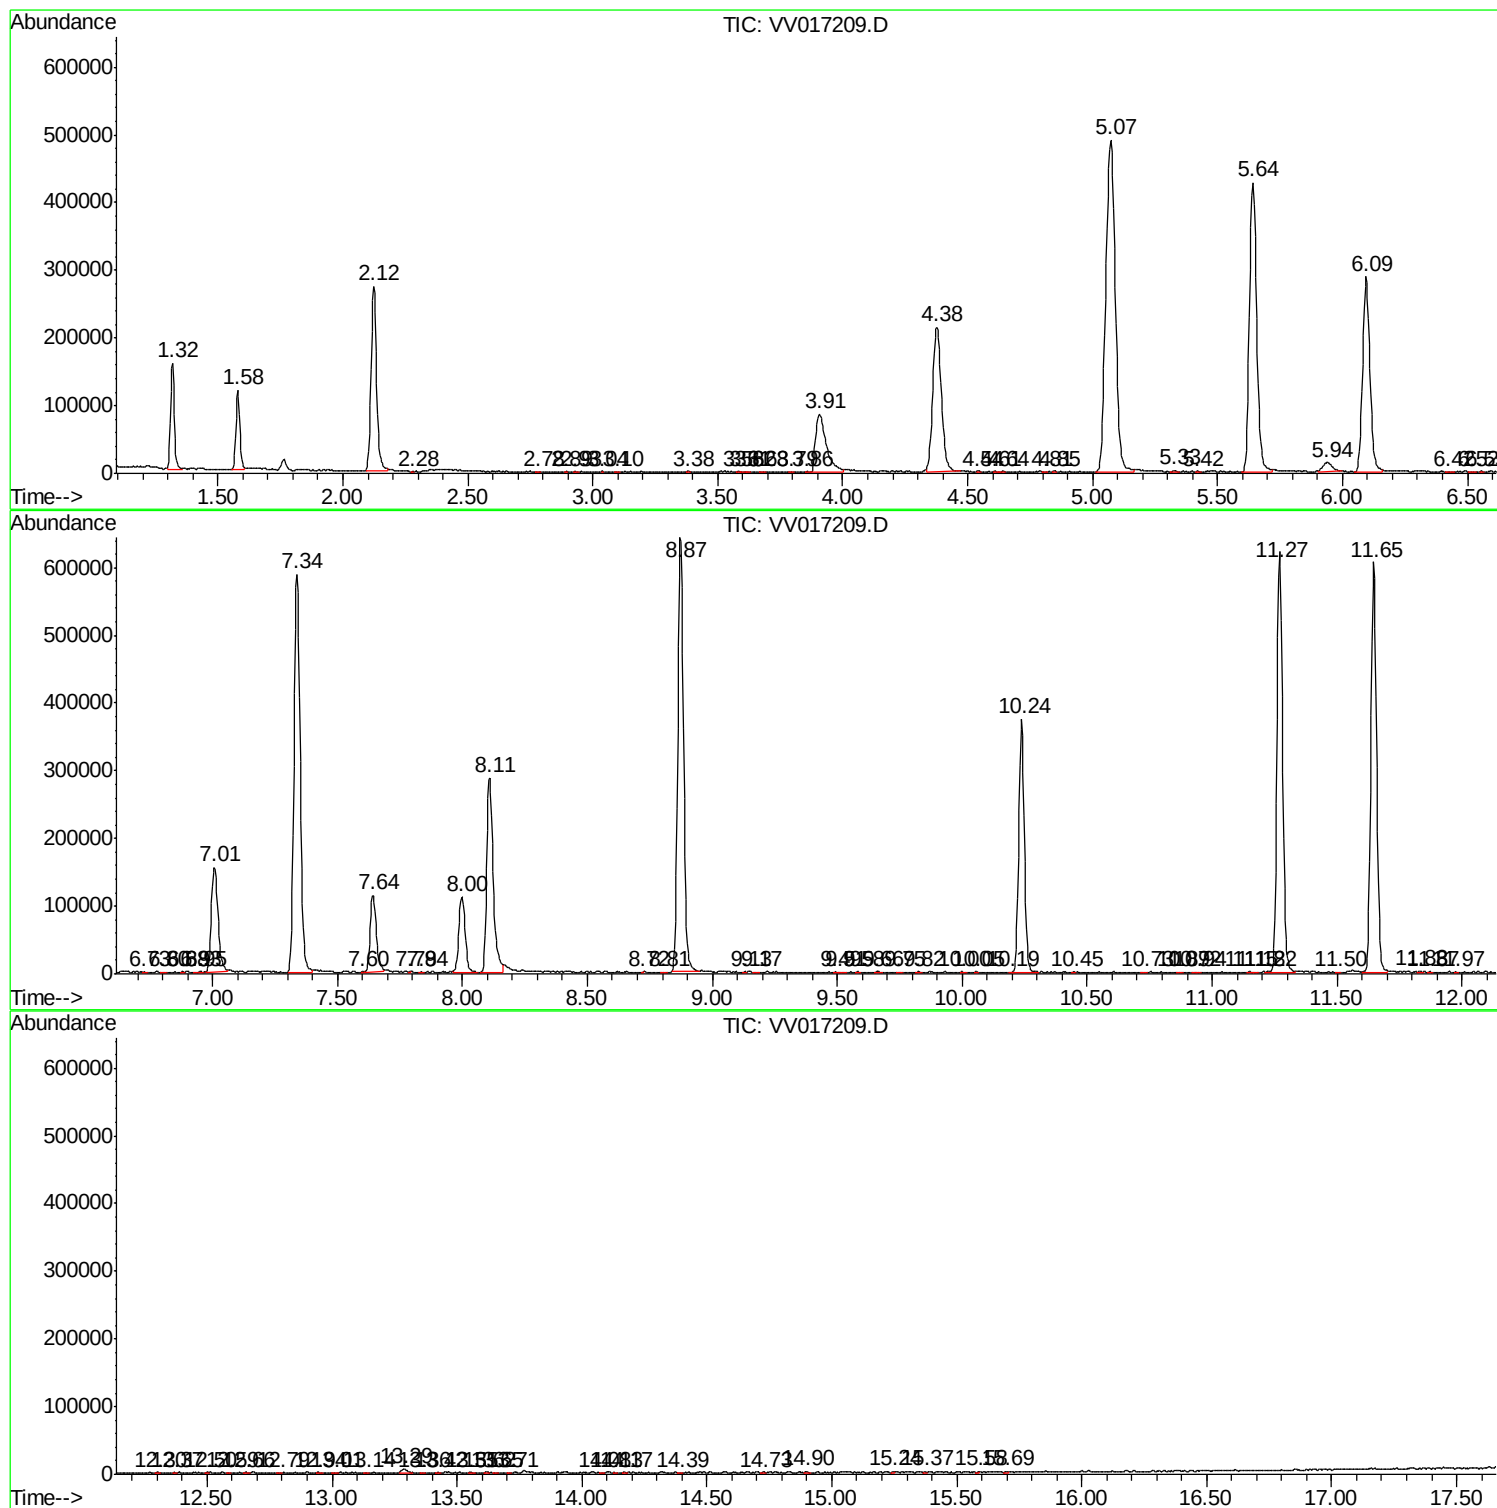

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017209.D
Acq On : 27 Jun 2020 03:07
Operator : SY/MD
Sample : L3132-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y24

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017209.D
Acq On : 27 Jun 2020 03:07
Operator : SY/MD
Sample : L3132-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y24

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc