

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017210.D
 Acq On : 27 Jun 2020 03:30
 Operator : SY/MD
 Sample : L3132-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y28

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	82	rVB	154654	166308	12.42%	1.542%
2	1.579	146	152	162	rVB	106304	118189	8.83%	1.096%
3	1.762	203	209	222	rVB	50077	66829	4.99%	0.620%
4	2.122	311	321	341	rBV	288440	431905	32.27%	4.004%
5	2.634	478	480	484	rBV5	1023	656	0.05%	0.006%
6	2.688	493	497	501	rBV5	1425	1312	0.10%	0.012%
7	2.708	501	503	504	rBV2	1129	598	0.04%	0.006%
8	2.762	518	520	522	rBV3	1555	749	0.06%	0.007%
9	2.859	548	550	553	rBV4	1058	830	0.06%	0.008%
10	2.971	580	585	587	rBV4	1924	1580	0.12%	0.015%
11	3.045	604	608	610	rBV3	1302	1028	0.08%	0.010%
12	3.074	613	617	618	rBV3	1330	839	0.06%	0.008%
13	3.109	625	628	632	rBV	11009	6074	0.45%	0.056%
14	3.315	689	692	696	rBV5	1815	1689	0.13%	0.016%
15	3.463	736	738	741	rVB4	1475	763	0.06%	0.007%
16	3.482	741	744	746	rBV3	1117	586	0.04%	0.005%
17	3.505	746	751	753	rBV4	994	831	0.06%	0.008%
18	3.637	790	792	794	rBV3	1131	605	0.05%	0.006%
19	3.823	847	850	853	rBV3	949	736	0.05%	0.007%
20	3.904	864	875	905	rBV2	93740	272947	20.39%	2.531%
21	4.302	997	999	1004	rVB4	1250	776	0.06%	0.007%
22	4.376	1004	1022	1043	rBV2	222765	547643	40.91%	5.078%
23	4.730	1130	1132	1135	rBV2	1008	701	0.05%	0.006%
24	4.949	1197	1200	1201	rBV3	1053	575	0.04%	0.005%
25	5.071	1220	1238	1269	rBV2	513761	1338590	100.00%	12.411%
26	5.498	1367	1371	1372	rBV3	941	664	0.05%	0.006%
27	5.572	1392	1394	1399	rBV4	1055	777	0.06%	0.007%
28	5.640	1402	1415	1439	rBV	423190	848731	63.40%	7.869%
29	5.939	1500	1508	1523	rVB6	34849	72316	5.40%	0.670%
30	6.093	1543	1556	1583	rBV	297290	603048	45.05%	5.591%
31	6.643	1721	1727	1730	rBV7	2926	3580	0.27%	0.033%
32	6.756	1758	1762	1764	rBV4	1120	671	0.05%	0.006%
33	6.842	1786	1789	1792	rBV5	1979	1317	0.10%	0.012%
34	6.858	1792	1794	1798	rVB5	1202	759	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017210.D
 Acq On : 27 Jun 2020 03:30
 Operator : SY/MD
 Sample : L3132-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y28

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.920	1810	1813	1814	rBV3	1285	601	0.04%	0.006%
36	7.006	1830	1840	1863	rBV	163713	290766	21.72%	2.696%
37	7.338	1932	1943	1963	rBV	614225	1049692	78.42%	9.732%
38	7.592	2020	2022	2024	rBV4	1618	742	0.06%	0.007%
39	7.643	2027	2038	2056	rVV	116851	207306	15.49%	1.922%
40	7.997	2135	2148	2165	rBV	311655	528932	39.51%	4.904%
41	8.109	2173	2183	2209	rBV	304470	561070	41.92%	5.202%
42	8.559	2321	2323	2326	rVB3	1700	737	0.06%	0.007%
43	8.704	2364	2368	2370	rBV4	1484	975	0.07%	0.009%
44	8.804	2396	2399	2403	rVB5	1573	1022	0.08%	0.009%
45	8.833	2405	2408	2409	rBV3	1011	565	0.04%	0.005%
46	8.871	2409	2420	2440	rBV	637041	1041268	77.79%	9.654%
47	9.029	2467	2469	2473	rBV2	1505	829	0.06%	0.008%
48	9.077	2481	2484	2485	rBV2	1446	817	0.06%	0.008%
49	9.154	2506	2508	2511	rBV3	1271	808	0.06%	0.007%
50	9.315	2556	2558	2560	rBV3	1071	590	0.04%	0.005%
51	9.485	2608	2611	2612	rBV3	1262	753	0.06%	0.007%
52	9.511	2616	2619	2622	rBV4	1017	728	0.05%	0.007%
53	9.527	2622	2624	2627	rBV3	842	571	0.04%	0.005%
54	9.624	2652	2654	2658	rVB4	1490	828	0.06%	0.008%
55	9.681	2671	2672	2674	rBV	1019	520	0.04%	0.005%
56	9.797	2705	2708	2710	rBV3	1171	556	0.04%	0.005%
57	9.926	2746	2748	2750	rBV3	1020	618	0.05%	0.006%
58	10.022	2774	2778	2781	rVB3	1116	936	0.07%	0.009%
59	10.103	2799	2803	2805	rVB5	1238	721	0.05%	0.007%
60	10.122	2807	2809	2811	rBV3	1345	645	0.05%	0.006%
61	10.238	2833	2845	2857	rBV	384288	608114	45.43%	5.638%
62	10.392	2891	2893	2894	rBV2	1551	649	0.05%	0.006%
63	10.463	2913	2915	2918	rBV4	1088	801	0.06%	0.007%
64	10.530	2932	2936	2938	rBV3	1152	888	0.07%	0.008%
65	10.559	2941	2945	2947	rBV4	1727	1139	0.09%	0.011%
66	10.649	2968	2973	2975	rBV5	1719	1647	0.12%	0.015%
67	11.006	3082	3084	3090	rVB6	1703	1321	0.10%	0.012%
68	11.080	3102	3107	3111	rBV7	1849	1709	0.13%	0.016%
69	11.151	3124	3129	3133	rBV5	1492	1329	0.10%	0.012%
70	11.270	3153	3166	3183	rVV	637923	960834	71.78%	8.909%
71	11.456	3222	3224	3227	rVB4	1329	741	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017210.D
 Acq On : 27 Jun 2020 03:30
 Operator : SY/MD
 Sample : L3132-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y28

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.476	3227	3230	3232	rBV3	1153	637	0.05%	0.006%
73	11.498	3234	3237	3240	rBV4	1414	923	0.07%	0.009%
74	11.559	3250	3256	3260	rBV7	3148	4351	0.33%	0.040%
75	11.646	3272	3283	3303	rVV	632051	991380	74.06%	9.192%
76	11.784	3322	3326	3329	rBV4	1293	1266	0.09%	0.012%
77	11.900	3360	3362	3366	rBV3	900	570	0.04%	0.005%
78	11.916	3366	3367	3370	rVV3	1198	746	0.06%	0.007%
79	11.932	3370	3372	3375	rVV4	1711	1053	0.08%	0.010%
80	11.955	3375	3379	3383	rVB6	1601	1401	0.10%	0.013%
81	12.051	3407	3409	3410	rBV2	1135	521	0.04%	0.005%
82	12.154	3438	3441	3443	rBV4	983	590	0.04%	0.005%
83	12.312	3488	3490	3494	rVB3	1495	942	0.07%	0.009%
84	12.331	3494	3496	3501	rBV3	1316	1196	0.09%	0.011%
85	12.482	3541	3543	3548	rVB5	1008	580	0.04%	0.005%
86	12.697	3608	3610	3613	rBV3	1140	774	0.06%	0.007%
87	12.784	3635	3637	3640	rVB3	1480	701	0.05%	0.006%
88	12.804	3640	3643	3645	rBV4	1446	939	0.07%	0.009%
89	12.868	3661	3663	3665	rBV3	1082	640	0.05%	0.006%
90	12.897	3669	3672	3674	rBV4	1557	776	0.06%	0.007%
91	13.215	3769	3771	3775	rVB4	1259	774	0.06%	0.007%
92	13.276	3788	3790	3792	rBV2	999	592	0.04%	0.005%
93	13.437	3837	3840	3841	rBV3	1333	600	0.04%	0.006%
94	13.524	3864	3867	3868	rBV3	968	576	0.04%	0.005%
95	13.662	3907	3910	3912	rBV3	1148	697	0.05%	0.006%
96	14.305	4108	4110	4113	rVB3	1810	791	0.06%	0.007%
97	14.623	4207	4209	4212	rBV2	1484	709	0.05%	0.007%
98	14.877	4286	4288	4290	rBV3	1351	582	0.04%	0.005%
99	15.447	4461	4465	4467	rBV4	1691	1493	0.11%	0.014%
100	15.504	4480	4483	4486	rBV4	1382	722	0.05%	0.007%


Sum of corrected areas: 10785492

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017210.D
Acq On : 27 Jun 2020 03:30
Operator : SY/MD
Sample : L3132-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y28

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

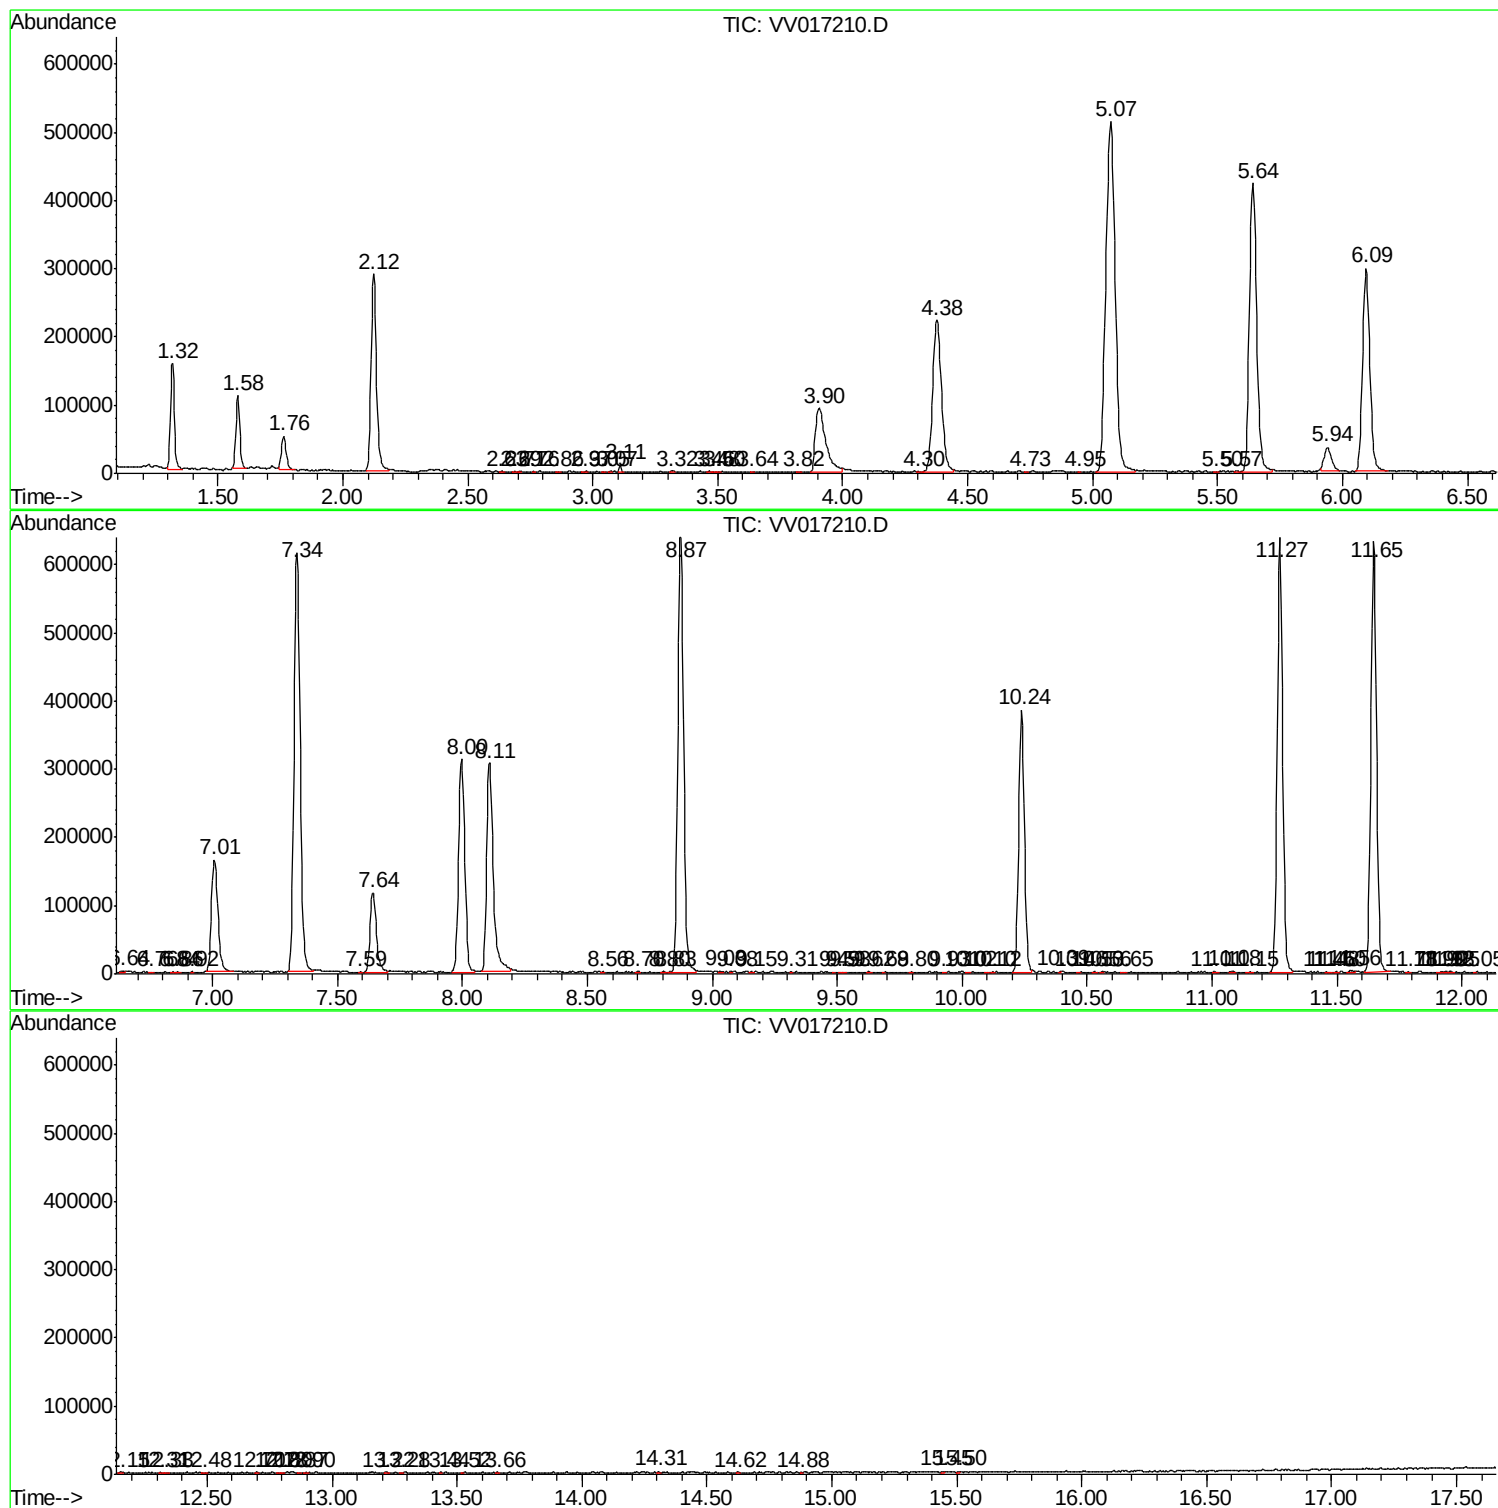

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017210.D
Acq On : 27 Jun 2020 03:30
Operator : SY/MD
Sample : L3132-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y28

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017210.D
Acq On : 27 Jun 2020 03:30
Operator : SY/MD
Sample : L3132-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y28

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc