

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017213.D
 Acq On : 27 Jun 2020 04:39
 Operator : SY/MD
 Sample : L3132-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	84	rVB	156596	161517	12.37%	1.438%
2	1.579	145	152	162	rBV	122236	136851	10.48%	1.219%
3	1.766	202	210	222	rVB	119446	160183	12.27%	1.426%
4	2.122	311	321	348	rBV	275538	421902	32.32%	3.757%
5	2.827	537	540	544	rBV3	1361	1440	0.11%	0.013%
6	2.939	571	575	577	rBV4	962	739	0.06%	0.007%
7	3.122	629	632	636	rBV4	994	773	0.06%	0.007%
8	3.164	640	645	648	rBV6	1187	1279	0.10%	0.011%
9	3.257	672	674	677	rBV3	1048	643	0.05%	0.006%
10	3.412	717	722	725	rBV5	1189	1482	0.11%	0.013%
11	3.508	745	752	753	rBV6	1373	1246	0.10%	0.011%
12	3.627	787	789	793	rVB4	1556	789	0.06%	0.007%
13	3.650	793	796	799	rBV2	1297	943	0.07%	0.008%
14	3.685	804	807	810	rBV4	964	720	0.06%	0.006%
15	3.756	827	829	832	rVB3	1263	720	0.06%	0.006%
16	3.775	832	835	838	rBV3	1019	903	0.07%	0.008%
17	3.804	841	844	850	rVB5	1108	1103	0.08%	0.010%
18	3.910	866	877	906	rBV	90055	261972	20.07%	2.333%
19	4.376	1005	1022	1042	rBV	216512	537337	41.16%	4.785%
20	4.618	1094	1097	1098	rBV3	1168	691	0.05%	0.006%
21	4.672	1111	1114	1118	rBV6	1685	1089	0.08%	0.010%
22	4.749	1134	1138	1143	rBV8	1515	1627	0.12%	0.014%
23	5.071	1219	1238	1265	rVV2	504482	1305348	100.00%	11.625%
24	5.640	1402	1415	1434	rBV	429276	841655	64.48%	7.495%
25	5.888	1490	1492	1494	rVV2	1662	772	0.06%	0.007%
26	5.936	1498	1507	1521	rVB9	16732	39883	3.06%	0.355%
27	6.093	1543	1556	1577	rBV	291478	581382	44.54%	5.177%
28	6.344	1632	1634	1635	rBV2	1599	748	0.06%	0.007%
29	6.415	1653	1656	1660	rBV5	985	1023	0.08%	0.009%
30	6.482	1676	1677	1682	rVB4	1103	657	0.05%	0.006%
31	6.515	1683	1687	1690	rVB5	1146	856	0.07%	0.008%
32	6.634	1720	1724	1728	rBV6	2011	2179	0.17%	0.019%
33	6.698	1741	1744	1745	rBV3	1497	830	0.06%	0.007%
34	6.826	1782	1784	1788	rVB3	1746	1064	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017213.D
 Acq On : 27 Jun 2020 04:39
 Operator : SY/MD
 Sample : L3132-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.846	1788	1790	1792	rBV2	1997	1026	0.08%	0.009%
36	7.010	1829	1841	1859	rBV	162417	291418	22.32%	2.595%
37	7.273	1921	1923	1928	rVB6	1994	1288	0.10%	0.011%
38	7.338	1928	1943	1963	rBV	604914	1036387	79.40%	9.229%
39	7.640	2028	2037	2055	rBV	115441	199487	15.28%	1.777%
40	7.797	2083	2086	2089	rBV5	1748	981	0.08%	0.009%
41	7.923	2123	2125	2128	rBV3	1096	711	0.05%	0.006%
42	7.997	2135	2148	2162	rBV	650353	1089331	83.45%	9.701%
43	8.106	2172	2182	2212	rBV	308932	560351	42.93%	4.990%
44	8.341	2253	2255	2258	rBV4	1443	729	0.06%	0.006%
45	8.405	2270	2275	2279	rBV7	1190	1371	0.11%	0.012%
46	8.479	2295	2298	2302	rBV4	1595	1366	0.10%	0.012%
47	8.588	2330	2332	2337	rVB5	1765	1137	0.09%	0.010%
48	8.614	2337	2340	2343	rBV3	1368	1006	0.08%	0.009%
49	8.653	2348	2352	2354	rBV3	1017	723	0.06%	0.006%
50	8.871	2408	2420	2444	rVV	623684	1016882	77.90%	9.056%
51	9.164	2508	2511	2515	rVB5	1143	754	0.06%	0.007%
52	9.280	2545	2547	2555	rVB8	1316	954	0.07%	0.008%
53	9.521	2618	2622	2624	rBV3	1198	915	0.07%	0.008%
54	9.630	2654	2656	2660	rBV3	1173	786	0.06%	0.007%
55	9.714	2679	2682	2684	rBV2	1155	813	0.06%	0.007%
56	9.836	2717	2720	2723	rBV5	1617	1187	0.09%	0.011%
57	10.071	2789	2793	2794	rBV3	979	808	0.06%	0.007%
58	10.125	2807	2810	2814	rVB4	963	834	0.06%	0.007%
59	10.193	2827	2831	2832	rBV3	1114	696	0.05%	0.006%
60	10.238	2834	2845	2863	rVB	377062	595191	45.60%	5.300%
61	10.325	2868	2872	2875	rBV5	1244	947	0.07%	0.008%
62	10.399	2889	2895	2896	rBV4	1601	1120	0.09%	0.010%
63	10.431	2902	2905	2908	rBV4	1539	1096	0.08%	0.010%
64	10.457	2910	2913	2915	rVV3	1227	802	0.06%	0.007%
65	10.469	2915	2917	2920	rVV4	1684	1157	0.09%	0.010%
66	10.511	2927	2930	2933	rBV3	1621	916	0.07%	0.008%
67	10.649	2970	2973	2976	rBV4	971	701	0.05%	0.006%
68	10.868	3038	3041	3042	rBV2	1813	1041	0.08%	0.009%
69	11.035	3092	3093	3097	rVB3	1115	624	0.05%	0.006%
70	11.157	3129	3131	3133	rBV3	1552	896	0.07%	0.008%
71	11.270	3153	3166	3185	rBV	612841	941452	72.12%	8.384%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017213.D
 Acq On : 27 Jun 2020 04:39
 Operator : SY/MD
 Sample : L3132-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.428	3213	3215	3220	rVB4	1234	747	0.06%	0.007%
73	11.450	3220	3222	3224	rBV3	1385	753	0.06%	0.007%
74	11.530	3245	3247	3249	rBV2	1205	651	0.05%	0.006%
75	11.646	3272	3283	3300	rVB	629535	971135	74.40%	8.648%
76	12.283	3476	3481	3484	rBV6	1778	1390	0.11%	0.012%
77	12.379	3509	3511	3513	rBV2	1420	806	0.06%	0.007%
78	12.399	3513	3517	3518	rVV2	1078	710	0.05%	0.006%
79	12.428	3523	3526	3530	rVV5	864	786	0.06%	0.007%
80	12.447	3530	3532	3535	rVB4	1446	662	0.05%	0.006%
81	12.521	3550	3555	3556	rBV3	1205	807	0.06%	0.007%
82	12.566	3567	3569	3573	rVB2	1152	628	0.05%	0.006%
83	12.739	3618	3623	3625	rBV5	1495	1088	0.08%	0.010%
84	12.810	3642	3645	3646	rBV3	1147	684	0.05%	0.006%
85	12.936	3682	3684	3687	rBV4	1106	730	0.06%	0.007%
86	12.952	3687	3689	3692	rVB3	1664	942	0.07%	0.008%
87	13.106	3735	3737	3742	rBV4	1312	1107	0.08%	0.010%
88	13.206	3764	3768	3770	rBV5	918	712	0.05%	0.006%
89	13.244	3778	3780	3783	rBV3	1240	651	0.05%	0.006%
90	13.427	3834	3837	3840	rBV4	1259	890	0.07%	0.008%
91	13.540	3867	3872	3876	rBV6	1817	1633	0.13%	0.015%
92	13.681	3914	3916	3919	rBV2	1099	696	0.05%	0.006%
93	13.997	4012	4014	4018	rBV5	1187	821	0.06%	0.007%
94	14.058	4027	4033	4036	rVB6	1730	1682	0.13%	0.015%
95	14.087	4036	4042	4045	rBV7	2128	2182	0.17%	0.019%
96	14.366	4124	4129	4133	rBV7	1433	1731	0.13%	0.015%
97	14.521	4173	4177	4180	rBV4	1354	1221	0.09%	0.011%
98	14.710	4233	4236	4237	rBV3	1248	768	0.06%	0.007%
99	14.816	4266	4269	4271	rBV3	1460	941	0.07%	0.008%
100	15.726	4549	4552	4557	rBV5	1943	1384	0.11%	0.012%


Sum of corrected areas: 11229168

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017213.D
Acq On : 27 Jun 2020 04:39
Operator : SY/MD
Sample : L3132-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y32

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

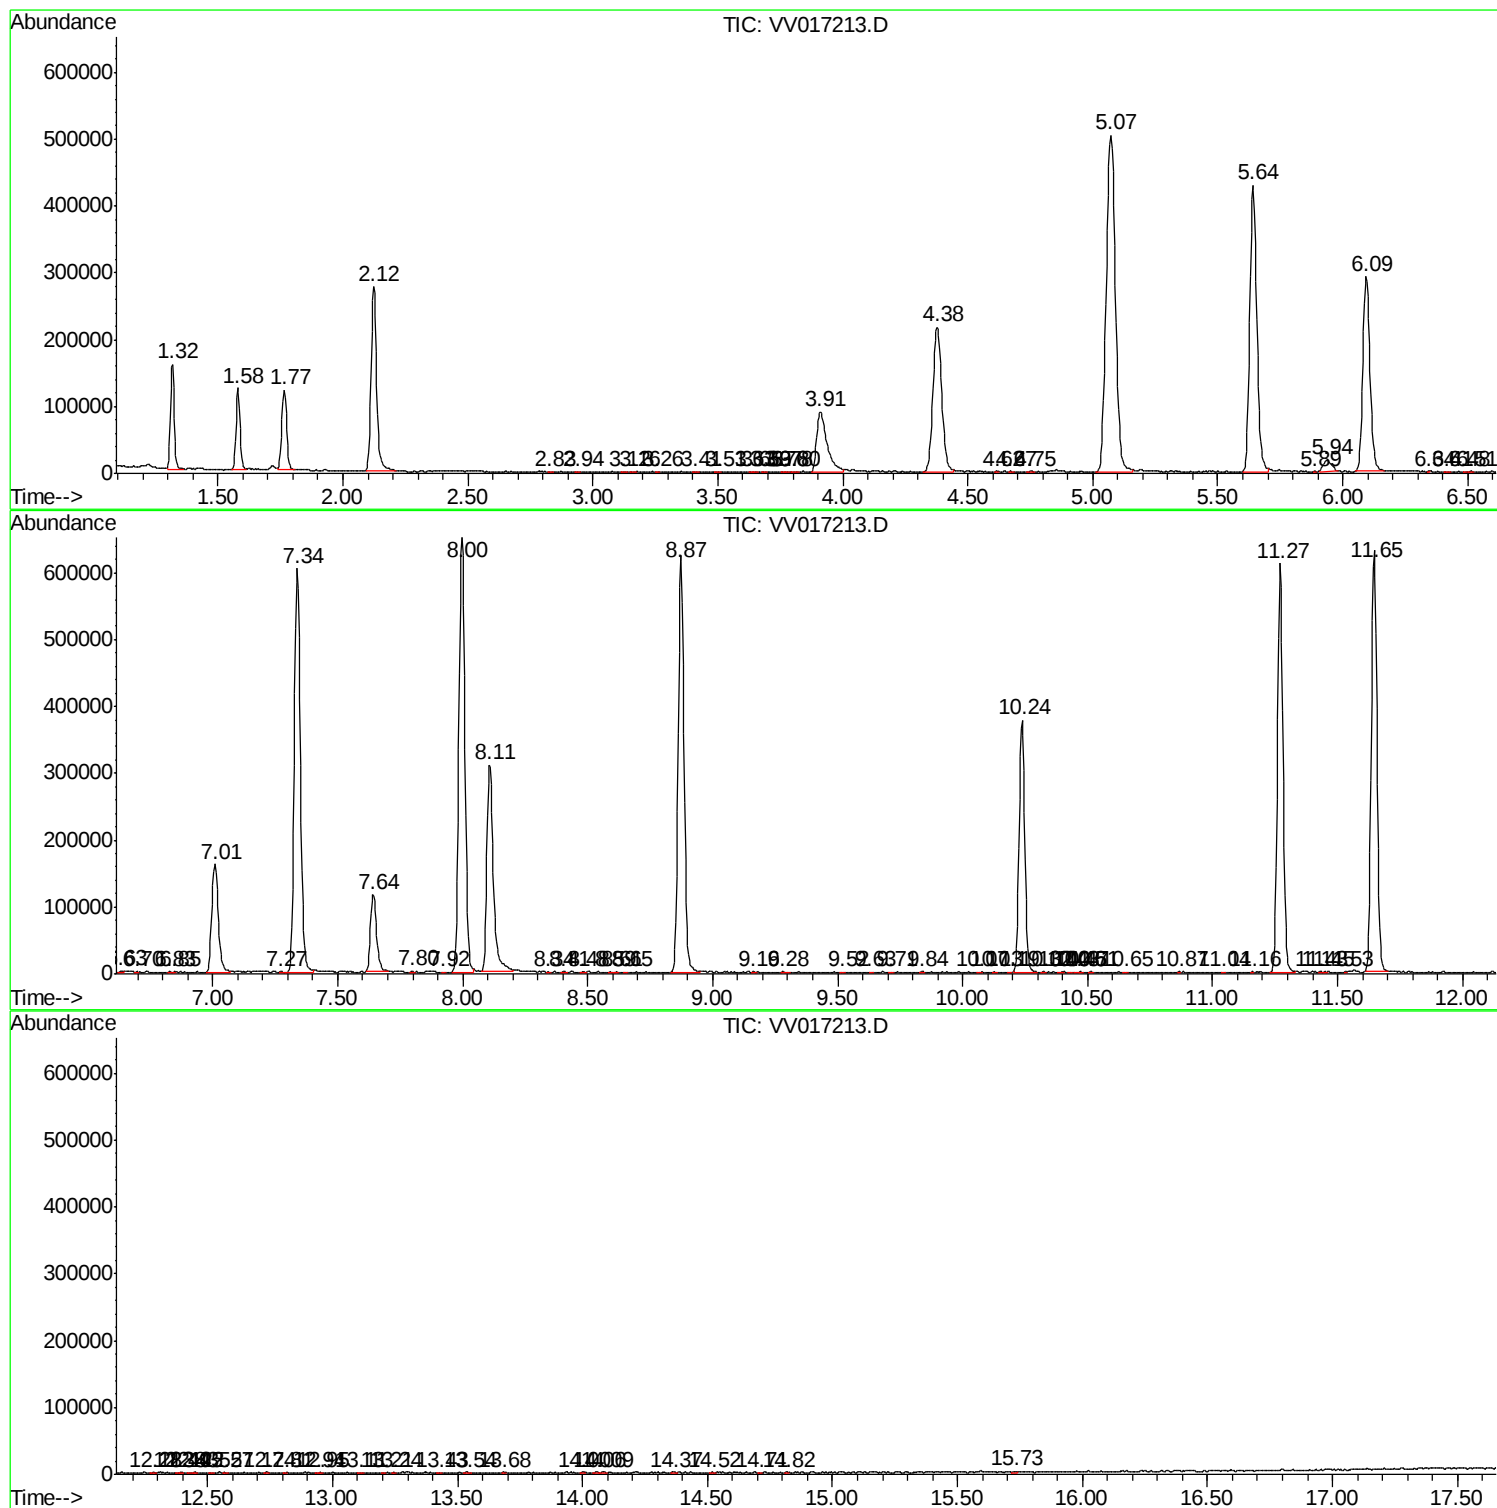

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017213.D
Acq On : 27 Jun 2020 04:39
Operator : SY/MD
Sample : L3132-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y32

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017213.D
Acq On : 27 Jun 2020 04:39
Operator : SY/MD
Sample : L3132-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y32

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc