

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017214.D
 Acq On : 27 Jun 2020 05:02
 Operator : SY/MD
 Sample : L3133-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	151744	156063	12.31%	1.521%
2	1.579	146	152	161	rVB	106081	112546	8.88%	1.097%
3	2.122	311	321	333	rBV	266024	399762	31.54%	3.896%
4	2.875	553	555	559	rBV4	1397	688	0.05%	0.007%
5	2.965	581	583	586	rBV4	834	553	0.04%	0.005%
6	3.068	612	615	619	rVB3	1179	789	0.06%	0.008%
7	3.135	633	636	638	rBV4	1210	717	0.06%	0.007%
8	3.200	653	656	658	rBV4	1260	910	0.07%	0.009%
9	3.312	688	691	692	rBV3	1530	974	0.08%	0.009%
10	3.495	744	748	752	rVV7	1364	1374	0.11%	0.013%
11	3.527	756	758	761	rBV3	917	590	0.05%	0.006%
12	3.585	773	776	778	rBV4	967	608	0.05%	0.006%
13	3.701	810	812	815	rVV3	1042	573	0.05%	0.006%
14	3.907	862	876	899	rBV	86987	247930	19.56%	2.416%
15	4.376	1006	1022	1049	rBV	215036	529415	41.77%	5.160%
16	4.582	1083	1086	1087	rBV3	1340	708	0.06%	0.007%
17	4.730	1130	1132	1137	rBV5	1268	924	0.07%	0.009%
18	4.984	1208	1211	1215	rBV4	1440	1111	0.09%	0.011%
19	5.074	1219	1239	1268	rVV2	486225	1267373	100.00%	12.353%
20	5.415	1340	1345	1346	rBV4	1750	1184	0.09%	0.012%
21	5.531	1376	1381	1382	rBV3	1581	1299	0.10%	0.013%
22	5.576	1393	1395	1398	rVB3	1613	732	0.06%	0.007%
23	5.640	1402	1415	1434	rBV	425732	851215	67.16%	8.296%
24	5.939	1497	1508	1526	rVB	218886	430322	33.95%	4.194%
25	6.093	1543	1556	1575	rBV2	281670	569133	44.91%	5.547%
26	6.460	1668	1670	1672	rBV4	957	582	0.05%	0.006%
27	6.508	1684	1685	1691	rVB5	1121	1036	0.08%	0.010%
28	6.540	1691	1695	1698	rBV4	1648	1381	0.11%	0.013%
29	7.006	1827	1840	1861	rBV	156358	283409	22.36%	2.762%
30	7.148	1881	1884	1886	rBV3	1461	974	0.08%	0.009%
31	7.215	1901	1905	1906	rBV3	1463	1062	0.08%	0.010%
32	7.283	1922	1926	1930	rBV7	1199	1243	0.10%	0.012%
33	7.338	1931	1943	1962	rBV	585924	1005390	79.33%	9.799%
34	7.640	2025	2037	2054	rBV	114225	198707	15.68%	1.937%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017214.D
 Acq On : 27 Jun 2020 05:02
 Operator : SY/MD
 Sample : L3133-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.926	2123	2126	2128	rBV4	904	739	0.06%	0.007%
36	7.994	2143	2147	2149	rBV5	2154	1920	0.15%	0.019%
37	8.064	2166	2169	2172	rBV3	1271	777	0.06%	0.008%
38	8.106	2172	2182	2216	rBV	295988	544950	43.00%	5.311%
39	8.498	2300	2304	2306	rBV4	1610	1225	0.10%	0.012%
40	8.765	2383	2387	2389	rBV4	1284	732	0.06%	0.007%
41	8.871	2406	2420	2441	rBV	636264	1040938	82.13%	10.146%
42	9.305	2552	2555	2558	rBV4	963	637	0.05%	0.006%
43	9.321	2558	2560	2564	rVB4	1094	573	0.05%	0.006%
44	9.428	2590	2593	2595	rBV3	1100	687	0.05%	0.007%
45	9.682	2669	2672	2676	rBV4	1311	1089	0.09%	0.011%
46	9.720	2683	2684	2690	rVB6	881	623	0.05%	0.006%
47	9.759	2692	2696	2697	rBV3	1626	982	0.08%	0.010%
48	9.923	2743	2747	2751	rBV8	1850	1777	0.14%	0.017%
49	10.074	2791	2794	2798	rBV4	872	700	0.06%	0.007%
50	10.238	2832	2845	2862	rBV	372728	585447	46.19%	5.706%
51	10.299	2862	2864	2866	rBV3	1318	709	0.06%	0.007%
52	10.405	2890	2897	2898	rBV5	1970	1736	0.14%	0.017%
53	10.665	2975	2978	2982	rBV5	1345	1214	0.10%	0.012%
54	10.717	2991	2994	2999	rBV6	1469	1325	0.10%	0.013%
55	10.826	3024	3028	3030	rBV4	1459	871	0.07%	0.008%
56	10.842	3030	3033	3035	rVB4	1084	573	0.05%	0.006%
57	10.936	3059	3062	3063	rBV2	1081	605	0.05%	0.006%
58	10.974	3070	3074	3076	rBV4	1758	1185	0.09%	0.012%
59	11.071	3102	3104	3110	rVB5	1147	882	0.07%	0.009%
60	11.135	3122	3124	3126	rBV3	1262	770	0.06%	0.008%
61	11.219	3148	3150	3154	rVB3	919	565	0.04%	0.006%
62	11.270	3154	3166	3182	rBV	637422	969820	76.52%	9.452%
63	11.360	3192	3194	3198	rBV3	1358	1173	0.09%	0.011%
64	11.556	3246	3255	3267	rBV3	13728	28511	2.25%	0.278%
65	11.646	3271	3283	3300	rVV	614931	959725	75.73%	9.354%
66	11.997	3389	3392	3394	rBV3	1148	895	0.07%	0.009%
67	12.029	3398	3402	3409	rVB10	2143	2565	0.20%	0.025%
68	12.058	3409	3411	3414	rBV4	1244	783	0.06%	0.008%
69	12.074	3414	3416	3420	rVB3	1235	830	0.07%	0.008%
70	12.096	3420	3423	3427	rBV4	1512	1279	0.10%	0.012%
71	12.132	3431	3434	3436	rBV4	1046	708	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017214.D
 Acq On : 27 Jun 2020 05:02
 Operator : SY/MD
 Sample : L3133-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.183	3444	3450	3451	rBV4	1529	1296	0.10%	0.013%
73	12.276	3477	3479	3483	rVB4	1806	1019	0.08%	0.010%
74	12.656	3594	3597	3600	rBV4	1429	894	0.07%	0.009%
75	12.807	3641	3644	3645	rBV3	1455	756	0.06%	0.007%
76	12.890	3668	3670	3672	rBV3	1093	598	0.05%	0.006%
77	12.926	3679	3681	3685	rBV3	904	579	0.05%	0.006%
78	13.054	3719	3721	3725	rVB3	880	630	0.05%	0.006%
79	13.109	3735	3738	3741	rBV2	1289	1189	0.09%	0.012%
80	13.305	3796	3799	3803	rBV4	1376	1003	0.08%	0.010%
81	13.325	3803	3805	3808	rBV3	1155	830	0.07%	0.008%
82	13.398	3825	3828	3831	rBV3	960	561	0.04%	0.005%
83	13.553	3874	3876	3880	rVB3	1385	747	0.06%	0.007%
84	13.620	3894	3897	3899	rBV4	1590	880	0.07%	0.009%
85	13.759	3936	3940	3942	rBV3	1399	1157	0.09%	0.011%
86	13.797	3949	3952	3955	rBV3	876	657	0.05%	0.006%
87	13.948	3995	3999	4001	rBV3	912	758	0.06%	0.007%
88	13.980	4007	4009	4013	rBV4	1509	926	0.07%	0.009%
89	14.025	4021	4023	4026	rVV3	1786	787	0.06%	0.008%
90	14.067	4032	4036	4041	rBV6	1419	1409	0.11%	0.014%
91	14.148	4056	4061	4062	rBV3	1075	889	0.07%	0.009%
92	14.260	4094	4096	4098	rBV4	1286	703	0.06%	0.007%
93	14.800	4261	4264	4266	rBV3	1498	1155	0.09%	0.011%
94	14.919	4299	4301	4303	rBV3	1366	584	0.05%	0.006%
95	15.087	4351	4353	4357	rBV3	1752	1320	0.10%	0.013%
96	15.141	4368	4370	4374	rBV4	1310	786	0.06%	0.008%
97	15.205	4386	4390	4393	rBV4	1367	1349	0.11%	0.013%
98	15.643	4524	4526	4528	rBV3	1409	682	0.05%	0.007%
99	15.681	4533	4538	4540	rBV3	2391	2052	0.16%	0.020%
100	15.884	4597	4601	4603	rBV4	2443	2028	0.16%	0.020%


Sum of corrected areas: 10260021

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017214.D
Acq On : 27 Jun 2020 05:02
Operator : SY/MD
Sample : L3133-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

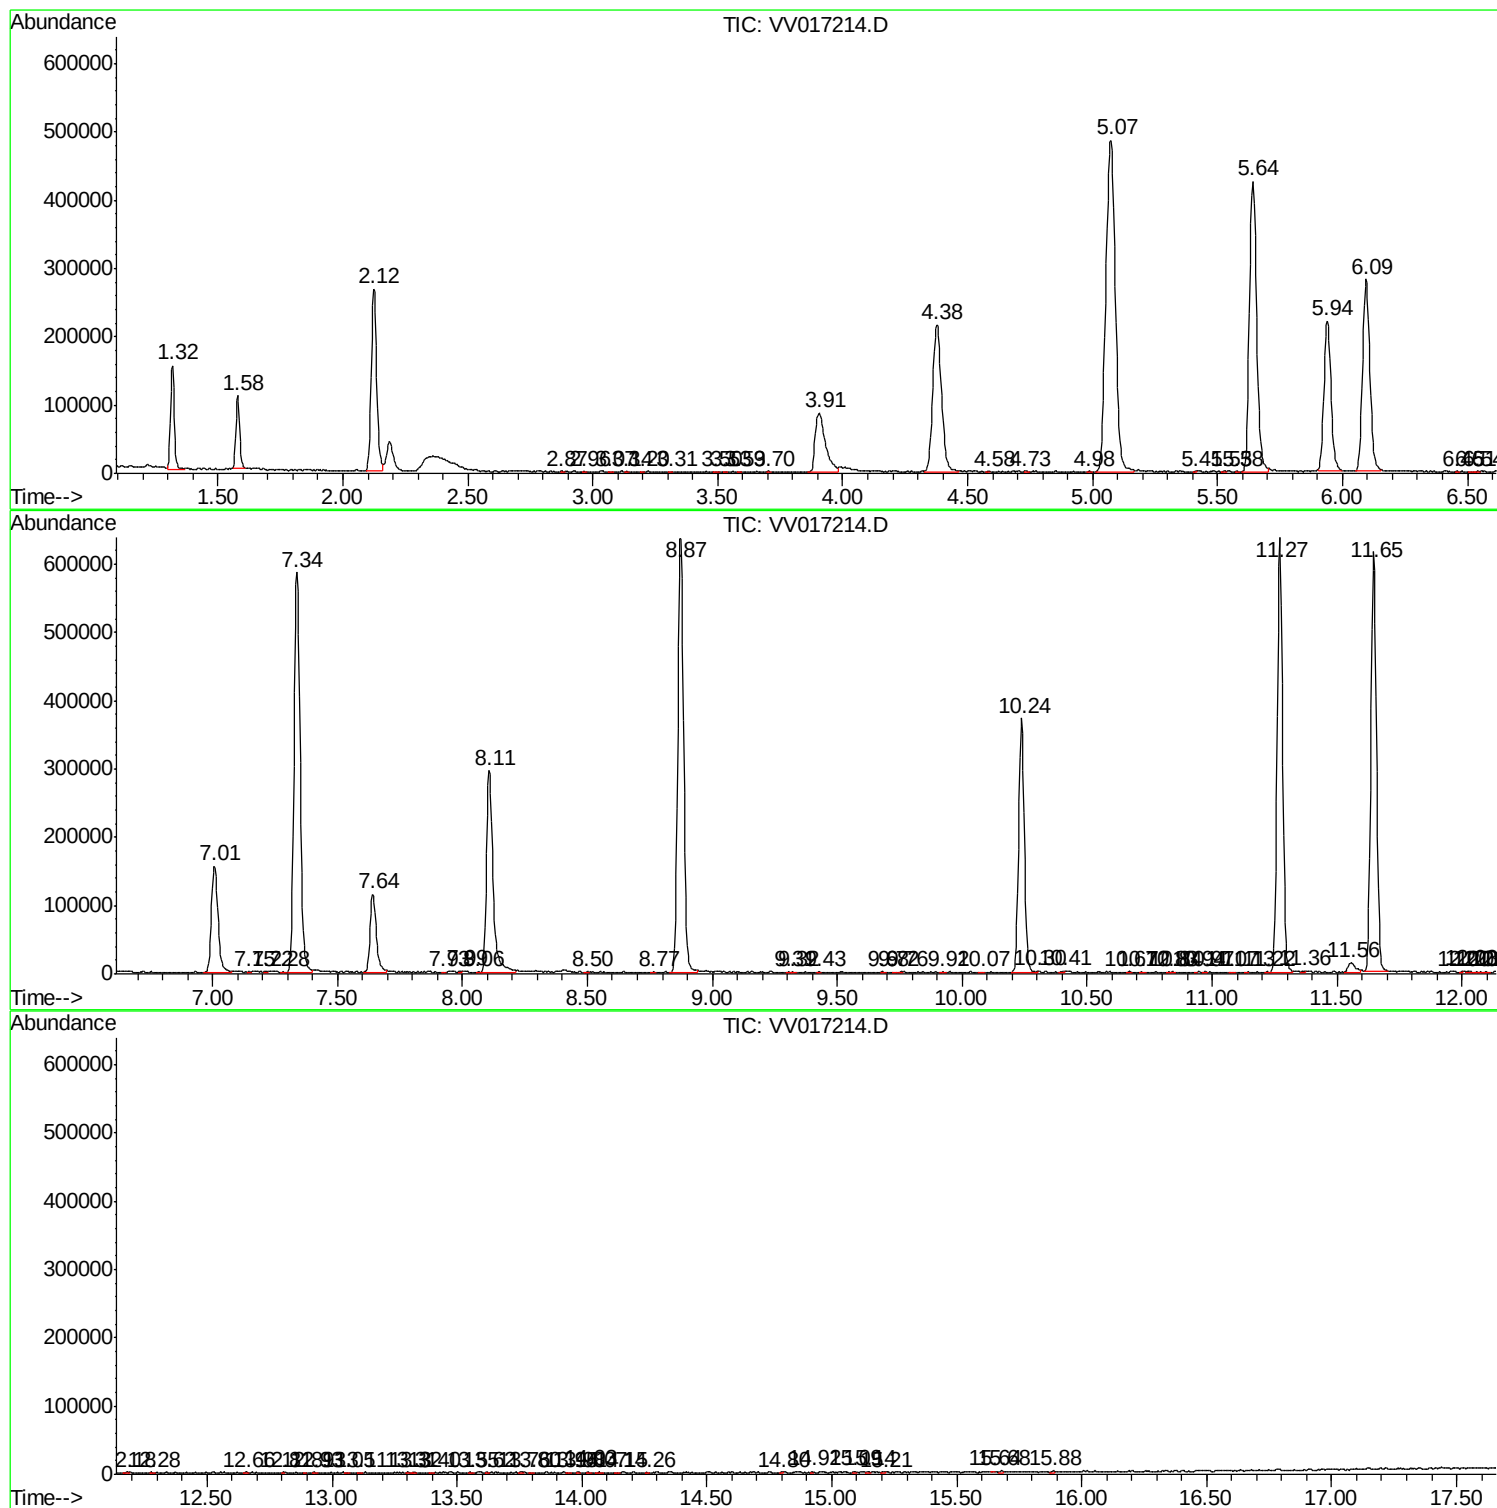

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017214.D
Acq On : 27 Jun 2020 05:02
Operator : SY/MD
Sample : L3133-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017214.D
Acq On : 27 Jun 2020 05:02
Operator : SY/MD
Sample : L3133-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q24

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc