

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017215.D
 Acq On : 27 Jun 2020 05:26
 Operator : SY/MD
 Sample : L3133-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	81	rVB	157603	159769	11.90%	1.488%
2	1.579	145	152	163	rBV	118449	128201	9.55%	1.194%
3	2.122	312	321	332	rBV	281562	422056	31.43%	3.932%
4	2.859	548	550	554	rBV5	1194	624	0.05%	0.006%
5	2.884	554	558	563	rVB7	1485	1258	0.09%	0.012%
6	2.962	575	582	587	rBV7	1353	1938	0.14%	0.018%
7	3.161	641	644	648	rBV3	677	596	0.04%	0.006%
8	3.209	653	659	660	rBV5	1306	1056	0.08%	0.010%
9	3.222	660	663	664	rBV3	1018	576	0.04%	0.005%
10	3.270	674	678	681	rBV3	1369	1182	0.09%	0.011%
11	3.319	681	693	702	rVV7	5345	11993	0.89%	0.112%
12	3.441	728	731	733	rBV3	873	571	0.04%	0.005%
13	3.611	781	784	785	rBV2	1011	540	0.04%	0.005%
14	3.701	810	812	815	rBV4	1016	645	0.05%	0.006%
15	3.907	864	876	904	rBV3	97939	366510	27.30%	3.414%
16	4.126	941	944	946	rBV4	1615	1047	0.08%	0.010%
17	4.376	1008	1022	1045	rVB	226891	552946	41.18%	5.151%
18	4.695	1115	1121	1127	rVB9	1770	2324	0.17%	0.022%
19	4.765	1140	1143	1145	rBV3	888	647	0.05%	0.006%
20	4.820	1157	1160	1163	rBV4	895	563	0.04%	0.005%
21	4.846	1166	1168	1169	rBV2	1185	548	0.04%	0.005%
22	4.900	1180	1185	1187	rBV3	1337	1093	0.08%	0.010%
23	4.942	1194	1198	1203	rBB7	1008	994	0.07%	0.009%
24	4.965	1203	1205	1212	rBV7	1123	959	0.07%	0.009%
25	5.074	1222	1239	1266	rBV2	523087	1342649	100.00%	12.508%
26	5.534	1379	1382	1386	rBV3	2315	1928	0.14%	0.018%
27	5.640	1403	1415	1438	rBV	426261	849376	63.26%	7.913%
28	5.939	1494	1508	1528	rBV	203881	406783	30.30%	3.790%
29	6.093	1544	1556	1576	rBV	300250	601758	44.82%	5.606%
30	6.318	1624	1626	1631	rVB4	1497	978	0.07%	0.009%
31	6.479	1674	1676	1679	rVB3	1434	725	0.05%	0.007%
32	6.605	1713	1715	1718	rBV4	1520	769	0.06%	0.007%
33	6.798	1773	1775	1779	rBV4	1465	699	0.05%	0.007%
34	6.920	1810	1813	1815	rBV3	1462	1129	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017215.D
 Acq On : 27 Jun 2020 05:26
 Operator : SY/MD
 Sample : L3133-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.007	1829	1840	1857	rBV	168993	298840	22.26%	2.784%
36	7.280	1923	1925	1929	rVB4	1755	1070	0.08%	0.010%
37	7.338	1931	1943	1963	rBV	624885	1069251	79.64%	9.961%
38	7.576	2014	2017	2018	rBV2	1483	707	0.05%	0.007%
39	7.643	2028	2038	2055	rBV2	119530	202748	15.10%	1.889%
40	7.839	2097	2099	2103	rVB4	1549	833	0.06%	0.008%
41	7.875	2108	2110	2113	rVV3	1272	606	0.05%	0.006%
42	7.945	2129	2132	2134	rBV3	1097	745	0.06%	0.007%
43	7.997	2146	2148	2153	rBV3	1132	942	0.07%	0.009%
44	8.106	2172	2182	2200	rBV	321583	565738	42.14%	5.270%
45	8.871	2407	2420	2443	rBV	631334	1037468	77.27%	9.665%
46	9.312	2552	2557	2558	rBV3	1203	936	0.07%	0.009%
47	9.473	2602	2607	2608	rBV2	1009	805	0.06%	0.007%
48	9.566	2633	2636	2640	rVB4	1017	698	0.05%	0.007%
49	9.675	2666	2670	2673	rBV3	1104	980	0.07%	0.009%
50	9.730	2685	2687	2689	rVB	1367	654	0.05%	0.006%
51	9.900	2738	2740	2742	rBV3	956	551	0.04%	0.005%
52	9.984	2764	2766	2770	rBV4	1197	652	0.05%	0.006%
53	10.238	2833	2845	2861	rBV	396998	619392	46.13%	5.770%
54	10.331	2871	2874	2877	rVB5	1164	826	0.06%	0.008%
55	10.383	2889	2890	2893	rBV3	1424	610	0.05%	0.006%
56	10.434	2904	2906	2908	rBV2	1304	654	0.05%	0.006%
57	10.463	2913	2915	2917	rVB3	1814	711	0.05%	0.007%
58	10.482	2917	2921	2925	rBV7	1364	1457	0.11%	0.014%
59	10.582	2950	2952	2955	rBV3	1838	1174	0.09%	0.011%
60	10.598	2955	2957	2959	rBV3	1274	680	0.05%	0.006%
61	10.807	3020	3022	3026	rVB4	883	632	0.05%	0.006%
62	10.829	3026	3029	3031	rBV2	1052	675	0.05%	0.006%
63	10.929	3057	3060	3063	rVB3	1594	1096	0.08%	0.010%
64	10.952	3063	3067	3070	rBV5	1225	1172	0.09%	0.011%
65	10.968	3070	3072	3076	rVV3	895	606	0.05%	0.006%
66	11.010	3081	3085	3086	rBV4	943	609	0.05%	0.006%
67	11.270	3155	3166	3191	rVB	634112	965110	71.88%	8.991%
68	11.453	3222	3223	3228	rBV5	1565	949	0.07%	0.009%
69	11.511	3239	3241	3245	rVB5	1048	584	0.04%	0.005%
70	11.553	3245	3254	3270	rBV4	17089	36687	2.73%	0.342%
71	11.646	3271	3283	3302	rVB	661370	1025200	76.36%	9.551%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017215.D
 Acq On : 27 Jun 2020 05:26
 Operator : SY/MD
 Sample : L3133-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.797	3327	3330	3333	rBV5	1267	969	0.07%	0.009%
73	12.058	3409	3411	3413	rBV2	1199	551	0.04%	0.005%
74	12.193	3451	3453	3458	rBV4	999	1009	0.08%	0.009%
75	12.270	3473	3477	3478	rBV4	1290	1171	0.09%	0.011%
76	12.354	3501	3503	3505	rBV2	1563	676	0.05%	0.006%
77	12.505	3548	3550	3553	rVB4	1497	796	0.06%	0.007%
78	12.649	3593	3595	3598	rBV3	1118	543	0.04%	0.005%
79	12.669	3599	3601	3605	rVB3	997	612	0.05%	0.006%
80	12.694	3605	3609	3613	rBV6	2197	1578	0.12%	0.015%
81	12.887	3667	3669	3673	rBV4	1887	1346	0.10%	0.013%
82	13.164	3753	3755	3759	rVB5	1293	541	0.04%	0.005%
83	13.392	3824	3826	3830	rVB5	1551	930	0.07%	0.009%
84	13.418	3830	3834	3837	rBV4	1666	1349	0.10%	0.013%
85	13.524	3865	3867	3869	rVB4	1220	558	0.04%	0.005%
86	13.550	3869	3875	3876	rBV5	1568	1081	0.08%	0.010%
87	13.685	3915	3917	3919	rBV3	1228	697	0.05%	0.006%
88	13.810	3953	3956	3957	rBV3	1138	572	0.04%	0.005%
89	13.987	4008	4011	4013	rBV4	1246	706	0.05%	0.007%
90	14.083	4036	4041	4042	rBV4	886	702	0.05%	0.007%
91	14.157	4059	4064	4066	rBV3	1365	1115	0.08%	0.010%
92	14.347	4121	4123	4126	rVB2	1067	532	0.04%	0.005%
93	14.376	4128	4132	4133	rBV4	1648	1079	0.08%	0.010%
94	14.517	4174	4176	4181	rBV4	948	679	0.05%	0.006%
95	14.646	4210	4216	4218	rBV5	1766	1641	0.12%	0.015%
96	14.681	4224	4227	4228	rBV2	1585	814	0.06%	0.008%
97	14.723	4238	4240	4243	rBV4	1044	719	0.05%	0.007%
98	14.778	4254	4257	4259	rBV4	1185	677	0.05%	0.006%
99	14.955	4310	4312	4315	rBV4	1244	870	0.06%	0.008%
100	15.228	4394	4397	4400	rBV4	1738	1129	0.08%	0.011%


Sum of corrected areas: 10734120

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017215.D
Acq On : 27 Jun 2020 05:26
Operator : SY/MD
Sample : L3133-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

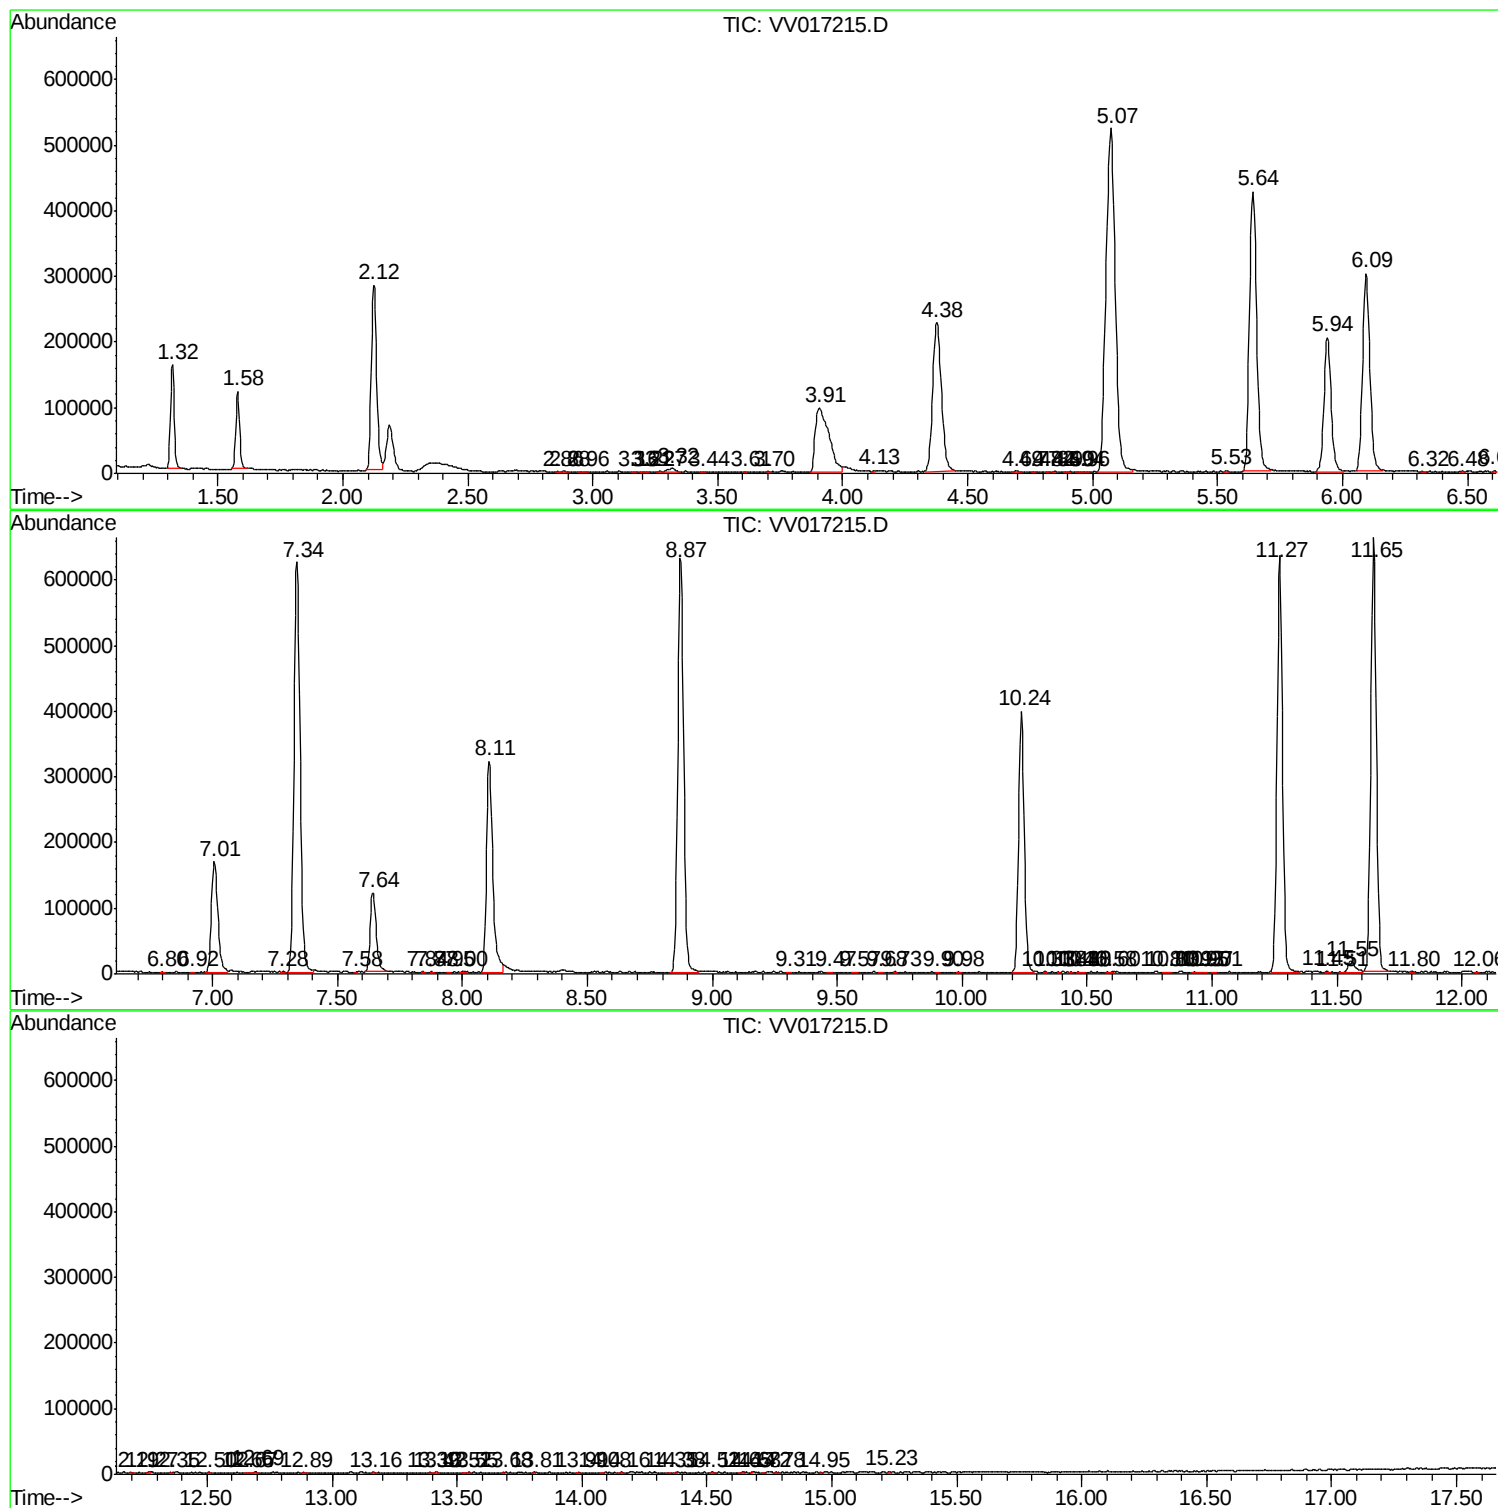

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017215.D
Acq On : 27 Jun 2020 05:26
Operator : SY/MD
Sample : L3133-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017215.D
Acq On : 27 Jun 2020 05:26
Operator : SY/MD
Sample : L3133-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q25

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc