

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017216.D
 Acq On : 27 Jun 2020 05:49
 Operator : SY/MD
 Sample : L3133-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	85	rVB	156445	164789	12.37%	1.527%
2	1.579	145	152	163	rBV	111698	122347	9.18%	1.134%
3	2.123	311	321	333	rBV	283821	418381	31.41%	3.877%
4	2.280	367	370	373	rBV5	1872	1539	0.12%	0.014%
5	3.049	604	609	611	rBV3	1565	1366	0.10%	0.013%
6	3.180	647	650	653	rBV3	1053	702	0.05%	0.007%
7	3.193	653	654	658	rBV3	1062	715	0.05%	0.007%
8	3.238	664	668	671	rBV5	1161	816	0.06%	0.008%
9	3.303	679	688	689	rBV7	4408	4509	0.34%	0.042%
10	3.367	705	708	709	rBV3	1303	628	0.05%	0.006%
11	3.415	720	723	728	rVB7	1286	1229	0.09%	0.011%
12	3.508	747	752	754	rBV4	918	781	0.06%	0.007%
13	3.676	801	804	808	rBV5	1337	1368	0.10%	0.013%
14	3.820	845	849	853	rVB4	1564	1110	0.08%	0.010%
15	3.907	861	876	904	rBV3	95549	397735	29.86%	3.685%
16	4.290	993	995	998	rBV3	1318	793	0.06%	0.007%
17	4.376	1008	1022	1045	rVB	227733	554692	41.64%	5.140%
18	4.569	1080	1082	1085	rBV3	1251	612	0.05%	0.006%
19	4.669	1111	1113	1117	rBV4	1317	931	0.07%	0.009%
20	4.769	1142	1144	1148	rBV3	884	625	0.05%	0.006%
21	4.823	1157	1161	1162	rBV3	1059	664	0.05%	0.006%
22	4.923	1189	1192	1195	rBV4	1272	830	0.06%	0.008%
23	4.955	1199	1202	1204	rBV3	1378	859	0.06%	0.008%
24	5.071	1220	1238	1267	rBV3	517520	1332110	100.00%	12.343%
25	5.508	1373	1374	1381	rVB6	1584	1110	0.08%	0.010%
26	5.640	1402	1415	1438	rBV	426365	848641	63.71%	7.863%
27	5.939	1495	1508	1526	rBV3	268936	537440	40.35%	4.980%
28	6.093	1544	1556	1575	rVB	293770	585438	43.95%	5.424%
29	6.537	1690	1694	1697	rBV3	1647	1528	0.11%	0.014%
30	6.698	1742	1744	1750	rVB6	1717	1503	0.11%	0.014%
31	6.830	1779	1785	1787	rBV8	1425	1221	0.09%	0.011%
32	6.875	1794	1799	1802	rBV7	1286	1240	0.09%	0.011%
33	7.007	1829	1840	1856	rBV2	164424	295686	22.20%	2.740%
34	7.338	1931	1943	1962	rBV	617754	1053609	79.09%	9.762%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017216.D
 Acq On : 27 Jun 2020 05:49
 Operator : SY/MD
 Sample : L3133-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.640	2027	2037	2058	rBV	121996	209465	15.72%	1.941%
36	8.109	2173	2183	2208	rBV	308931	569818	42.78%	5.280%
37	8.704	2365	2368	2372	rBV4	718	645	0.05%	0.006%
38	8.727	2373	2375	2380	rVB4	1634	1193	0.09%	0.011%
39	8.749	2380	2382	2384	rBV3	1201	622	0.05%	0.006%
40	8.807	2397	2400	2402	rBV3	1381	1014	0.08%	0.009%
41	8.871	2407	2420	2442	rBV	638521	1037971	77.92%	9.617%
42	9.042	2471	2473	2476	rBV4	1316	752	0.06%	0.007%
43	9.097	2488	2490	2494	rBV5	861	634	0.05%	0.006%
44	9.460	2600	2603	2605	rBV3	893	644	0.05%	0.006%
45	9.521	2619	2622	2627	rBV5	826	622	0.05%	0.006%
46	9.688	2672	2674	2678	rVB4	1393	938	0.07%	0.009%
47	9.717	2678	2683	2685	rBV4	857	771	0.06%	0.007%
48	9.769	2694	2699	2702	rBV4	1564	1204	0.09%	0.011%
49	9.887	2732	2736	2740	rVB4	1317	1024	0.08%	0.009%
50	9.913	2740	2744	2746	rBV6	1358	1063	0.08%	0.010%
51	10.132	2808	2812	2817	rVB6	1128	1147	0.09%	0.011%
52	10.187	2825	2829	2832	rBV4	1436	1106	0.08%	0.010%
53	10.238	2832	2845	2860	rBV	390410	614678	46.14%	5.695%
54	10.486	2917	2922	2927	rBV7	1422	1744	0.13%	0.016%
55	10.585	2951	2953	2955	rBV4	1433	723	0.05%	0.007%
56	10.868	3037	3041	3044	rBV5	1229	1049	0.08%	0.010%
57	10.884	3044	3046	3051	rVB4	2315	1540	0.12%	0.014%
58	10.968	3071	3072	3075	rVB3	1444	680	0.05%	0.006%
59	11.170	3132	3135	3137	rBV3	1054	891	0.07%	0.008%
60	11.270	3154	3166	3181	rBV	617186	945513	70.98%	8.761%
61	11.556	3245	3255	3269	rBV5	11626	25702	1.93%	0.238%
62	11.646	3272	3283	3299	rVB	634437	992030	74.47%	9.192%
63	11.775	3320	3323	3325	rBV4	1422	975	0.07%	0.009%
64	11.826	3333	3339	3340	rBV6	1641	1540	0.12%	0.014%
65	11.949	3375	3377	3381	rBV4	888	658	0.05%	0.006%
66	12.003	3390	3394	3396	rBV5	2283	1771	0.13%	0.016%
67	12.183	3447	3450	3454	rVB6	1181	922	0.07%	0.009%
68	12.203	3454	3456	3460	rBV5	874	707	0.05%	0.007%
69	12.244	3466	3469	3471	rVB3	1347	706	0.05%	0.007%
70	12.428	3524	3526	3530	rVB3	1740	1174	0.09%	0.011%
71	12.469	3535	3539	3540	rBV3	1183	915	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017216.D
 Acq On : 27 Jun 2020 05:49
 Operator : SY/MD
 Sample : L3133-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.566	3564	3569	3575	rBV7	1391	1553	0.12%	0.014%
73	12.653	3593	3596	3598	rBV3	1014	611	0.05%	0.006%
74	12.813	3640	3646	3651	rBV7	1674	2140	0.16%	0.020%
75	12.871	3662	3664	3667	rBV3	1035	671	0.05%	0.006%
76	13.022	3709	3711	3715	rBV4	1446	1263	0.09%	0.012%
77	13.087	3728	3731	3732	rBV3	1163	698	0.05%	0.006%
78	13.241	3774	3779	3782	rBV6	2140	1704	0.13%	0.016%
79	13.315	3799	3802	3803	rBV3	1781	997	0.07%	0.009%
80	13.395	3824	3827	3831	rVB6	1150	881	0.07%	0.008%
81	13.415	3831	3833	3838	rBV4	1909	1685	0.13%	0.016%
82	13.476	3848	3852	3855	rBV5	1628	1305	0.10%	0.012%
83	13.624	3894	3898	3900	rBV3	1142	856	0.06%	0.008%
84	13.829	3956	3962	3965	rVB7	1200	1077	0.08%	0.010%
85	13.852	3965	3969	3972	rBV4	1520	1375	0.10%	0.013%
86	13.868	3972	3974	3982	rVB7	1765	1700	0.13%	0.016%
87	13.900	3982	3984	3987	rBV3	1312	838	0.06%	0.008%
88	13.939	3994	3996	4001	rVB5	1858	1359	0.10%	0.013%
89	13.968	4003	4005	4008	rVV4	969	617	0.05%	0.006%
90	14.022	4019	4022	4024	rBV3	1169	653	0.05%	0.006%
91	14.466	4159	4160	4164	rBV4	1010	688	0.05%	0.006%
92	14.521	4175	4177	4179	rBV2	1213	725	0.05%	0.007%
93	14.649	4215	4217	4222	rVB4	1140	924	0.07%	0.009%
94	14.730	4239	4242	4243	rBV2	1297	662	0.05%	0.006%
95	14.868	4283	4285	4287	rBV3	1558	657	0.05%	0.006%
96	14.907	4294	4297	4299	rBV4	1299	862	0.06%	0.008%
97	15.077	4346	4350	4352	rBV4	1723	1195	0.09%	0.011%
98	15.299	4417	4419	4421	rBV2	1298	659	0.05%	0.006%
99	15.546	4493	4496	4497	rBV2	1374	845	0.06%	0.008%
100	15.620	4517	4519	4523	rBV5	1523	1285	0.10%	0.012%


Sum of corrected areas: 10792583

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017216.D
Acq On : 27 Jun 2020 05:49
Operator : SY/MD
Sample : L3133-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

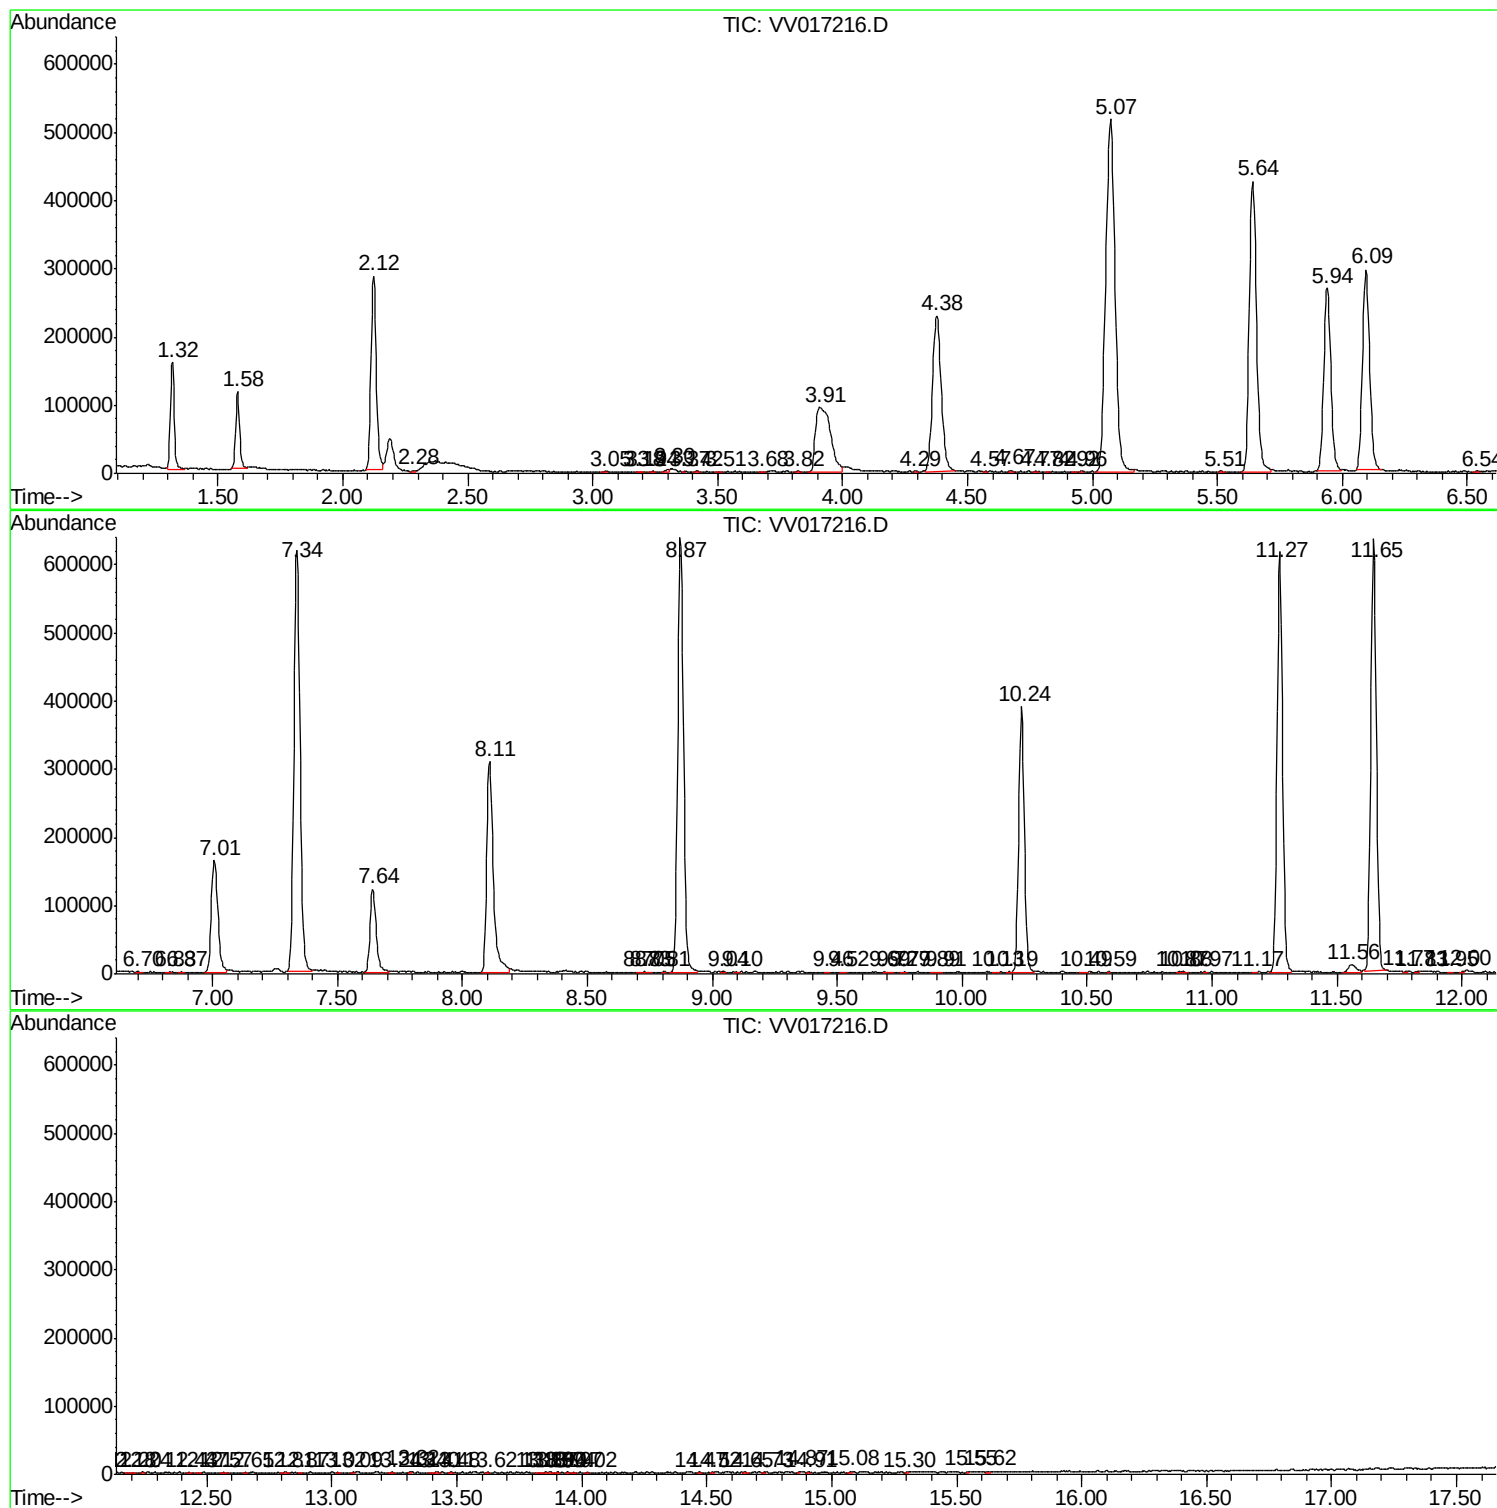

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017216.D
Acq On : 27 Jun 2020 05:49
Operator : SY/MD
Sample : L3133-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017216.D
Acq On : 27 Jun 2020 05:49
Operator : SY/MD
Sample : L3133-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc