

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017217.D
 Acq On : 27 Jun 2020 06:12
 Operator : SY/MD
 Sample : L3133-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	81	rVB	144487	152753	11.99%	1.508%
2	1.579	146	152	163	rVB	113621	121494	9.54%	1.199%
3	2.122	312	321	334	rBV	266189	396700	31.14%	3.916%
4	2.926	566	571	575	rBV6	1751	1932	0.15%	0.019%
5	3.126	631	633	635	rBV3	957	659	0.05%	0.007%
6	3.155	640	642	645	rBV2	988	699	0.05%	0.007%
7	3.312	679	691	706	rVV5	13631	31924	2.51%	0.315%
8	3.447	729	733	737	rBV6	869	675	0.05%	0.007%
9	3.524	755	757	760	rBV3	1472	635	0.05%	0.006%
10	3.547	761	764	767	rBV5	741	598	0.05%	0.006%
11	3.849	855	858	861	rBV3	1308	937	0.07%	0.009%
12	3.907	865	876	907	rBV3	89998	314029	24.65%	3.100%
13	4.376	1008	1022	1044	rBV	216614	520733	40.88%	5.140%
14	4.711	1120	1126	1130	rBV7	1652	1933	0.15%	0.019%
15	4.733	1130	1133	1135	rVV3	1223	756	0.06%	0.007%
16	4.743	1135	1136	1142	rVV5	1386	1224	0.10%	0.012%
17	4.781	1145	1148	1151	rBV3	1706	1133	0.09%	0.011%
18	4.820	1157	1160	1163	rBV4	1027	665	0.05%	0.007%
19	4.891	1178	1182	1183	rBV4	1639	933	0.07%	0.009%
20	4.955	1200	1202	1208	rVB6	1604	1110	0.09%	0.011%
21	5.003	1214	1217	1220	rVB4	1379	920	0.07%	0.009%
22	5.071	1220	1238	1263	rBV3	492548	1273723	100.00%	12.572%
23	5.408	1340	1343	1346	rBV4	801	540	0.04%	0.005%
24	5.495	1368	1370	1372	rBV3	1309	781	0.06%	0.008%
25	5.640	1402	1415	1442	rBV	420676	838663	65.84%	8.278%
26	5.939	1495	1508	1525	rBV2	160100	319710	25.10%	3.156%
27	6.093	1542	1556	1574	rBV	284920	581955	45.69%	5.744%
28	6.338	1630	1632	1637	rBV5	1322	1188	0.09%	0.012%
29	6.563	1699	1702	1705	rBV5	1617	1260	0.10%	0.012%
30	6.752	1757	1761	1763	rBV3	1267	845	0.07%	0.008%
31	6.769	1763	1766	1767	rBV3	1599	867	0.07%	0.009%
32	6.801	1774	1776	1779	rBV4	1016	620	0.05%	0.006%
33	6.907	1805	1809	1811	rBV4	1385	1164	0.09%	0.011%
34	7.006	1829	1840	1856	rVV	155490	278955	21.90%	2.753%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017217.D
 Acq On : 27 Jun 2020 06:12
 Operator : SY/MD
 Sample : L3133-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.260	1915	1919	1920	rBV4	1497	959	0.08%	0.009%
36	7.338	1931	1943	1967	rBV	593267	1008764	79.20%	9.957%
37	7.643	2029	2038	2051	rBV	109917	184958	14.52%	1.826%
38	7.839	2096	2099	2102	rBV3	1327	937	0.07%	0.009%
39	8.000	2146	2149	2151	rBV3	1664	1023	0.08%	0.010%
40	8.109	2172	2183	2210	rBV	296056	548997	43.10%	5.419%
41	8.598	2333	2335	2338	rBV2	1216	615	0.05%	0.006%
42	8.646	2348	2350	2352	rVB3	1876	823	0.06%	0.008%
43	8.727	2373	2375	2378	rBV4	1441	835	0.07%	0.008%
44	8.875	2408	2421	2441	rBV	618614	1005927	78.98%	9.929%
45	9.190	2517	2519	2522	rVB3	1107	535	0.04%	0.005%
46	9.270	2542	2544	2546	rVB2	1165	530	0.04%	0.005%
47	9.408	2584	2587	2592	rVB6	1564	973	0.08%	0.010%
48	9.434	2592	2595	2597	rBV2	1274	731	0.06%	0.007%
49	9.460	2600	2603	2606	rVV4	2044	1351	0.11%	0.013%
50	9.489	2609	2612	2615	rVB3	1142	698	0.05%	0.007%
51	9.530	2622	2625	2627	rBV3	810	513	0.04%	0.005%
52	9.543	2627	2629	2632	rVB3	1196	612	0.05%	0.006%
53	9.643	2655	2660	2661	rBV6	1413	995	0.08%	0.010%
54	10.048	2783	2786	2788	rVB3	1270	725	0.06%	0.007%
55	10.064	2788	2791	2792	rBV3	1577	888	0.07%	0.009%
56	10.238	2833	2845	2859	rBV	376355	588467	46.20%	5.808%
57	10.434	2903	2906	2909	rVB3	1255	802	0.06%	0.008%
58	10.460	2911	2914	2916	rBV4	1193	724	0.06%	0.007%
59	10.505	2926	2928	2929	rBV2	1250	580	0.05%	0.006%
60	10.534	2934	2937	2939	rBV4	1077	545	0.04%	0.005%
61	10.550	2939	2942	2944	rVV2	1281	828	0.07%	0.008%
62	10.566	2945	2947	2950	rVB3	1693	823	0.06%	0.008%
63	10.666	2976	2978	2981	rVB2	1102	512	0.04%	0.005%
64	10.727	2991	2997	2998	rBV6	1520	1638	0.13%	0.016%
65	10.826	3026	3028	3031	rVB3	1124	606	0.05%	0.006%
66	11.048	3095	3097	3099	rBV3	1214	567	0.04%	0.006%
67	11.167	3131	3134	3138	rBV4	1120	1128	0.09%	0.011%
68	11.270	3155	3166	3182	rBV	620327	928549	72.90%	9.165%
69	11.473	3226	3229	3230	rBV3	1035	568	0.04%	0.006%
70	11.495	3232	3236	3238	rVB4	1702	1229	0.10%	0.012%
71	11.646	3272	3283	3299	rVB	620645	960927	75.44%	9.485%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017217.D
 Acq On : 27 Jun 2020 06:12
 Operator : SY/MD
 Sample : L3133-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.945	3374	3376	3379	rVB2	1257	796	0.06%	0.008%
73	11.961	3379	3381	3382	rBV	1098	548	0.04%	0.005%
74	12.122	3429	3431	3435	rVB3	1570	851	0.07%	0.008%
75	12.199	3450	3455	3460	rBV9	1955	2237	0.18%	0.022%
76	12.225	3461	3463	3467	rBV4	1111	673	0.05%	0.007%
77	12.251	3467	3471	3474	rBV6	1058	1037	0.08%	0.010%
78	12.302	3483	3487	3489	rVB4	1484	995	0.08%	0.010%
79	12.354	3501	3503	3506	rBV4	1284	690	0.05%	0.007%
80	12.440	3527	3530	3532	rBV4	1243	868	0.07%	0.009%
81	12.608	3578	3582	3583	rBV4	933	534	0.04%	0.005%
82	12.820	3645	3648	3650	rBV2	1113	649	0.05%	0.006%
83	13.006	3703	3706	3707	rBV3	1098	549	0.04%	0.005%
84	13.074	3722	3727	3728	rBV4	874	786	0.06%	0.008%
85	13.083	3728	3730	3733	rVV3	1206	787	0.06%	0.008%
86	13.315	3800	3802	3805	rVB2	1715	991	0.08%	0.010%
87	13.353	3811	3814	3817	rBV3	1274	1043	0.08%	0.010%
88	13.469	3846	3850	3852	rBV4	1247	1101	0.09%	0.011%
89	13.656	3907	3908	3914	rVB4	1774	1030	0.08%	0.010%
90	13.723	3926	3929	3932	rVB2	1229	713	0.06%	0.007%
91	13.739	3932	3934	3936	rBV3	986	674	0.05%	0.007%
92	13.800	3949	3953	3955	rBV4	1103	972	0.08%	0.010%
93	13.923	3989	3991	3998	rVV8	1377	1569	0.12%	0.015%
94	13.948	3998	3999	4004	rVB4	1334	688	0.05%	0.007%
95	14.321	4110	4115	4117	rBV4	1290	1103	0.09%	0.011%
96	14.447	4151	4154	4156	rBV2	1995	1192	0.09%	0.012%
97	14.556	4186	4188	4191	rVB4	1344	676	0.05%	0.007%
98	14.624	4204	4209	4214	rBV8	1954	1904	0.15%	0.019%
99	15.218	4390	4394	4397	rVB5	2573	1613	0.13%	0.016%
100	15.585	4506	4508	4509	rBV2	1373	597	0.05%	0.006%


Sum of corrected areas: 10131461

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017217.D
Acq On : 27 Jun 2020 06:12
Operator : SY/MD
Sample : L3133-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q27

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

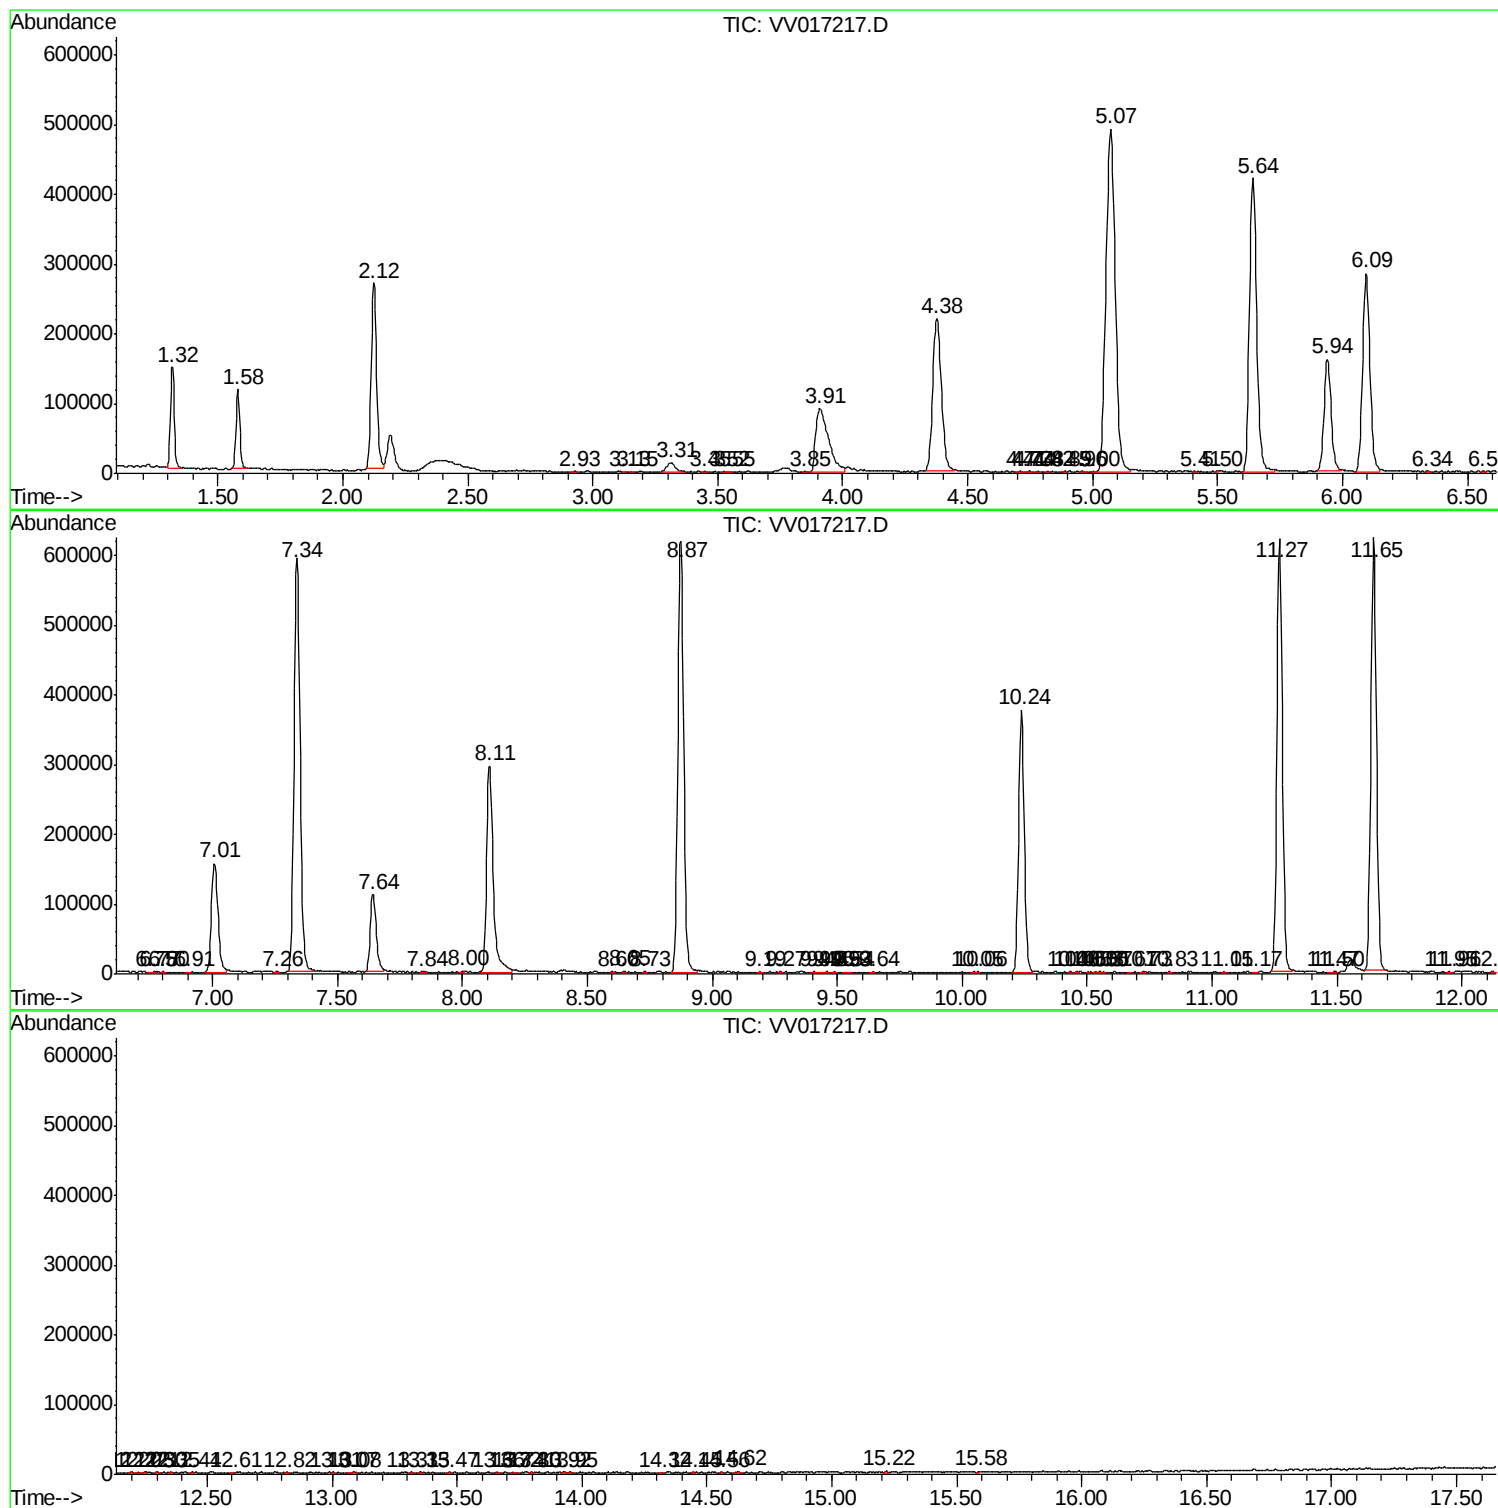

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017217.D
Acq On : 27 Jun 2020 06:12
Operator : SY/MD
Sample : L3133-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q27

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017217.D
Acq On : 27 Jun 2020 06:12
Operator : SY/MD
Sample : L3133-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q27

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc