

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017218.D
 Acq On : 27 Jun 2020 06:35
 Operator : SY/MD
 Sample : L3133-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q28

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	151176	158945	11.89%	1.445%
2	1.579	145	152	163	rBV	118169	129010	9.65%	1.173%
3	2.122	311	321	336	rBV	279230	423728	31.68%	3.853%
4	2.614	471	474	476	rBV4	1066	797	0.06%	0.007%
5	2.775	517	524	526	rBV6	3068	2900	0.22%	0.026%
6	2.849	544	547	550	rVB4	1195	703	0.05%	0.006%
7	3.087	616	621	623	rBV4	1437	1038	0.08%	0.009%
8	3.155	639	642	646	rVB5	1480	1000	0.07%	0.009%
9	3.183	649	651	655	rBV3	1089	858	0.06%	0.008%
10	3.209	655	659	664	rVB6	772	861	0.06%	0.008%
11	3.254	670	673	677	rBV4	1420	1180	0.09%	0.011%
12	3.302	684	688	694	rVB6	963	897	0.07%	0.008%
13	3.605	778	782	785	rBV4	681	685	0.05%	0.006%
14	3.910	865	877	908	rBV2	94626	366226	27.38%	3.330%
15	4.277	987	991	994	rBV5	1544	1067	0.08%	0.010%
16	4.376	1006	1022	1041	rBV	225652	552991	41.35%	5.028%
17	4.691	1113	1120	1121	rBV6	2453	2445	0.18%	0.022%
18	4.765	1141	1143	1149	rBV6	935	759	0.06%	0.007%
19	4.826	1158	1162	1164	rBV3	1699	1137	0.09%	0.010%
20	4.849	1167	1169	1173	rVB3	1143	754	0.06%	0.007%
21	4.884	1178	1180	1183	rBV3	1106	768	0.06%	0.007%
22	5.074	1221	1239	1264	rVV2	517717	1337328	100.00%	12.160%
23	5.405	1339	1342	1346	rBV4	1286	1088	0.08%	0.010%
24	5.505	1370	1373	1375	rBV3	1479	812	0.06%	0.007%
25	5.640	1402	1415	1435	rBV	432959	851746	63.69%	7.744%
26	5.939	1495	1508	1527	rBV	368522	718485	53.73%	6.533%
27	6.093	1544	1556	1580	rVB	304870	605320	45.26%	5.504%
28	6.511	1682	1686	1689	rBV3	1372	1070	0.08%	0.010%
29	6.566	1699	1703	1705	rBV3	1189	829	0.06%	0.008%
30	6.852	1788	1792	1793	rBV4	1100	717	0.05%	0.007%
31	6.888	1798	1803	1805	rBV5	1888	1346	0.10%	0.012%
32	6.949	1820	1822	1827	rVB4	1188	816	0.06%	0.007%
33	7.006	1827	1840	1858	rBV	166651	300621	22.48%	2.733%
34	7.267	1919	1921	1925	rVB5	1448	715	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017218.D
 Acq On : 27 Jun 2020 06:35
 Operator : SY/MD
 Sample : L3133-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q28

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.293	1925	1929	1930	rBV2	1863	1255	0.09%	0.011%
36	7.338	1931	1943	1964	rVV	622111	1058899	79.18%	9.628%
37	7.643	2027	2038	2055	rVV	115972	204392	15.28%	1.858%
38	7.859	2103	2105	2110	rVB4	1474	754	0.06%	0.007%
39	7.945	2130	2132	2135	rVV3	1539	1031	0.08%	0.009%
40	7.971	2138	2140	2143	rVV3	1127	845	0.06%	0.008%
41	8.000	2146	2149	2152	rVB4	1342	918	0.07%	0.008%
42	8.106	2169	2182	2216	rVV	315582	581762	43.50%	5.290%
43	8.537	2313	2316	2320	rBV4	1381	1234	0.09%	0.011%
44	8.640	2346	2348	2354	rVB6	1246	1181	0.09%	0.011%
45	8.733	2372	2377	2379	rBV4	822	727	0.05%	0.007%
46	8.752	2379	2383	2388	rVB7	1849	1919	0.14%	0.017%
47	8.778	2388	2391	2394	rBV4	1559	774	0.06%	0.007%
48	8.875	2407	2421	2443	rBV	634986	1031900	77.16%	9.382%
49	9.039	2469	2472	2474	rBV3	1402	808	0.06%	0.007%
50	9.080	2482	2485	2487	rVV4	1000	709	0.05%	0.006%
51	9.106	2490	2493	2495	rBV3	1406	953	0.07%	0.009%
52	9.502	2612	2616	2620	rVB5	1428	896	0.07%	0.008%
53	9.604	2642	2648	2650	rBV7	1176	1071	0.08%	0.010%
54	9.678	2668	2671	2676	rBV4	2417	1889	0.14%	0.017%
55	9.846	2721	2723	2727	rBV4	1130	1028	0.08%	0.009%
56	9.932	2743	2750	2752	rBV5	1062	1010	0.08%	0.009%
57	9.990	2765	2768	2770	rBV4	1064	812	0.06%	0.007%
58	10.022	2774	2778	2780	rBV4	1338	975	0.07%	0.009%
59	10.238	2830	2845	2858	rBV	394945	617796	46.20%	5.617%
60	10.534	2932	2937	2938	rBV5	1164	835	0.06%	0.008%
61	10.852	3032	3036	3040	rBV6	1116	919	0.07%	0.008%
62	10.945	3061	3065	3066	rBV4	1539	886	0.07%	0.008%
63	11.016	3082	3087	3090	rVB5	1259	1196	0.09%	0.011%
64	11.080	3100	3107	3110	rBV7	1097	1524	0.11%	0.014%
65	11.199	3137	3144	3147	rVB6	2007	2073	0.16%	0.019%
66	11.270	3155	3166	3183	rBV	635182	962167	71.95%	8.748%
67	11.460	3222	3225	3228	rBV4	1254	701	0.05%	0.006%
68	11.511	3237	3241	3244	rBV5	1083	972	0.07%	0.009%
69	11.563	3254	3257	3260	rBV4	1257	751	0.06%	0.007%
70	11.646	3270	3283	3303	rBV	647041	1010657	75.57%	9.189%
71	11.842	3342	3344	3347	rBV4	1437	920	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017218.D
 Acq On : 27 Jun 2020 06:35
 Operator : SY/MD
 Sample : L3133-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q28

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.231	3463	3465	3471	rVV6	1266	1025	0.08%	0.009%
73	12.260	3471	3474	3479	rVV7	1301	1101	0.08%	0.010%
74	12.379	3509	3511	3516	rBV4	1091	1013	0.08%	0.009%
75	12.505	3547	3550	3552	rBV3	1415	955	0.07%	0.009%
76	12.553	3563	3565	3570	rBV5	1279	1087	0.08%	0.010%
77	12.813	3643	3646	3650	rBV3	1182	1015	0.08%	0.009%
78	12.887	3667	3669	3672	rBV4	1415	989	0.07%	0.009%
79	13.099	3732	3735	3739	rVB4	1033	769	0.06%	0.007%
80	13.186	3758	3762	3766	rVV5	1333	1023	0.08%	0.009%
81	13.257	3781	3784	3788	rVB5	1162	1032	0.08%	0.009%
82	13.283	3788	3792	3795	rBV5	1310	1377	0.10%	0.013%
83	13.299	3795	3797	3801	rVB3	1313	687	0.05%	0.006%
84	13.530	3865	3869	3872	rBV3	1493	1254	0.09%	0.011%
85	13.607	3888	3893	3897	rBV5	1440	1555	0.12%	0.014%
86	13.656	3904	3908	3911	rBV3	1743	1537	0.11%	0.014%
87	13.672	3911	3913	3918	rVB3	1657	1002	0.07%	0.009%
88	13.704	3918	3923	3927	rBV8	1198	1230	0.09%	0.011%
89	13.861	3968	3972	3974	rBV4	1189	801	0.06%	0.007%
90	14.003	4013	4016	4019	rBV4	1098	757	0.06%	0.007%
91	14.042	4024	4028	4031	rBV5	982	688	0.05%	0.006%
92	14.212	4077	4081	4084	rBV5	1604	1003	0.08%	0.009%
93	14.376	4129	4132	4134	rBV3	1219	868	0.06%	0.008%
94	14.714	4232	4237	4240	rBV6	826	789	0.06%	0.007%
95	14.807	4264	4266	4270	rVB4	1265	719	0.05%	0.007%
96	14.990	4317	4323	4324	rBV5	2086	1646	0.12%	0.015%
97	15.276	4410	4412	4414	rBV3	1616	804	0.06%	0.007%
98	15.350	4431	4435	4436	rBV2	1417	951	0.07%	0.009%
99	15.440	4461	4463	4466	rBV4	1395	1028	0.08%	0.009%
100	15.765	4562	4564	4566	rBV3	1506	698	0.05%	0.006%


Sum of corrected areas: 10998184

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017218.D
Acq On : 27 Jun 2020 06:35
Operator : SY/MD
Sample : L3133-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q28

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

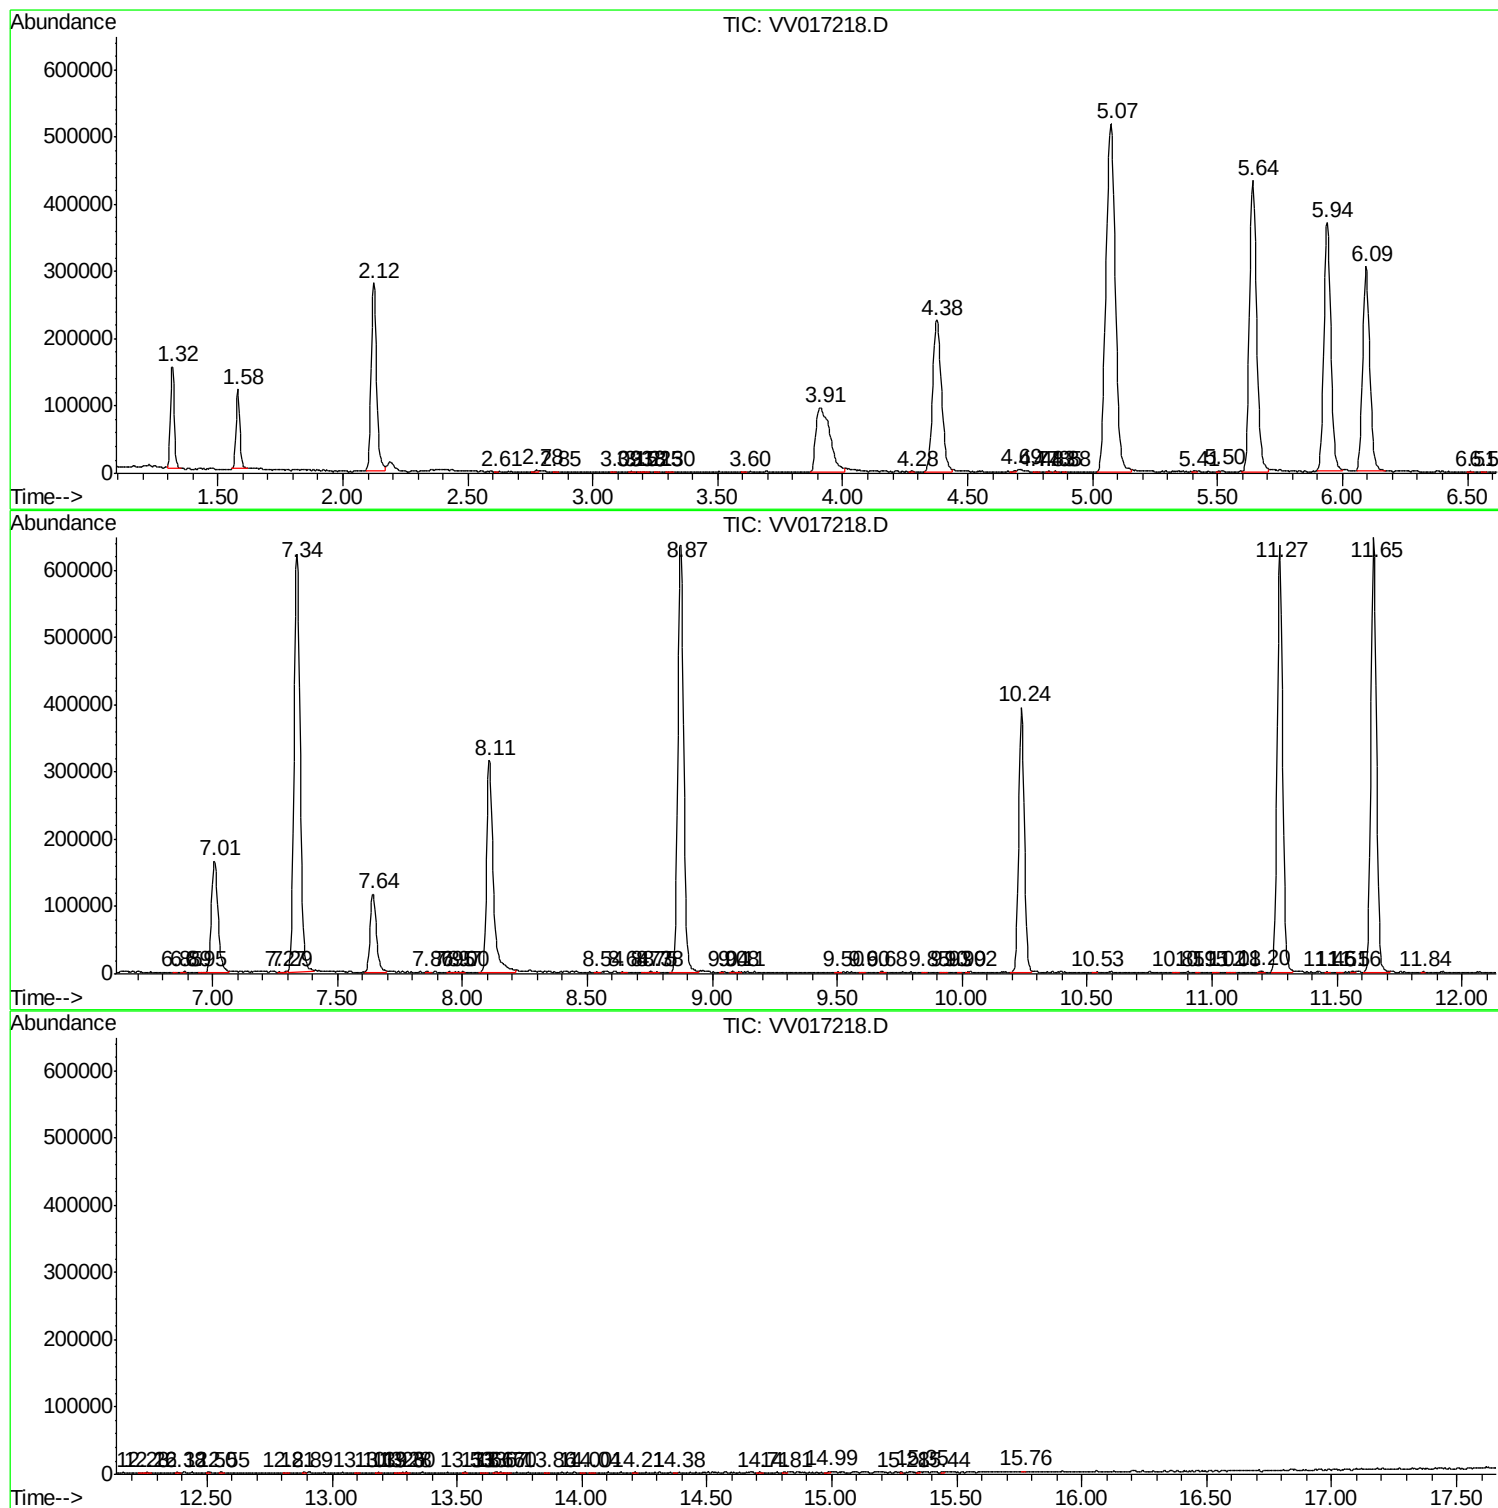

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV062620\
Data File : VV017218.D
Acq On : 27 Jun 2020 06:35
Operator : SY/MD
Sample : L3133-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9Q28

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017218.D
Acq On : 27 Jun 2020 06:35
Operator : SY/MD
Sample : L3133-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q28

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc