

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017219.D
 Acq On : 27 Jun 2020 06:58
 Operator : SY/MD
 Sample : L3133-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q29

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	80	rVB	149598	150805	11.89%	1.496%
2	1.579	145	152	160	rBV	111860	122213	9.63%	1.212%
3	2.122	312	321	335	rBV	266684	402360	31.72%	3.990%
4	2.273	365	368	370	rBV2	1733	1109	0.09%	0.011%
5	3.048	607	609	612	rBV2	940	723	0.06%	0.007%
6	3.087	619	621	625	rVB4	1002	684	0.05%	0.007%
7	3.109	625	628	630	rBV4	893	600	0.05%	0.006%
8	3.164	641	645	647	rBV4	1473	1021	0.08%	0.010%
9	3.482	740	744	747	rBV4	1257	967	0.08%	0.010%
10	3.666	796	801	802	rBV4	817	624	0.05%	0.006%
11	3.679	802	805	809	rVB3	1372	1081	0.09%	0.011%
12	3.746	822	826	828	rBV3	871	844	0.07%	0.008%
13	3.907	865	876	909	rBV	90324	299029	23.57%	2.966%
14	4.219	968	973	974	rBV5	1227	1100	0.09%	0.011%
15	4.241	978	980	982	rBV3	1432	659	0.05%	0.007%
16	4.376	1004	1022	1047	rBV	219134	535801	42.24%	5.314%
17	4.589	1084	1088	1093	rBV8	1527	1543	0.12%	0.015%
18	4.929	1191	1194	1197	rBV3	1224	738	0.06%	0.007%
19	4.962	1201	1204	1207	rBV3	1236	828	0.07%	0.008%
20	5.074	1222	1239	1265	rBV2	492341	1268521	100.00%	12.580%
21	5.367	1328	1330	1335	rVB2	1910	1303	0.10%	0.013%
22	5.389	1335	1337	1339	rBV3	1630	953	0.08%	0.009%
23	5.482	1364	1366	1369	rVB4	1444	763	0.06%	0.008%
24	5.553	1385	1388	1390	rBV2	1091	742	0.06%	0.007%
25	5.640	1403	1415	1434	rBV	422700	842946	66.45%	8.360%
26	5.939	1494	1508	1530	rBV3	137620	286642	22.60%	2.843%
27	6.093	1544	1556	1580	rVB	284280	568871	44.85%	5.642%
28	6.293	1616	1618	1620	rBV3	1517	634	0.05%	0.006%
29	6.540	1690	1695	1696	rBV3	1068	810	0.06%	0.008%
30	6.733	1753	1755	1757	rBV2	1414	844	0.07%	0.008%
31	6.833	1782	1786	1787	rBV5	1192	856	0.07%	0.008%
32	6.894	1803	1805	1808	rVB3	1037	619	0.05%	0.006%
33	6.923	1811	1814	1817	rBV5	1183	938	0.07%	0.009%
34	7.006	1830	1840	1859	rBV	153308	273653	21.57%	2.714%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017219.D
 Acq On : 27 Jun 2020 06:58
 Operator : SY/MD
 Sample : L3133-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q29

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1962	rBV	583975	1004053	79.15%	9.958%
36	7.563	2011	2013	2017	rBV4	1121	919	0.07%	0.009%
37	7.608	2023	2027	2028	rBV3	1379	913	0.07%	0.009%
38	7.640	2028	2037	2054	rVV2	111978	193247	15.23%	1.917%
39	7.855	2101	2104	2106	rBV3	1380	868	0.07%	0.009%
40	7.920	2121	2124	2126	rBV4	815	679	0.05%	0.007%
41	7.997	2145	2148	2152	rBV3	1001	751	0.06%	0.007%
42	8.055	2164	2166	2170	rVB3	1061	703	0.06%	0.007%
43	8.106	2172	2182	2215	rBV	303324	551867	43.50%	5.473%
44	8.611	2336	2339	2345	rBV7	1552	1524	0.12%	0.015%
45	8.672	2354	2358	2360	rBV5	1794	1050	0.08%	0.010%
46	8.717	2369	2372	2378	rVV6	1414	1218	0.10%	0.012%
47	8.823	2402	2405	2408	rBV2	1392	821	0.06%	0.008%
48	8.871	2408	2420	2440	rBV	632877	1027647	81.01%	10.192%
49	9.022	2465	2467	2470	rBV3	1275	617	0.05%	0.006%
50	9.129	2498	2500	2503	rBV3	997	605	0.05%	0.006%
51	9.215	2523	2527	2528	rBV2	1014	676	0.05%	0.007%
52	9.376	2571	2577	2580	rBV6	774	912	0.07%	0.009%
53	9.395	2580	2583	2585	rVV3	1128	700	0.06%	0.007%
54	9.498	2612	2615	2620	rVB4	1865	1600	0.13%	0.016%
55	9.537	2620	2627	2629	rBV6	1188	1341	0.11%	0.013%
56	9.585	2639	2642	2645	rBV3	1040	761	0.06%	0.008%
57	9.698	2674	2677	2681	rBV4	1037	662	0.05%	0.007%
58	9.752	2692	2694	2701	rVB4	1472	1404	0.11%	0.014%
59	9.794	2701	2707	2709	rBV6	1761	1436	0.11%	0.014%
60	9.817	2709	2714	2715	rBV3	944	656	0.05%	0.007%
61	9.916	2740	2745	2748	rBV6	2029	1515	0.12%	0.015%
62	10.238	2834	2845	2866	rVB	374787	579040	45.65%	5.743%
63	10.331	2872	2874	2875	rBV2	1366	673	0.05%	0.007%
64	10.444	2907	2909	2914	rVV3	974	946	0.07%	0.009%
65	10.501	2924	2927	2929	rVB3	1347	631	0.05%	0.006%
66	10.575	2946	2950	2952	rBV3	1118	693	0.05%	0.007%
67	10.772	3005	3011	3015	rBV8	1684	1942	0.15%	0.019%
68	10.868	3037	3041	3042	rBV3	1250	947	0.07%	0.009%
69	10.878	3042	3044	3047	rVB4	1758	929	0.07%	0.009%
70	11.019	3087	3088	3092	rVB2	1606	633	0.05%	0.006%
71	11.048	3092	3097	3098	rBV3	1700	1039	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017219.D
 Acq On : 27 Jun 2020 06:58
 Operator : SY/MD
 Sample : L3133-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q29

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.100	3109	3113	3114	rBV3	1068	701	0.06%	0.007%
73	11.183	3135	3139	3140	rBV3	1088	830	0.07%	0.008%
74	11.270	3155	3166	3184	rBV	624835	950732	74.95%	9.429%
75	11.556	3250	3255	3258	rBV7	2957	3420	0.27%	0.034%
76	11.646	3272	3283	3298	rBV	611956	947182	74.67%	9.394%
77	12.161	3439	3443	3446	rVB4	1790	1281	0.10%	0.013%
78	12.190	3449	3452	3456	rVB4	1565	1065	0.08%	0.011%
79	12.215	3456	3460	3461	rBV3	1495	1005	0.08%	0.010%
80	12.299	3485	3486	3492	rVB4	1049	884	0.07%	0.009%
81	12.366	3505	3507	3509	rBV3	1224	637	0.05%	0.006%
82	12.591	3574	3577	3581	rVB3	1344	979	0.08%	0.010%
83	12.620	3581	3586	3589	rBV7	1238	1192	0.09%	0.012%
84	12.640	3589	3592	3597	rBV6	1335	1037	0.08%	0.010%
85	12.855	3655	3659	3662	rBV5	1382	1148	0.09%	0.011%
86	12.868	3662	3663	3668	rBV5	906	773	0.06%	0.008%
87	12.935	3682	3684	3688	rVB4	1515	799	0.06%	0.008%
88	13.042	3714	3717	3718	rBV2	1478	805	0.06%	0.008%
89	13.353	3812	3814	3819	rVB3	1290	1066	0.08%	0.011%
90	13.376	3819	3821	3824	rBV3	1295	1009	0.08%	0.010%
91	13.392	3824	3826	3830	rVV5	1790	1123	0.09%	0.011%
92	13.543	3870	3873	3875	rBV3	985	615	0.05%	0.006%
93	13.935	3993	3995	3998	rVV4	847	643	0.05%	0.006%
94	14.032	4023	4025	4029	rVV5	1167	696	0.05%	0.007%
95	14.064	4032	4035	4039	rVB5	1194	1250	0.10%	0.012%
96	14.093	4041	4044	4047	rBV5	1476	837	0.07%	0.008%
97	14.186	4068	4073	4074	rBV4	782	628	0.05%	0.006%
98	14.456	4155	4157	4162	rVB5	1517	980	0.08%	0.010%
99	14.636	4210	4213	4214	rBV3	1110	619	0.05%	0.006%
100	15.572	4500	4504	4505	rBV3	1395	919	0.07%	0.009%


Sum of corrected areas: 10083297

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017219.D
Acq On : 27 Jun 2020 06:58
Operator : SY/MD
Sample : L3133-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q29

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

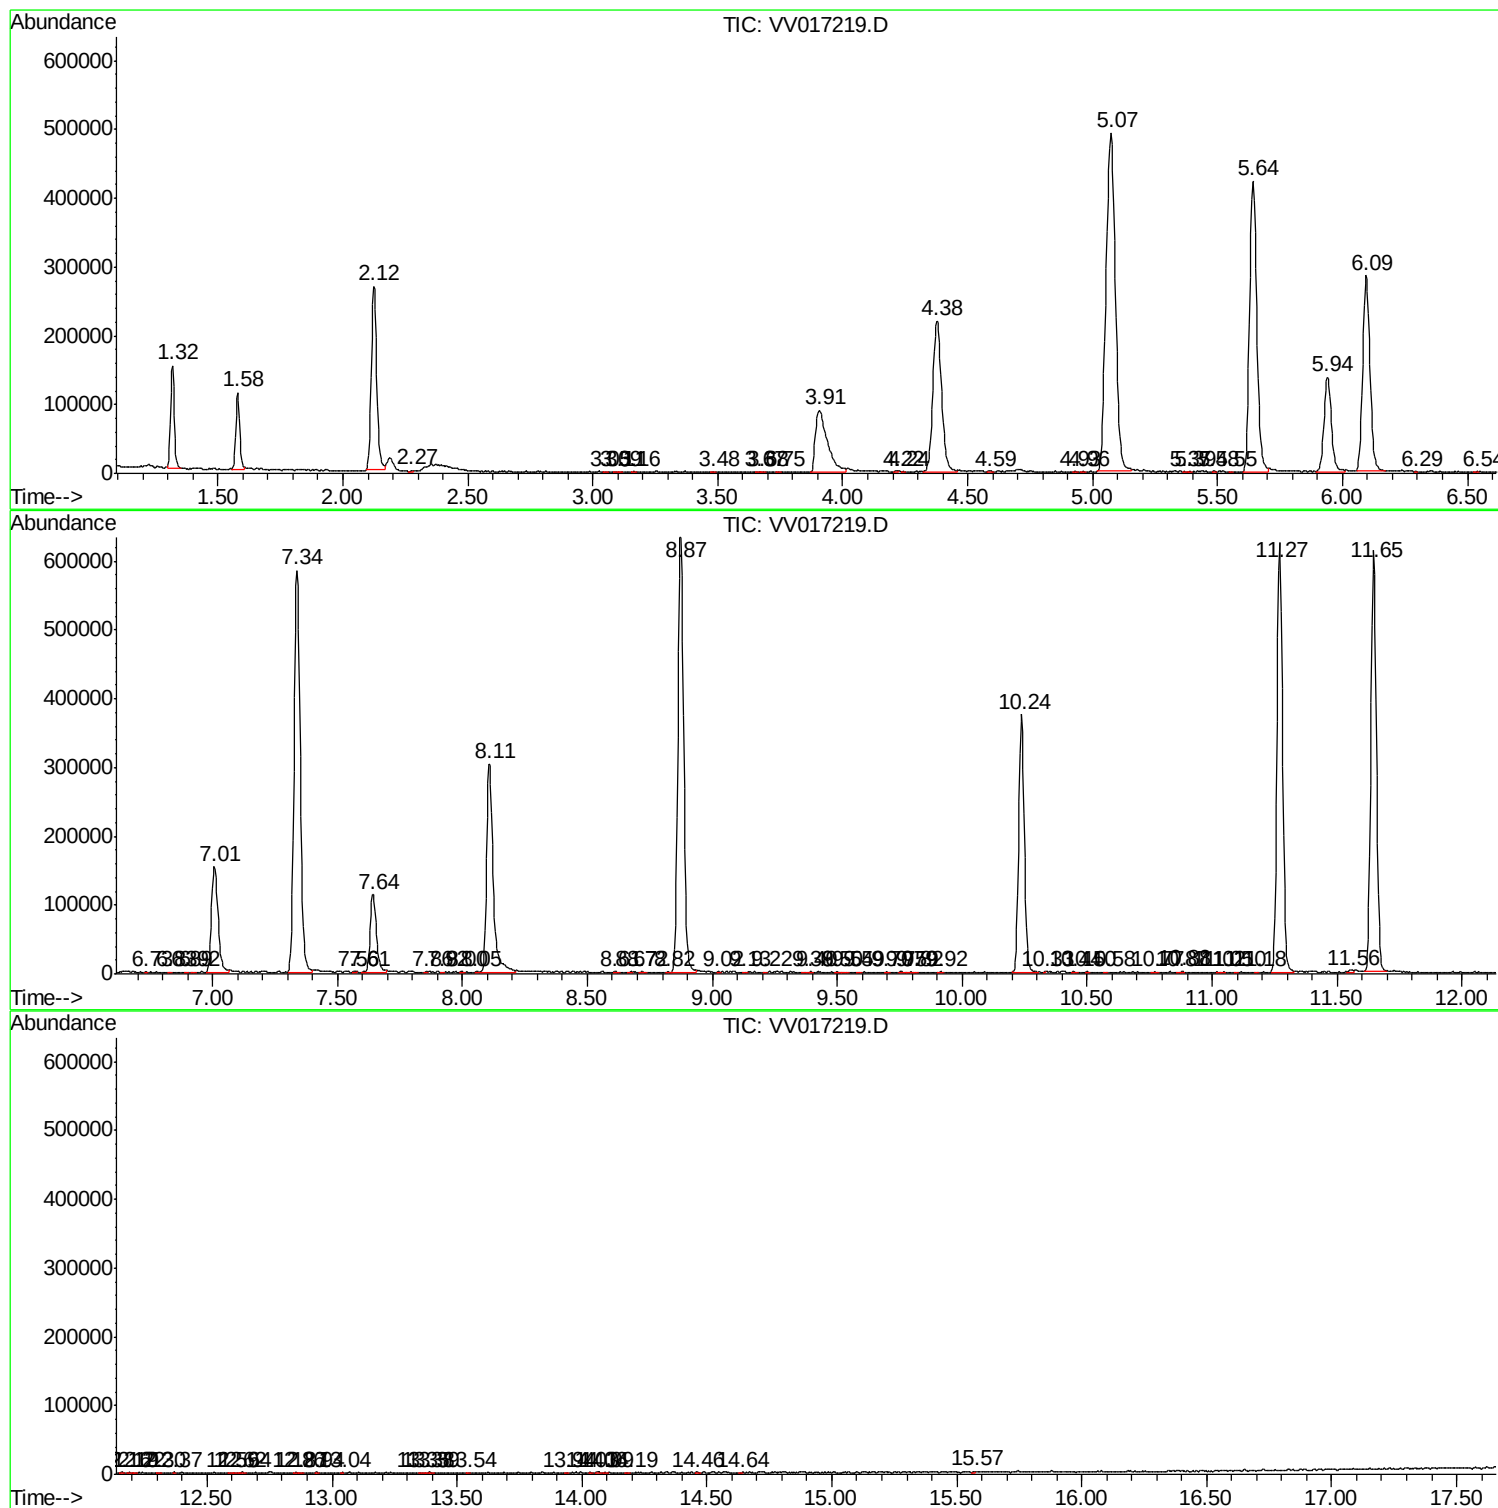

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017219.D
Acq On : 27 Jun 2020 06:58
Operator : SY/MD
Sample : L3133-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q29

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017219.D
Acq On : 27 Jun 2020 06:58
Operator : SY/MD
Sample : L3133-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q29

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
