

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017220.D
 Acq On : 27 Jun 2020 07:21
 Operator : SY/MD
 Sample : L3133-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	153334	157108	12.02%	1.524%
2	1.579	145	152	164	rBV	114523	125340	9.59%	1.216%
3	2.122	312	321	335	rBV	273121	406731	31.12%	3.946%
4	2.653	483	486	488	rBV3	1120	678	0.05%	0.007%
5	2.769	520	522	527	rBV5	1477	1329	0.10%	0.013%
6	2.958	577	581	582	rVV2	1323	746	0.06%	0.007%
7	3.081	613	619	622	rBV7	1115	1197	0.09%	0.012%
8	3.164	643	645	646	rBV2	1344	604	0.05%	0.006%
9	3.315	677	692	707	rBV3	10332	23948	1.83%	0.232%
10	3.434	725	729	731	rBV4	1586	1096	0.08%	0.011%
11	3.595	776	779	782	rBV5	1136	579	0.04%	0.006%
12	3.646	792	795	797	rBV3	974	774	0.06%	0.008%
13	3.746	820	826	828	rBV6	1340	1361	0.10%	0.013%
14	3.762	828	831	833	rBV4	1747	1145	0.09%	0.011%
15	3.833	850	853	858	rVB7	875	756	0.06%	0.007%
16	3.855	858	860	862	rBV3	1592	579	0.04%	0.006%
17	3.907	863	876	900	rBV	89955	275675	21.09%	2.674%
18	4.380	1008	1023	1047	rBV	215877	527966	40.39%	5.122%
19	4.679	1113	1116	1118	rBV3	1243	765	0.06%	0.007%
20	4.804	1152	1155	1158	rBV3	1226	957	0.07%	0.009%
21	4.843	1164	1167	1170	rBV3	1082	709	0.05%	0.007%
22	5.074	1221	1239	1264	rBV2	503244	1307157	100.00%	12.681%
23	5.261	1295	1297	1302	rBV3	1290	638	0.05%	0.006%
24	5.572	1391	1394	1397	rBV3	2048	1288	0.10%	0.012%
25	5.643	1403	1416	1440	rBV	422579	837489	64.07%	8.125%
26	5.820	1467	1471	1473	rBV4	1290	954	0.07%	0.009%
27	5.849	1478	1480	1482	rBV3	1131	735	0.06%	0.007%
28	5.939	1497	1508	1527	rVB3	160208	316006	24.18%	3.066%
29	6.093	1542	1556	1579	rBV	288057	587696	44.96%	5.702%
30	6.331	1628	1630	1633	rVB4	1482	646	0.05%	0.006%
31	6.351	1633	1636	1638	rBV2	1348	973	0.07%	0.009%
32	6.881	1799	1801	1804	rVB3	1273	614	0.05%	0.006%
33	7.006	1830	1840	1863	rBV	159635	285559	21.85%	2.770%
34	7.154	1881	1886	1888	rBV5	1520	1556	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017220.D
 Acq On : 27 Jun 2020 07:21
 Operator : SY/MD
 Sample : L3133-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.338	1930	1943	1963	rBV	605209	1033999	79.10%	10.031%
36	7.498	1990	1993	1994	rBV3	1030	630	0.05%	0.006%
37	7.550	2007	2009	2012	rBV4	1224	657	0.05%	0.006%
38	7.598	2016	2024	2026	rBV8	1842	1984	0.15%	0.019%
39	7.643	2028	2038	2055	rVV	116234	195070	14.92%	1.892%
40	7.881	2110	2112	2114	rVB3	1613	586	0.04%	0.006%
41	7.913	2120	2122	2127	rBV6	1128	1150	0.09%	0.011%
42	8.032	2155	2159	2162	rVB4	2472	1339	0.10%	0.013%
43	8.106	2172	2182	2211	rBV	307041	552651	42.28%	5.362%
44	8.392	2265	2271	2274	rBV7	2243	2361	0.18%	0.023%
45	8.473	2292	2296	2299	rBV4	962	1062	0.08%	0.010%
46	8.762	2384	2386	2390	rVV5	1186	761	0.06%	0.007%
47	8.830	2403	2407	2408	rBV4	838	620	0.05%	0.006%
48	8.871	2409	2420	2443	rVV	632773	1028033	78.65%	9.973%
49	9.096	2488	2490	2491	rBV2	1235	610	0.05%	0.006%
50	9.244	2534	2536	2539	rBV4	1021	800	0.06%	0.008%
51	9.280	2545	2547	2549	rBV3	1310	614	0.05%	0.006%
52	9.318	2556	2559	2561	rBV3	1514	883	0.07%	0.009%
53	9.366	2571	2574	2576	rBV4	1250	922	0.07%	0.009%
54	9.428	2590	2593	2595	rBV2	1540	716	0.05%	0.007%
55	9.537	2624	2627	2630	rBV3	1233	1035	0.08%	0.010%
56	9.672	2665	2669	2674	rBV5	2000	1860	0.14%	0.018%
57	9.849	2722	2724	2726	rVB3	1561	619	0.05%	0.006%
58	9.923	2743	2747	2749	rBV4	1221	903	0.07%	0.009%
59	10.010	2769	2774	2775	rBV4	1115	1129	0.09%	0.011%
60	10.238	2833	2845	2863	rVB	382642	598489	45.79%	5.806%
61	10.431	2903	2905	2909	rBV5	1150	949	0.07%	0.009%
62	10.601	2956	2958	2960	rBV3	983	609	0.05%	0.006%
63	10.672	2979	2980	2988	rVB6	1021	979	0.07%	0.009%
64	10.823	3024	3027	3029	rBV2	1122	742	0.06%	0.007%
65	10.919	3055	3057	3060	rBV3	1023	619	0.05%	0.006%
66	10.997	3077	3081	3082	rBV4	1043	745	0.06%	0.007%
67	11.061	3097	3101	3102	rBV4	1106	645	0.05%	0.006%
68	11.141	3124	3126	3131	rVB4	1500	886	0.07%	0.009%
69	11.167	3131	3134	3138	rBV3	1826	1658	0.13%	0.016%
70	11.228	3151	3153	3155	rBV3	1135	637	0.05%	0.006%
71	11.270	3155	3166	3185	rVV	632046	958671	73.34%	9.301%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017220.D
 Acq On : 27 Jun 2020 07:21
 Operator : SY/MD
 Sample : L3133-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.427	3213	3215	3218	rVB3	1169	793	0.06%	0.008%
73	11.553	3245	3254	3271	rBV4	12285	27900	2.13%	0.271%
74	11.646	3272	3283	3302	rVB	645389	985403	75.39%	9.560%
75	11.961	3379	3381	3383	rBV3	1394	711	0.05%	0.007%
76	12.019	3396	3399	3401	rVB2	1414	654	0.05%	0.006%
77	12.177	3446	3448	3451	rBV2	1245	931	0.07%	0.009%
78	12.337	3495	3498	3502	rVB4	1377	881	0.07%	0.009%
79	12.434	3526	3528	3534	rVB7	1698	944	0.07%	0.009%
80	12.669	3598	3601	3604	rVB3	1501	738	0.06%	0.007%
81	12.752	3621	3627	3629	rBV5	1663	1575	0.12%	0.015%
82	12.817	3644	3647	3650	rVB3	1410	1085	0.08%	0.011%
83	12.845	3650	3656	3658	rBV5	1356	931	0.07%	0.009%
84	12.961	3690	3692	3695	rBV4	1888	1086	0.08%	0.011%
85	12.980	3695	3698	3701	rVV4	1259	782	0.06%	0.008%
86	13.434	3833	3839	3841	rBV6	1536	1403	0.11%	0.014%
87	13.501	3857	3860	3863	rVV5	1537	1120	0.09%	0.011%
88	13.530	3867	3869	3872	rVV4	1041	630	0.05%	0.006%
89	13.669	3911	3912	3914	rBV2	1196	634	0.05%	0.006%
90	14.074	4035	4038	4041	rBV4	1067	737	0.06%	0.007%
91	14.148	4058	4061	4064	rBV4	1111	737	0.06%	0.007%
92	14.656	4215	4219	4221	rBV5	1079	865	0.07%	0.008%
93	14.704	4229	4234	4238	rBV6	1163	1567	0.12%	0.015%
94	14.752	4246	4249	4251	rBV4	1131	624	0.05%	0.006%
95	14.765	4251	4253	4258	rVV5	1277	962	0.07%	0.009%
96	14.951	4309	4311	4313	rBV3	1342	685	0.05%	0.007%
97	15.575	4503	4505	4509	rBV4	1757	1193	0.09%	0.012%
98	15.765	4560	4564	4565	rBV4	2079	1425	0.11%	0.014%
99	16.000	4635	4637	4642	rVB6	2287	1463	0.11%	0.014%
100	16.160	4685	4687	4689	rBV3	2326	1231	0.09%	0.012%


Sum of corrected areas: 10307667

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017220.D
Acq On : 27 Jun 2020 07:21
Operator : SY/MD
Sample : L3133-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q34

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

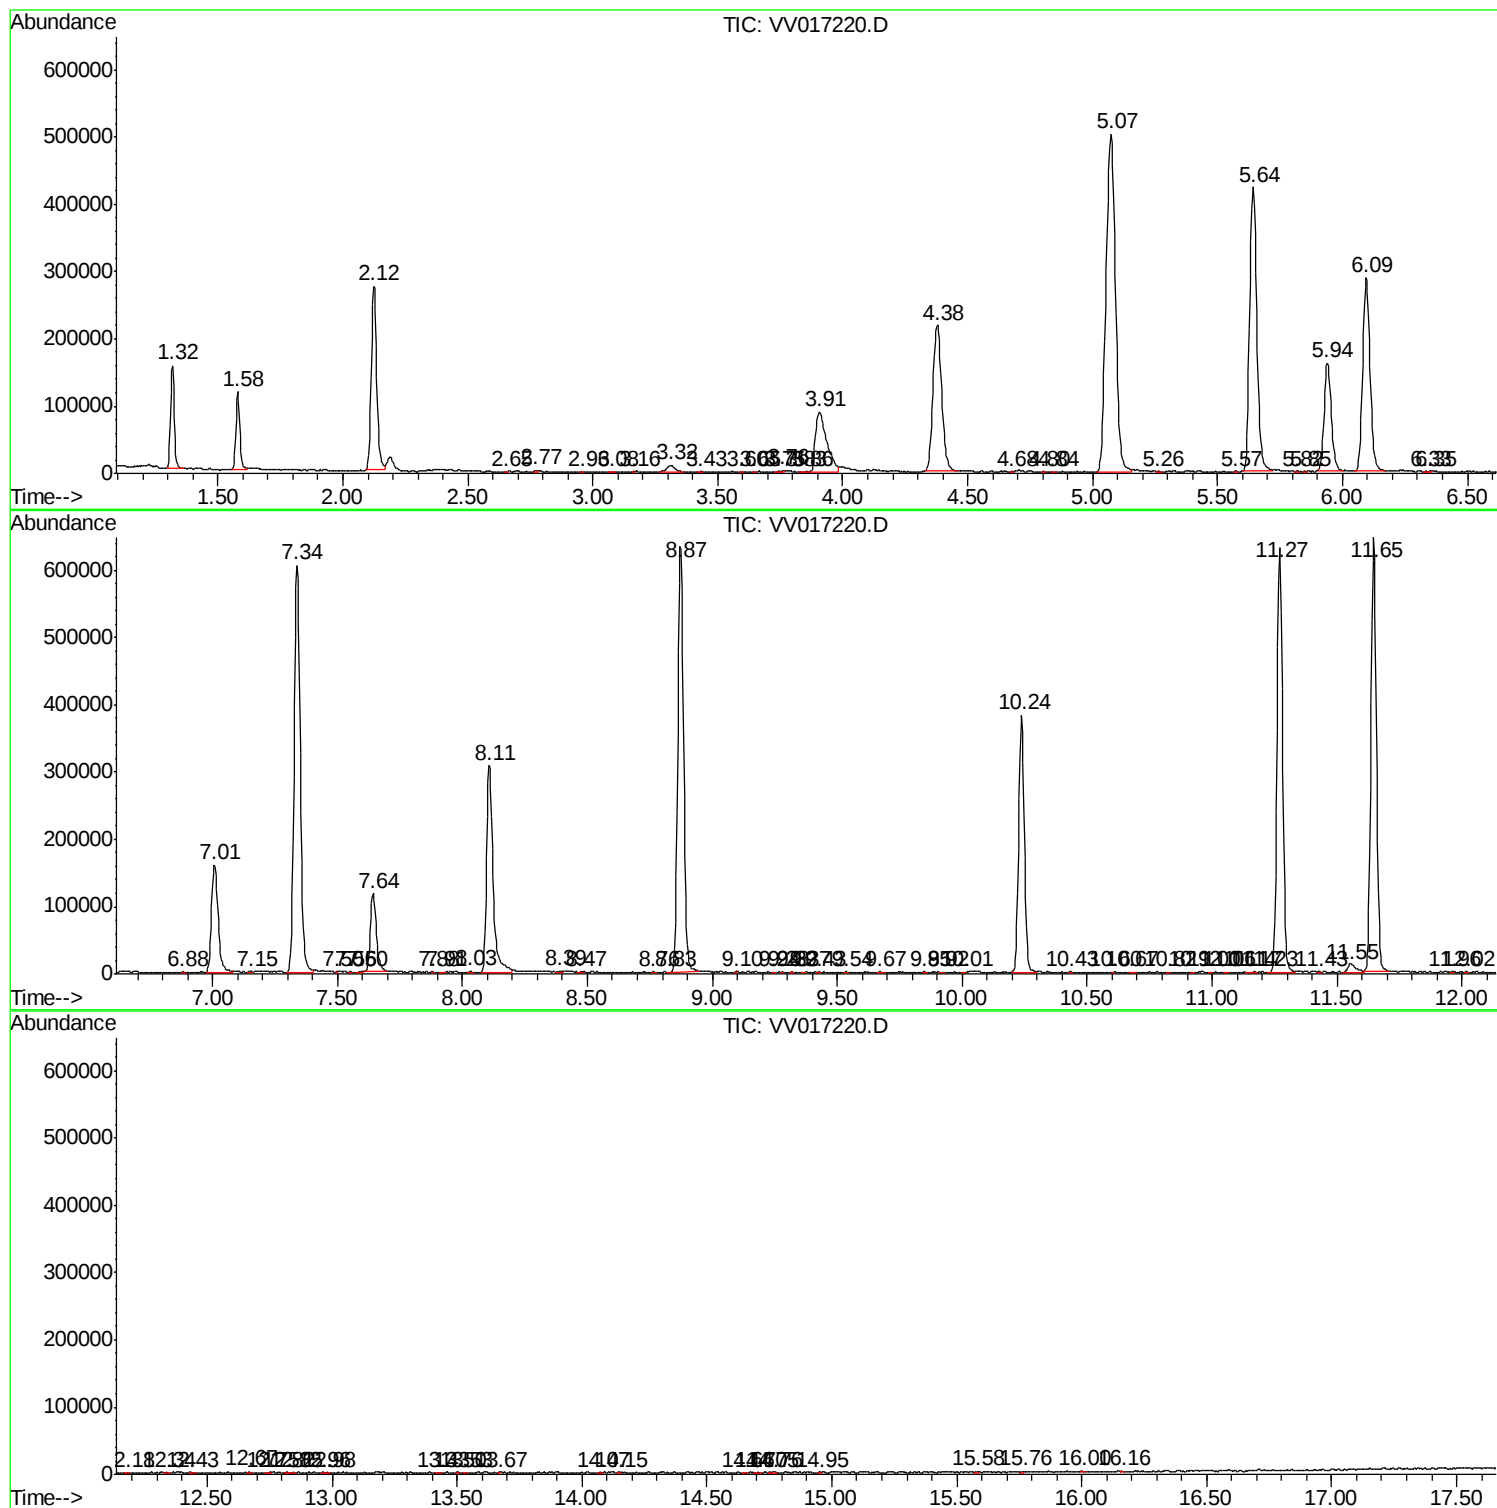

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017220.D
Acq On : 27 Jun 2020 07:21
Operator : SY/MD
Sample : L3133-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q34

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017220.D
Acq On : 27 Jun 2020 07:21
Operator : SY/MD
Sample : L3133-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q34

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc