

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017221.D
 Acq On : 27 Jun 2020 07:45
 Operator : SY/MD
 Sample : L3133-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	146235	149749	11.65%	1.465%
2	1.579	146	152	160	rVB	111090	118067	9.18%	1.155%
3	2.123	311	321	334	rBV	268787	402898	31.33%	3.941%
4	2.923	569	570	573	rVB2	1005	391	0.03%	0.004%
5	3.232	663	666	667	rBV2	1427	657	0.05%	0.006%
6	3.309	679	690	703	rBV4	10682	23318	1.81%	0.228%
7	3.422	722	725	727	rVV3	737	501	0.04%	0.005%
8	3.566	768	770	773	rVB3	885	407	0.03%	0.004%
9	3.672	801	803	805	rVB3	1119	387	0.03%	0.004%
10	3.698	809	811	814	rBV5	1165	524	0.04%	0.005%
11	3.849	856	858	860	rBV4	854	472	0.04%	0.005%
12	3.907	864	876	898	rBV	87682	276445	21.50%	2.704%
13	4.376	1008	1022	1043	rBV2	215642	516942	40.20%	5.056%
14	4.701	1112	1123	1126	rBV7	3670	6133	0.48%	0.060%
15	4.782	1146	1148	1150	rBV3	981	396	0.03%	0.004%
16	4.907	1184	1187	1191	rVB4	896	505	0.04%	0.005%
17	4.936	1191	1196	1197	rBV3	1774	1038	0.08%	0.010%
18	5.074	1216	1239	1261	rBV2	492826	1285945	100.00%	12.578%
19	5.380	1332	1334	1338	rBV4	987	719	0.06%	0.007%
20	5.537	1380	1383	1384	rBV4	893	418	0.03%	0.004%
21	5.573	1392	1394	1396	rVB	1485	565	0.04%	0.006%
22	5.640	1403	1415	1438	rBV	432679	854525	66.45%	8.358%
23	5.939	1495	1508	1526	rBV2	158540	318902	24.80%	3.119%
24	6.093	1544	1556	1574	rBV	282950	569954	44.32%	5.575%
25	6.399	1647	1651	1654	rVB5	1961	1453	0.11%	0.014%
26	6.473	1668	1674	1676	rBV6	1684	1858	0.14%	0.018%
27	6.524	1688	1690	1693	rBV4	1363	883	0.07%	0.009%
28	6.749	1758	1760	1764	rVB4	2025	1286	0.10%	0.013%
29	6.855	1789	1793	1794	rBV2	1427	1026	0.08%	0.010%
30	7.007	1828	1840	1856	rBV	157405	281960	21.93%	2.758%
31	7.338	1931	1943	1964	rBV	596886	1018391	79.19%	9.961%
32	7.643	2028	2038	2054	rBV	114094	194978	15.16%	1.907%
33	7.830	2094	2096	2098	rBV2	938	469	0.04%	0.005%
34	7.952	2131	2134	2135	rBV3	1022	526	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017221.D
 Acq On : 27 Jun 2020 07:45
 Operator : SY/MD
 Sample : L3133-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.106	2173	2182	2210	rBV	298967	543771	42.29%	5.319%
36	8.524	2310	2312	2314	rBV3	1666	766	0.06%	0.007%
37	8.691	2362	2364	2367	rBV3	1157	829	0.06%	0.008%
38	8.772	2387	2389	2393	rVB4	1665	877	0.07%	0.009%
39	8.801	2396	2398	2400	rBV3	1057	684	0.05%	0.007%
40	8.875	2408	2421	2442	rBV	648480	1046291	81.36%	10.234%
41	9.090	2486	2488	2492	rBV5	1383	1087	0.08%	0.011%
42	9.135	2498	2502	2505	rBV5	1366	1318	0.10%	0.013%
43	9.228	2529	2531	2532	rBV2	1112	470	0.04%	0.005%
44	9.283	2546	2548	2550	rVB3	1070	406	0.03%	0.004%
45	9.367	2570	2574	2580	rVB9	1264	1610	0.13%	0.016%
46	9.489	2610	2612	2614	rVB2	1094	510	0.04%	0.005%
47	9.524	2621	2623	2628	rVB5	1251	824	0.06%	0.008%
48	9.550	2628	2631	2634	rBV4	1279	951	0.07%	0.009%
49	9.650	2658	2662	2666	rBV5	1520	1581	0.12%	0.015%
50	9.730	2682	2687	2690	rVB6	2017	1890	0.15%	0.018%
51	9.746	2690	2692	2696	rBV3	1156	946	0.07%	0.009%
52	9.981	2762	2765	2766	rBV4	1229	710	0.06%	0.007%
53	10.032	2775	2781	2782	rBV5	1799	1654	0.13%	0.016%
54	10.109	2801	2805	2806	rBV3	1089	830	0.06%	0.008%
55	10.154	2816	2819	2827	rBV6	1466	1569	0.12%	0.015%
56	10.190	2828	2830	2833	rVB3	1081	578	0.04%	0.006%
57	10.238	2833	2845	2859	rBV	372008	585066	45.50%	5.723%
58	10.363	2879	2884	2888	rBV7	957	1132	0.09%	0.011%
59	10.408	2894	2898	2899	rBV4	1503	1058	0.08%	0.010%
60	10.473	2917	2918	2921	rVB3	1127	477	0.04%	0.005%
61	10.489	2921	2923	2928	rBV5	920	615	0.05%	0.006%
62	10.743	2998	3002	3004	rBV3	1095	944	0.07%	0.009%
63	10.810	3021	3023	3026	rBV2	1121	513	0.04%	0.005%
64	10.826	3026	3028	3033	rVV6	975	594	0.05%	0.006%
65	10.865	3038	3040	3041	rBV2	1074	423	0.03%	0.004%
66	10.987	3076	3078	3080	rBV3	1087	573	0.04%	0.006%
67	11.093	3109	3111	3113	rBV2	741	412	0.03%	0.004%
68	11.106	3113	3115	3116	rVV2	879	425	0.03%	0.004%
69	11.135	3120	3124	3127	rBV3	1312	1488	0.12%	0.015%
70	11.270	3154	3166	3185	rBV	638824	970497	75.47%	9.493%
71	11.476	3227	3230	3232	rBV3	1443	917	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017221.D
 Acq On : 27 Jun 2020 07:45
 Operator : SY/MD
 Sample : L3133-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.553	3249	3254	3269	rVB6	13500	24067	1.87%	0.235%
73	11.646	3272	3283	3306	rVB	624183	970336	75.46%	9.491%
74	11.977	3383	3386	3388	rBV3	1353	896	0.07%	0.009%
75	12.148	3437	3439	3443	rBV3	959	575	0.04%	0.006%
76	12.215	3456	3460	3463	rBV6	1479	1211	0.09%	0.012%
77	12.286	3480	3482	3487	rVB5	1420	1054	0.08%	0.010%
78	12.338	3496	3498	3500	rVB3	1030	379	0.03%	0.004%
79	12.553	3563	3565	3568	rBV5	1308	676	0.05%	0.007%
80	12.723	3617	3618	3620	rBV2	1027	527	0.04%	0.005%
81	12.743	3622	3624	3626	rVV2	1384	680	0.05%	0.007%
82	12.759	3627	3629	3633	rVV5	1244	880	0.07%	0.009%
83	12.997	3701	3703	3705	rVB2	1369	453	0.04%	0.004%
84	13.151	3749	3751	3753	rBV3	841	372	0.03%	0.004%
85	13.167	3753	3756	3757	rBV3	763	391	0.03%	0.004%
86	13.440	3838	3841	3842	rBV	1108	481	0.04%	0.005%
87	13.669	3909	3912	3913	rBV2	1014	500	0.04%	0.005%
88	13.833	3960	3963	3965	rBV4	1003	721	0.06%	0.007%
89	13.871	3973	3975	3977	rVB3	1365	550	0.04%	0.005%
90	13.891	3977	3981	3983	rBV2	1661	1334	0.10%	0.013%
91	13.955	3998	4001	4004	rBV2	1236	808	0.06%	0.008%
92	14.006	4015	4017	4018	rBV2	1581	580	0.05%	0.006%
93	14.100	4043	4046	4048	rBV3	1344	855	0.07%	0.008%
94	14.112	4048	4050	4055	rVB4	1743	1131	0.09%	0.011%
95	14.206	4076	4079	4080	rBV3	1116	681	0.05%	0.007%
96	14.357	4123	4126	4132	rBV7	1186	1357	0.11%	0.013%
97	14.527	4177	4179	4181	rBV3	1121	414	0.03%	0.004%
98	14.736	4242	4244	4246	rBV4	1345	764	0.06%	0.007%
99	14.964	4313	4315	4317	rBV3	1501	716	0.06%	0.007%
100	16.029	4641	4646	4648	rBV4	2430	2390	0.19%	0.023%


Sum of corrected areas: 10223753

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017221.D
Acq On : 27 Jun 2020 07:45
Operator : SY/MD
Sample : L3133-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q35

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

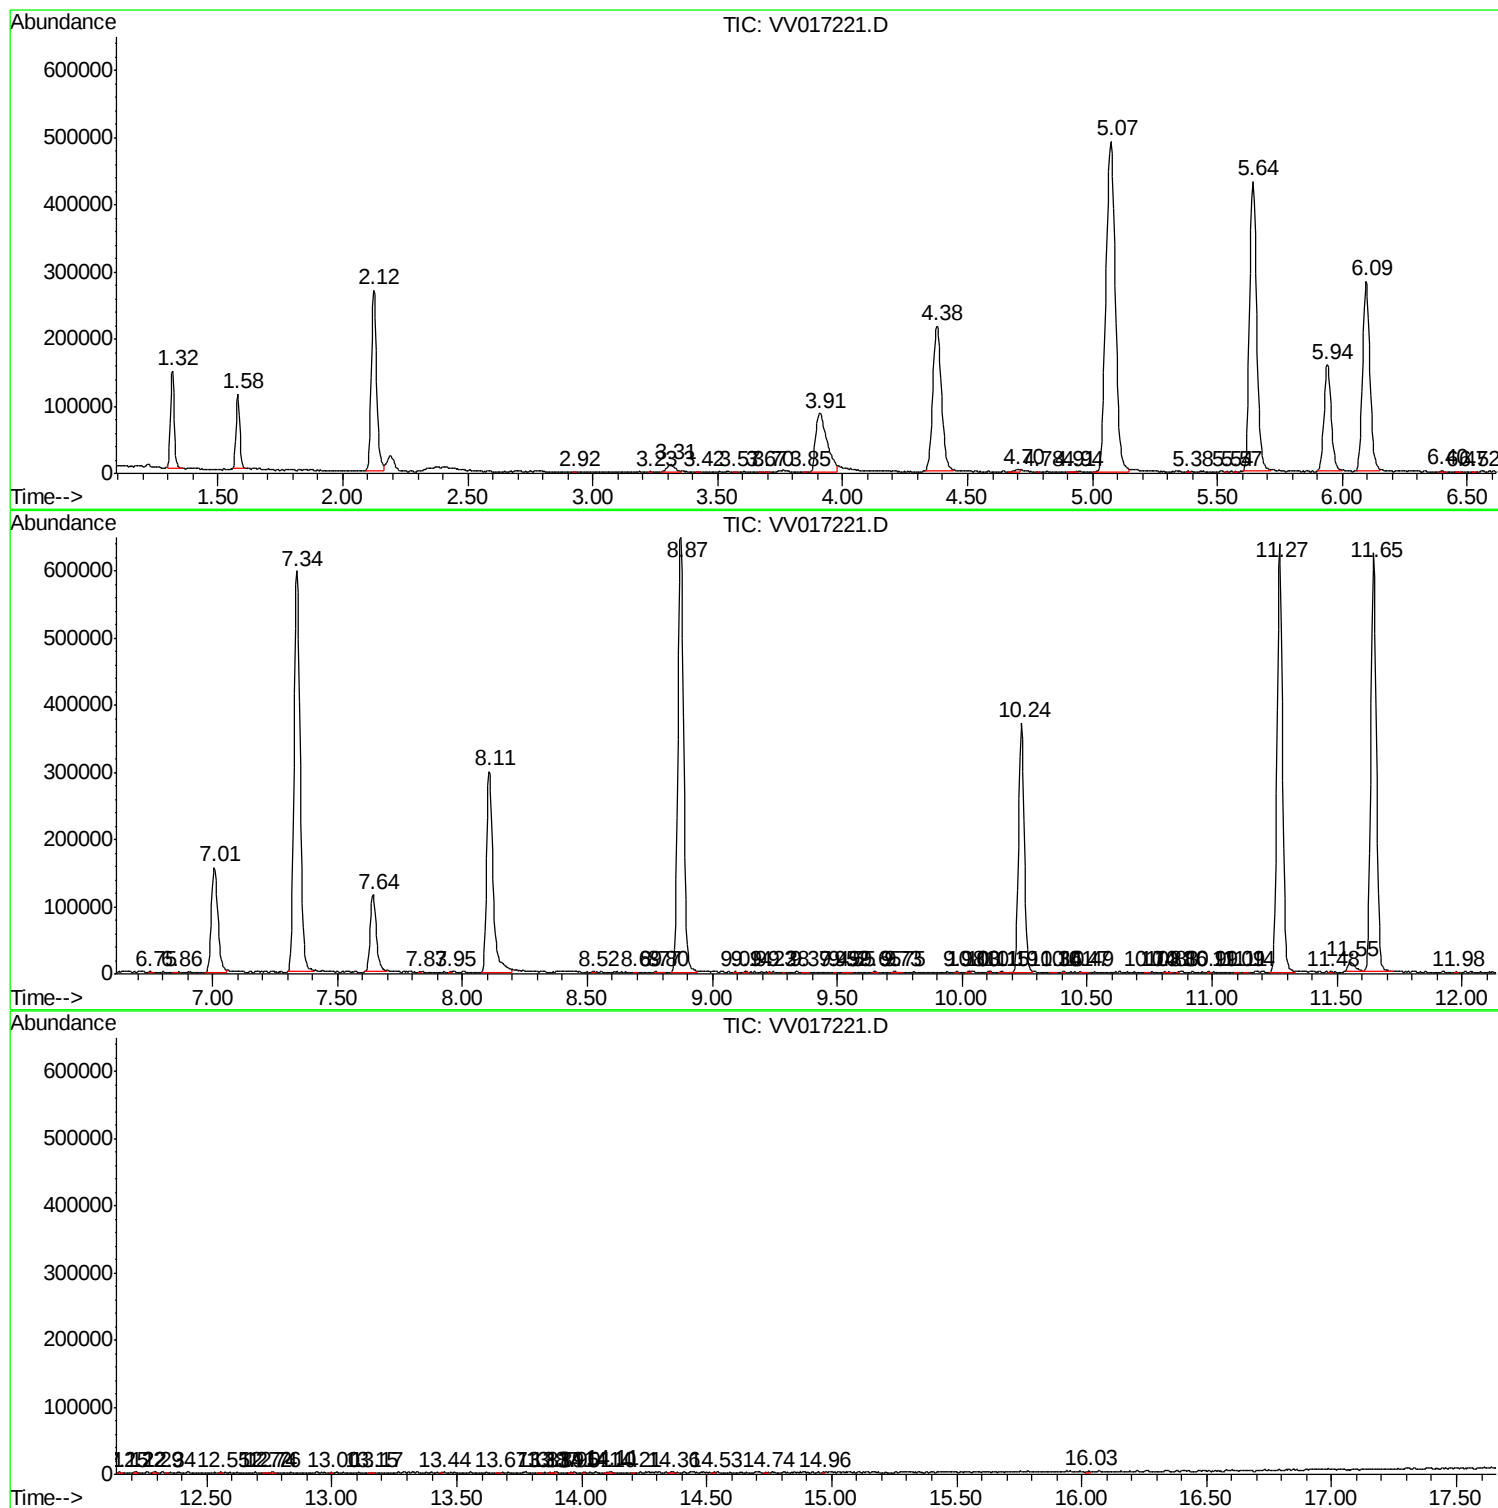

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017221.D
Acq On : 27 Jun 2020 07:45
Operator : SY/MD
Sample : L3133-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q35

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017221.D
Acq On : 27 Jun 2020 07:45
Operator : SY/MD
Sample : L3133-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q35

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc