

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017222.D
 Acq On : 27 Jun 2020 08:08
 Operator : SY/MD
 Sample : L3103-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	150649	154535	12.08%	1.584%
2	1.579	146	152	164	rVB	109393	119659	9.35%	1.227%
3	2.122	308	321	336	rBV	264514	412559	32.25%	4.230%
4	2.582	461	464	466	rBV2	1361	1007	0.08%	0.010%
5	2.621	474	476	481	rBV5	848	591	0.05%	0.006%
6	2.704	500	502	506	rVB4	1489	813	0.06%	0.008%
7	3.048	605	609	611	rBV5	825	704	0.06%	0.007%
8	3.126	628	633	637	rBV6	1438	1293	0.10%	0.013%
9	3.206	655	658	661	rVB3	1143	791	0.06%	0.008%
10	3.264	674	676	680	rVB3	1126	733	0.06%	0.008%
11	3.286	680	683	685	rBV3	1100	712	0.06%	0.007%
12	3.341	698	700	704	rVB4	1217	663	0.05%	0.007%
13	3.428	724	727	730	rBV4	1746	1144	0.09%	0.012%
14	3.460	734	737	740	rBV4	952	649	0.05%	0.007%
15	3.592	775	778	781	rVB5	1029	648	0.05%	0.007%
16	3.717	815	817	820	rBV3	1074	738	0.06%	0.008%
17	3.849	853	858	861	rBV6	1880	1687	0.13%	0.017%
18	3.907	865	876	906	rVV2	87108	245027	19.16%	2.512%
19	4.222	972	974	978	rBV3	1463	945	0.07%	0.010%
20	4.380	1006	1023	1047	rBV	214752	526113	41.13%	5.394%
21	4.566	1078	1081	1083	rBV3	1129	848	0.07%	0.009%
22	5.071	1220	1238	1259	rBV2	496216	1279139	100.00%	13.114%
23	5.264	1296	1298	1301	rBV3	1554	1193	0.09%	0.012%
24	5.286	1302	1305	1308	rVB	7165	3823	0.30%	0.039%
25	5.560	1388	1390	1394	rVB3	982	726	0.06%	0.007%
26	5.579	1394	1396	1402	rBV5	1984	1813	0.14%	0.019%
27	5.640	1402	1415	1445	rBV	417176	832164	65.06%	8.531%
28	5.872	1483	1487	1491	rVB4	1026	1123	0.09%	0.012%
29	5.933	1491	1506	1519	rBV4	8485	22722	1.78%	0.233%
30	6.019	1531	1533	1535	rBV3	1080	633	0.05%	0.006%
31	6.093	1544	1556	1579	rVB2	288630	574039	44.88%	5.885%
32	6.553	1695	1699	1700	rBV3	1026	615	0.05%	0.006%
33	6.617	1715	1719	1721	rBV2	1070	803	0.06%	0.008%
34	6.634	1721	1724	1726	rBV3	1479	1225	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017222.D
 Acq On : 27 Jun 2020 08:08
 Operator : SY/MD
 Sample : L3103-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.695	1741	1743	1746	rBV2	1453	695	0.05%	0.007%
36	6.765	1760	1765	1769	rBV7	1220	1338	0.10%	0.014%
37	6.849	1787	1791	1797	rVB8	932	899	0.07%	0.009%
38	6.939	1815	1819	1822	rBV4	1221	712	0.06%	0.007%
39	7.007	1829	1840	1859	rBV	154875	284153	22.21%	2.913%
40	7.338	1931	1943	1962	rBV	595260	1016174	79.44%	10.418%
41	7.643	2027	2038	2059	rBV	115751	202716	15.85%	2.078%
42	7.994	2144	2147	2151	rBV6	1795	1208	0.09%	0.012%
43	8.109	2172	2183	2201	rBV	296434	533807	41.73%	5.473%
44	8.389	2265	2270	2271	rBV4	783	639	0.05%	0.007%
45	8.482	2298	2299	2304	rBV4	917	649	0.05%	0.007%
46	8.531	2311	2314	2317	rVB4	1543	1053	0.08%	0.011%
47	8.550	2318	2320	2323	rBV4	1561	961	0.08%	0.010%
48	8.666	2353	2356	2362	rVB6	1295	1258	0.10%	0.013%
49	8.695	2362	2365	2371	rVB7	1406	1155	0.09%	0.012%
50	8.871	2408	2420	2438	rBV	623510	1006454	78.68%	10.318%
51	9.219	2526	2528	2531	rVB4	1543	916	0.07%	0.009%
52	9.238	2531	2534	2536	rBV3	1596	827	0.06%	0.008%
53	9.257	2538	2540	2545	rVV3	1045	886	0.07%	0.009%
54	9.312	2553	2557	2559	rBV3	1377	969	0.08%	0.010%
55	10.013	2772	2775	2779	rVB4	1150	880	0.07%	0.009%
56	10.035	2779	2782	2786	rBV4	1030	789	0.06%	0.008%
57	10.125	2807	2810	2813	rBV5	1236	811	0.06%	0.008%
58	10.238	2832	2845	2862	rBV	373007	591252	46.22%	6.062%
59	10.460	2910	2914	2916	rBV4	942	775	0.06%	0.008%
60	10.518	2928	2932	2933	rBV3	1244	730	0.06%	0.007%
61	10.582	2950	2952	2954	rBV3	995	574	0.04%	0.006%
62	10.598	2955	2957	2960	rVV2	1955	1148	0.09%	0.012%
63	10.746	2999	3003	3005	rBV4	819	783	0.06%	0.008%
64	10.801	3016	3020	3021	rBV4	1485	758	0.06%	0.008%
65	10.913	3052	3055	3058	rBV4	942	858	0.07%	0.009%
66	11.010	3083	3085	3089	rVB3	1418	698	0.05%	0.007%
67	11.032	3089	3092	3095	rBV4	1009	792	0.06%	0.008%
68	11.090	3109	3110	3114	rVB3	1455	801	0.06%	0.008%
69	11.112	3114	3117	3119	rBV2	1079	665	0.05%	0.007%
70	11.151	3126	3129	3135	rBV9	1652	1274	0.10%	0.013%
71	11.270	3154	3166	3188	rBV	605246	922332	72.11%	9.456%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062620\
 Data File : VV017222.D
 Acq On : 27 Jun 2020 08:08
 Operator : SY/MD
 Sample : L3103-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.537	3245	3249	3250	rBV3	1202	700	0.05%	0.007%
73	11.646	3272	3283	3302	rBV	616915	952310	74.45%	9.763%
74	11.801	3327	3331	3336	rBV5	1446	1596	0.12%	0.016%
75	11.862	3348	3350	3354	rBV4	1134	911	0.07%	0.009%
76	12.000	3388	3393	3395	rBV4	1729	1373	0.11%	0.014%
77	12.058	3409	3411	3413	rBV2	971	562	0.04%	0.006%
78	12.206	3454	3457	3459	rVV3	920	588	0.05%	0.006%
79	12.418	3521	3523	3525	rBV2	1246	652	0.05%	0.007%
80	12.479	3539	3542	3544	rBV4	1060	891	0.07%	0.009%
81	12.620	3582	3586	3590	rBV6	1710	1279	0.10%	0.013%
82	12.649	3590	3595	3599	rVV6	1701	1337	0.10%	0.014%
83	12.762	3625	3630	3632	rBV4	1556	1253	0.10%	0.013%
84	12.775	3632	3634	3637	rVV4	1395	737	0.06%	0.008%
85	12.800	3640	3642	3646	rVB4	1914	948	0.07%	0.010%
86	13.022	3709	3711	3717	rVV6	1666	1211	0.09%	0.012%
87	13.125	3738	3743	3744	rBV3	888	758	0.06%	0.008%
88	13.427	3835	3837	3839	rBV2	1289	738	0.06%	0.008%
89	13.498	3855	3859	3860	rBV3	1141	564	0.04%	0.006%
90	13.627	3893	3899	3901	rBV6	1396	1448	0.11%	0.015%
91	13.820	3956	3959	3962	rBV3	1269	749	0.06%	0.008%
92	13.935	3991	3995	3999	rBV6	1342	1555	0.12%	0.016%
93	13.974	4005	4007	4010	rVB2	1228	717	0.06%	0.007%
94	14.019	4019	4021	4025	rBV5	705	567	0.04%	0.006%
95	14.154	4058	4063	4065	rBV4	1383	1158	0.09%	0.012%
96	14.196	4072	4076	4078	rBV3	1399	1052	0.08%	0.011%
97	14.498	4167	4170	4172	rVB2	1443	726	0.06%	0.007%
98	14.910	4296	4298	4301	rBV3	1159	843	0.07%	0.009%
99	15.141	4368	4370	4373	rVB3	1263	622	0.05%	0.006%
100	15.463	4466	4470	4471	rBV3	1465	1026	0.08%	0.011%


Sum of corrected areas: 9754137

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062620\
Data File : VV017222.D
Acq On : 27 Jun 2020 08:08
Operator : SY/MD
Sample : L3103-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q79

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

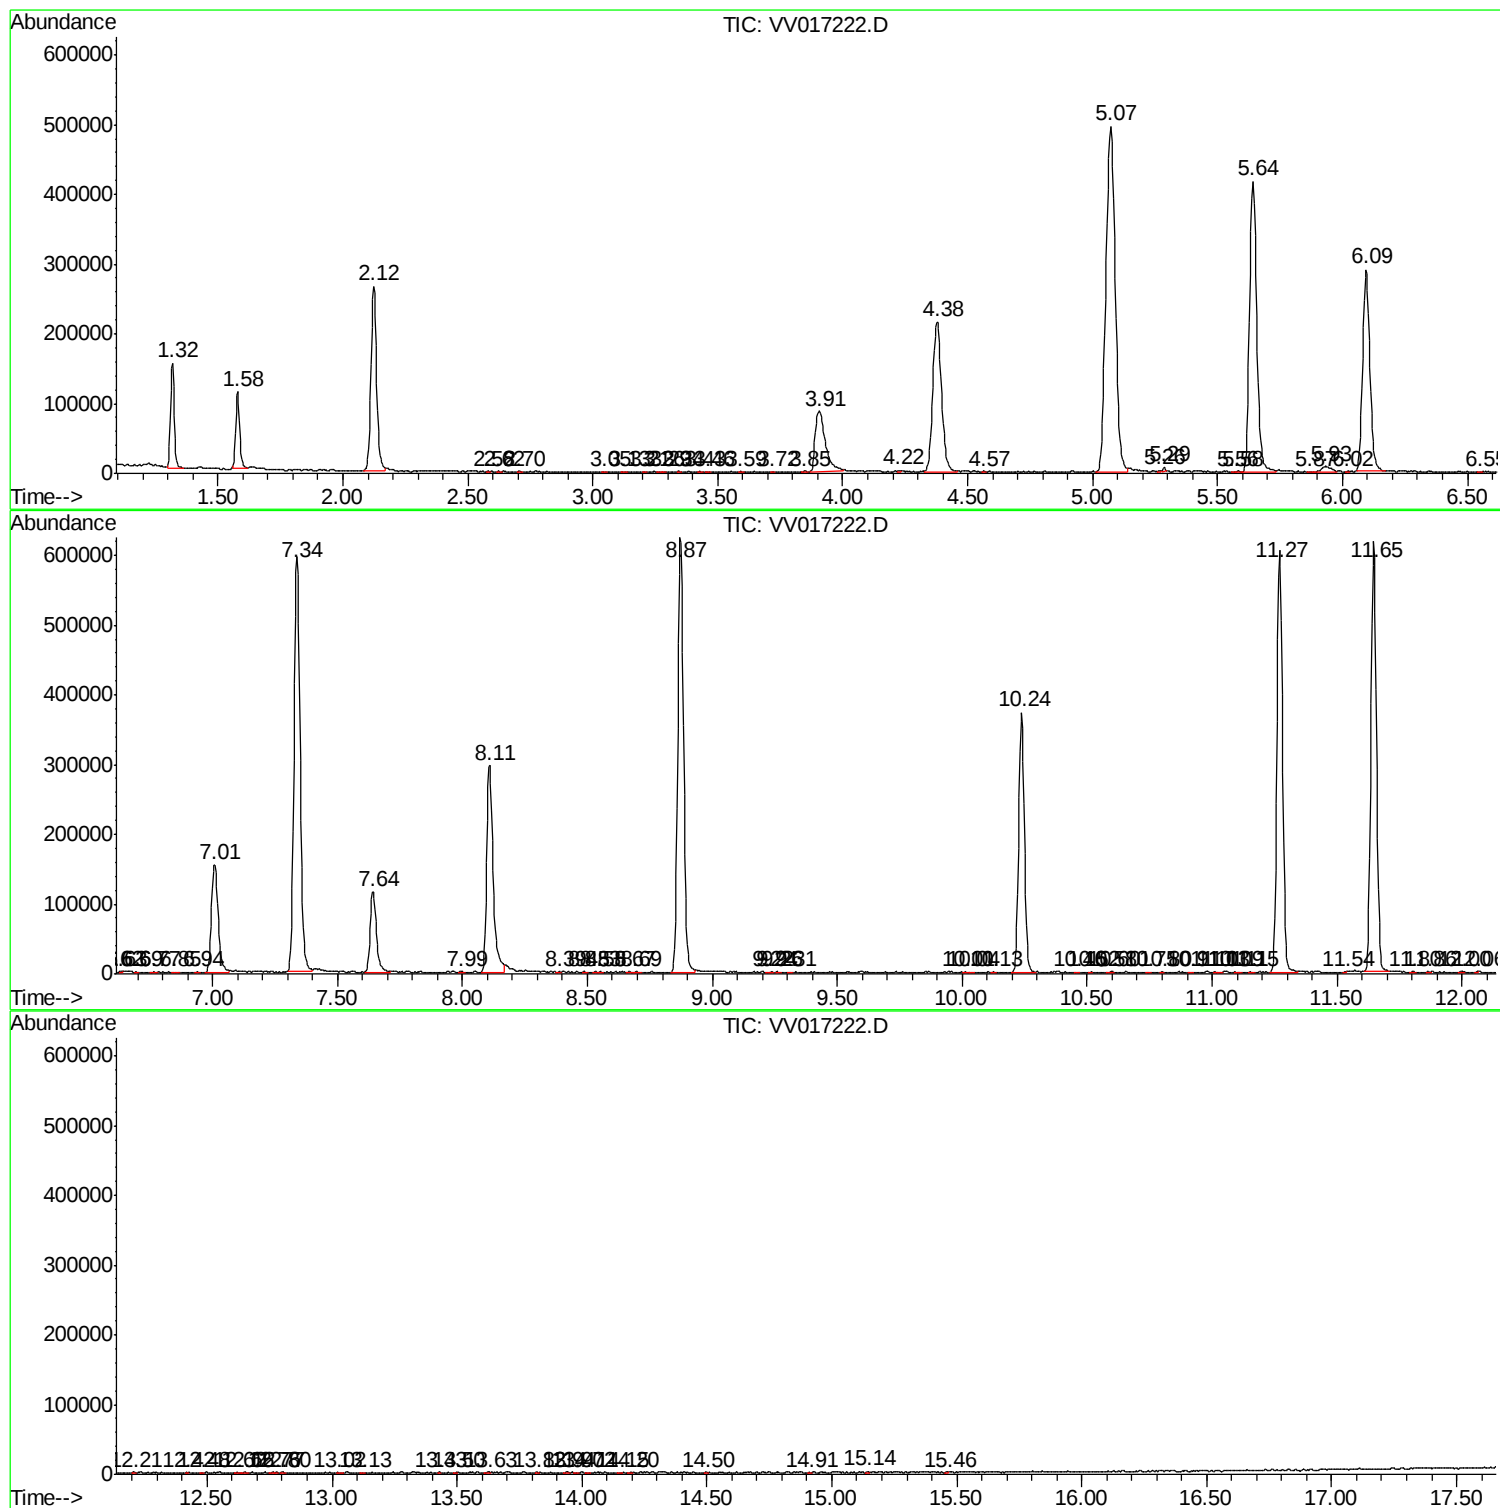

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017222.D
Acq On : 27 Jun 2020 08:08
Operator : SY/MD
Sample : L3103-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q79

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062620\
Data File : VV017222.D
Acq On : 27 Jun 2020 08:08
Operator : SY/MD
Sample : L3103-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q79

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc