


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062719\
Data File : VV011758.D
Acq On : 26 Jun 2019 14:07
Operator : SY/MD
Sample : BFB06
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062719SIM.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jun 27 04:08:35 2019

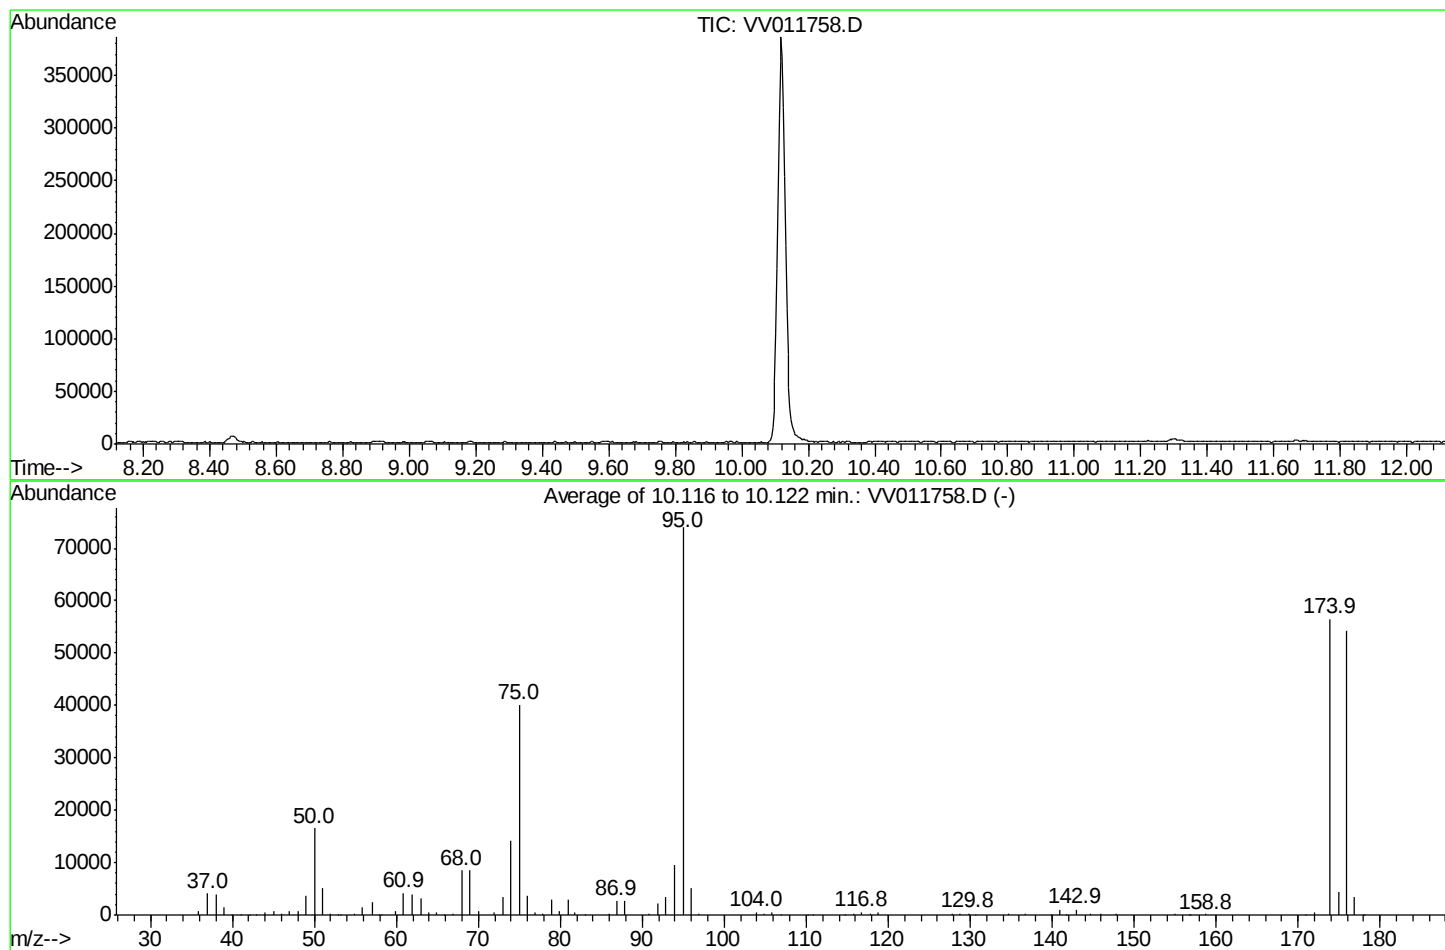

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	16609	PASS
75	95	30	80	54.2	40074	PASS
95	95	100	100	100.0	73989	PASS
96	95	5	9	6.8	5057	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.3	56461	PASS
175	174	5	9	7.9	4452	PASS
176	174	95	101	96.2	54304	PASS
177	176	5	9	6.4	3495	PASS

Scan 2794 (10.074 min): VV011758.D
BFB06

m/z	Abundance
35.20	115.0
35.80	150.0
36.70	162.0
38.80	133.0
40.00	389.0
41.20	125.0
43.90	392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB06

m/z	Abundance
35.90	921.0
37.00	4117.0
38.00	3765.0
39.00	1759.0
39.90	440.0
41.00	204.0
42.10	109.0
43.90	981.0
45.00	752.0
46.10	122.0
46.90	780.0
47.90	670.0
49.00	3644.0
50.00	17144.0
51.00	4961.0
52.00	317.0
52.90	116.0
55.00	264.0
55.90	1372.0
57.00	2515.0
57.90	157.0
59.90	694.0
60.90	4209.0
62.00	3916.0
62.90	3031.0
63.90	415.0
64.90	438.0
65.90	107.0
66.90	315.0
68.00	8408.0
69.00	8640.0
70.00	602.0
71.90	637.0
72.90	3352.0
74.00	13660.0
75.00	39272.0
76.00	3784.0
76.90	609.0
77.80	293.0
78.90	2850.0
79.80	697.0
80.90	2983.0
81.80	620.0
86.00	195.0
86.90	2665.0
87.90	2475.0
90.80	276.0
92.00	1983.0
92.90	3461.0
94.00	9425.0
95.00	71664.0
96.00	5083.0
96.90	267.0
104.00	522.0
104.80	167.0
105.80	556.0
106.90	102.0
110.80	125.0
114.70	133.0
115.80	253.0
116.80	514.0
117.90	365.0
118.80	472.0
127.80	290.0
128.80	131.0
129.80	270.0
134.70	171.0
136.80	174.0
139.90	105.0
140.90	884.0
142.90	1014.0
144.80	235.0
145.90	158.0
147.70	189.0
154.90	183.0
156.70	149.0
158.80	166.0
170.80	111.0
171.90	585.0
173.90	53640.0
174.90	4376.0
175.90	51960.0
176.90	3376.0
177.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB06

m/z	Abundance
35.90	932.0
36.90	4249.0
37.90	3969.0
39.00	1731.0
39.90	419.0
41.00	191.0
42.10	107.0
43.90	959.0
45.00	718.0
45.90	134.0
46.00	135.0
46.90	829.0
48.00	726.0
48.90	3806.0
50.00	17184.0
51.00	5298.0
51.90	329.0
52.90	125.0
54.90	294.0
55.90	1461.0
57.00	2551.0
57.90	119.0
58.20	128.0
59.90	789.0
60.90	4281.0
62.00	4124.0
63.00	3210.0
63.90	404.0
64.90	440.0
66.90	301.0
68.00	8748.0
69.00	8981.0
70.00	748.0
72.00	604.0
73.00	3628.0
74.00	14682.0
75.00	41456.0
76.00	3764.0
76.90	645.0
77.80	294.0
78.90	2938.0
79.90	759.0
80.90	3112.0
81.80	602.0
83.00	122.0
85.90	207.0
86.90	2779.0
87.90	2687.0
90.90	282.0
91.90	2240.0
92.90	3714.0
94.00	9804.0
95.00	76736.0
96.00	5304.0
96.90	207.0
103.90	483.0
104.80	185.0
105.80	501.0
110.20	103.0
110.80	106.0
114.80	109.0
115.90	297.0
116.80	567.0
117.80	371.0
118.80	497.0
127.80	279.0
128.70	141.0
129.80	346.0
130.70	124.0
134.70	225.0
136.80	186.0
140.90	929.0
141.70	140.0
142.90	1019.0
144.70	243.0
145.90	181.0
147.70	210.0
155.00	161.0
156.90	171.0
158.80	171.0
172.00	633.0
173.90	58496.0
174.90	4619.0
175.90	56392.0
176.90	3611.0
178.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB06

m/z	Abundance
35.10	108.0
35.90	838.0
36.90	4000.0
37.90	3904.0
39.00	1617.0
39.90	383.0
41.00	149.0
42.80	130.0
43.90	873.0
45.00	709.0
45.90	162.0
46.90	814.0
48.00	643.0
48.90	3527.0
50.00	15501.0
51.00	5030.0
51.90	310.0
52.80	134.0
53.20	113.0
54.90	273.0
55.90	1391.0
57.00	2311.0
60.00	794.0
60.90	3988.0
61.90	3793.0
63.00	3052.0
63.90	363.0
65.00	402.0
66.90	279.0
68.00	8317.0
69.00	8271.0
70.00	755.0
71.90	501.0
73.00	3533.0
74.00	14112.0
75.00	39496.0
76.00	3344.0
76.90	597.0
77.90	256.0
78.90	2748.0
79.90	742.0
80.90	2866.0
81.80	545.0
83.00	131.0
85.90	207.0
86.90	2723.0
87.90	2627.0
90.80	316.0
91.90	2254.0
92.90	3467.0
94.00	9256.0
95.00	73568.0
96.00	4785.0
96.90	154.0
103.90	479.0
104.80	172.0
105.80	398.0
115.90	333.0
116.80	506.0
117.80	298.0
118.80	467.0
127.80	242.0
128.70	137.0
129.80	371.0
130.70	114.0
134.70	212.0
136.70	172.0
140.90	875.0
141.60	123.0
142.90	958.0
144.70	201.0
145.90	156.0
147.80	221.0
155.00	142.0
156.90	177.0
158.70	154.0
170.90	168.0
172.00	602.0
173.90	57248.0
174.90	4361.0
175.90	54560.0
176.90	3500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB06