

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062722\
 Data File : VV026567.D
 Acq On : 27 Jun 2022 11:50
 Operator : SY/MD
 Sample : VV0627WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK386

Quant Time: Jun 28 01:52:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 28 01:50:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	217457	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	205372	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	86572	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	98861	5.653	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.000%
7) Chloroethane-d5	1.580	69	79668	5.671	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.400%
11) 1,1-Dichloroethene-d2	2.121	63	131583	4.234	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.600%
20) 2-Butanone-d5	3.915	46	108667	62.500	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.000%
24) Chloroform-d	4.362	84	145309	5.083	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
26) 1,2-Dichloroethane-d4	5.040	65	59136	5.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%
32) Benzene-d6	5.056	84	303706	5.148	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
36) 1,2-Dichloropropane-d6	6.075	67	86533	5.334	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%
41) Toluene-d8	7.317	98	247123	4.659	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
43) trans-1,3-Dichloroprop...	7.625	79	20868	4.977	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.600%
46) 2-Hexanone-d5	8.091	63	75516	47.283	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.560%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	53567	5.048	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	79079	5.520	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.400%
Target Compounds						
16) Methylene chloride	2.519	84	3046	0.195	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062722\
Data File : VV026567.D
Acq On : 27 Jun 2022 11:50
Operator : SY/MD
Sample : VV0627WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK386


Quant Time: Jun 28 01:52:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 28 01:50:05 2022
Response via : Initial Calibration

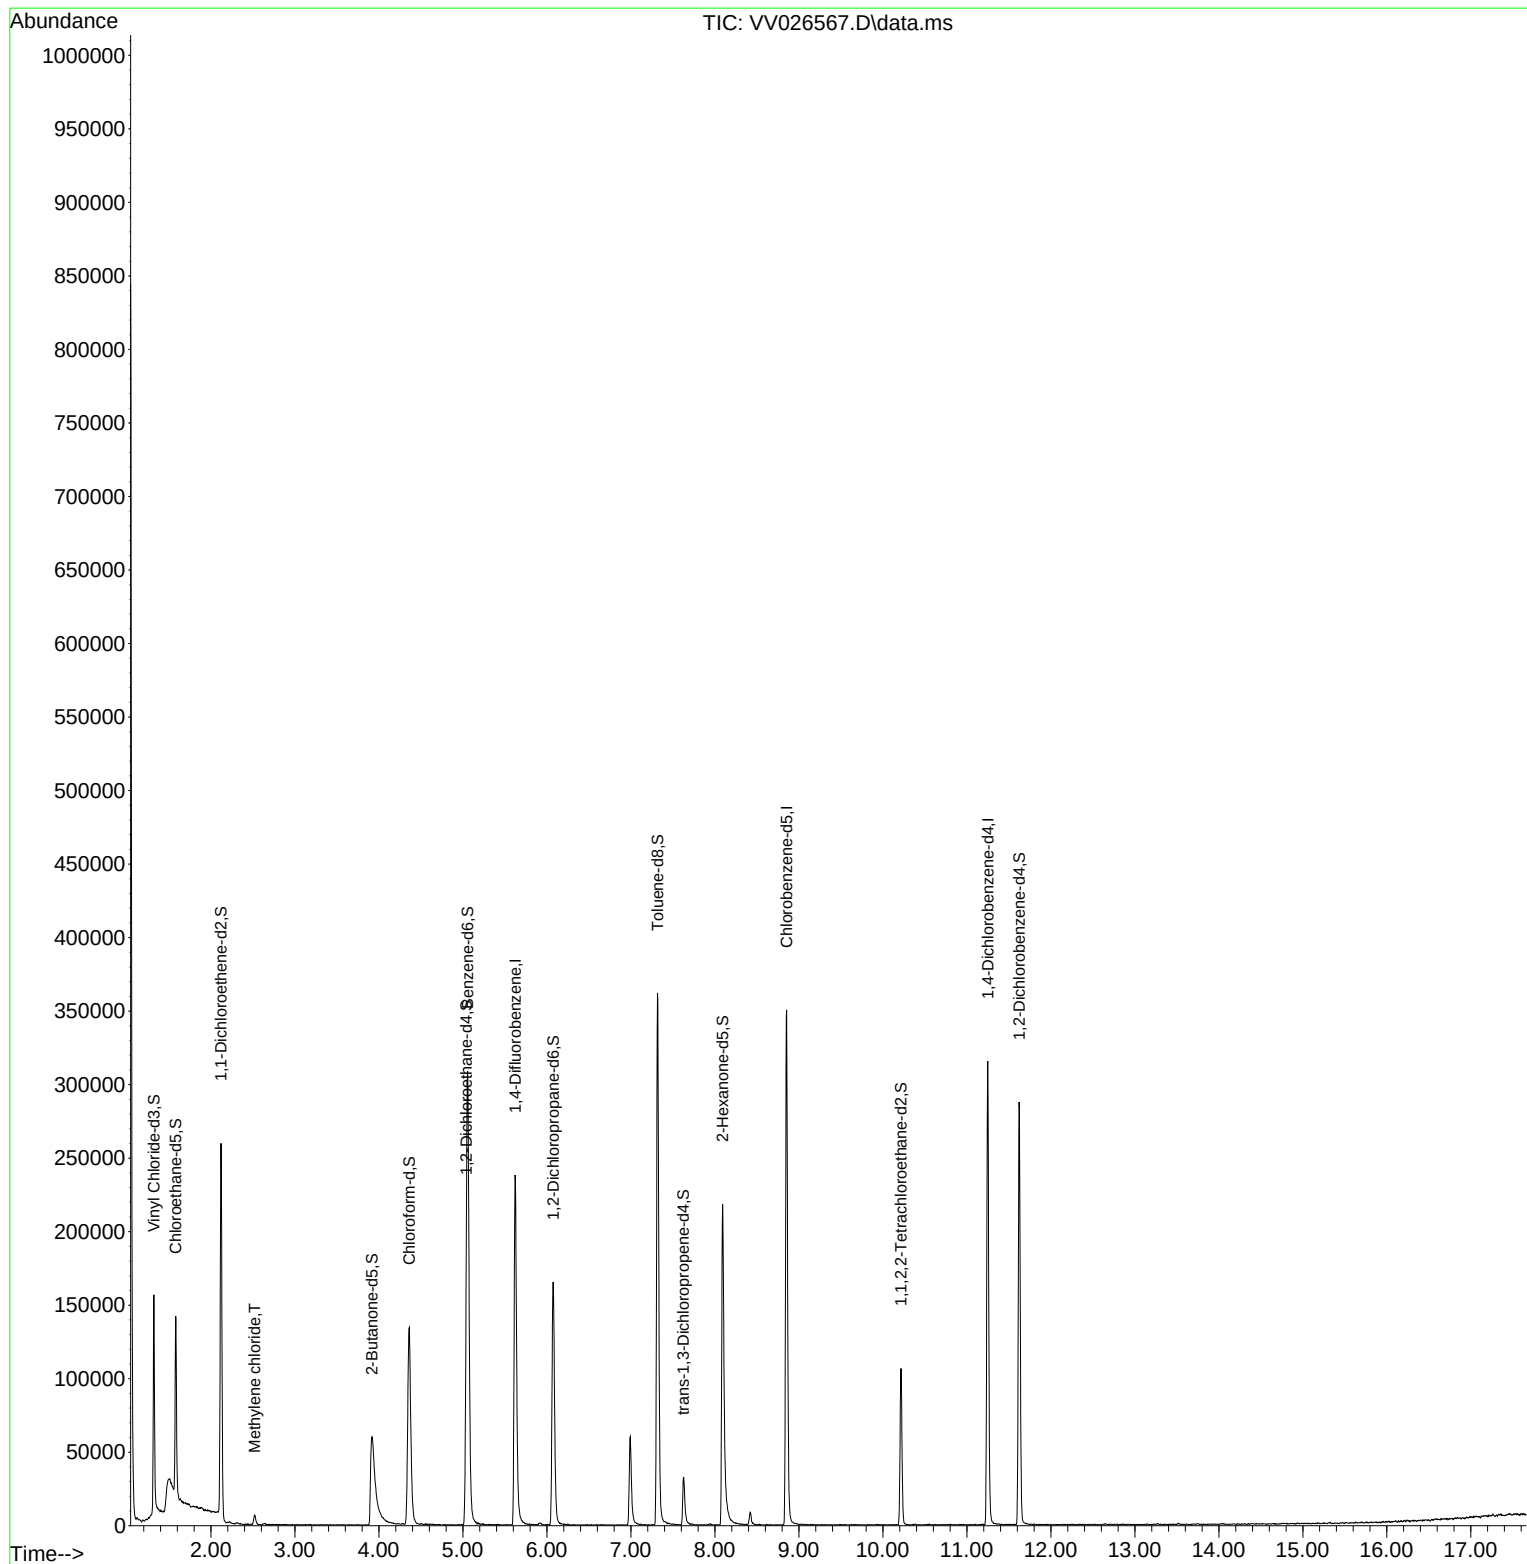

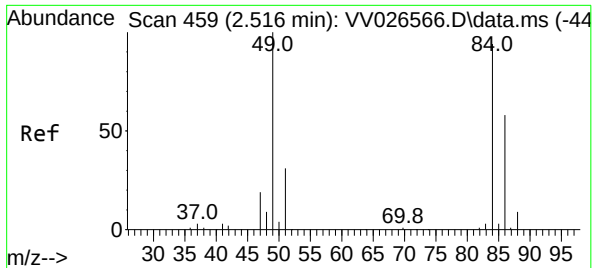

#16
Methylene chloride
Concen: 0.195 ug/L
RT: 2.519 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026567.D
Acq: 27 Jun 2022 11:50

Instrument :
MSVOA_V
ClientSampleId :
VBLK386

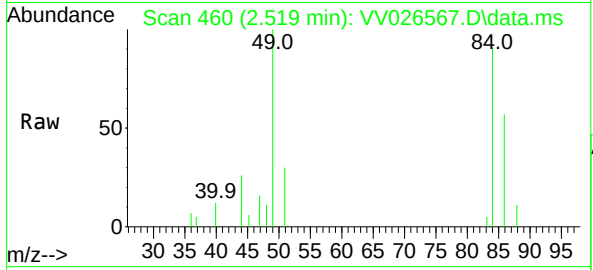

Tgt Ion: 84 Resp: 3046
Ion Ratio Lower Upper
84 100
86 62.1 46.0 85.4
49 109.5 77.7 144.3

