
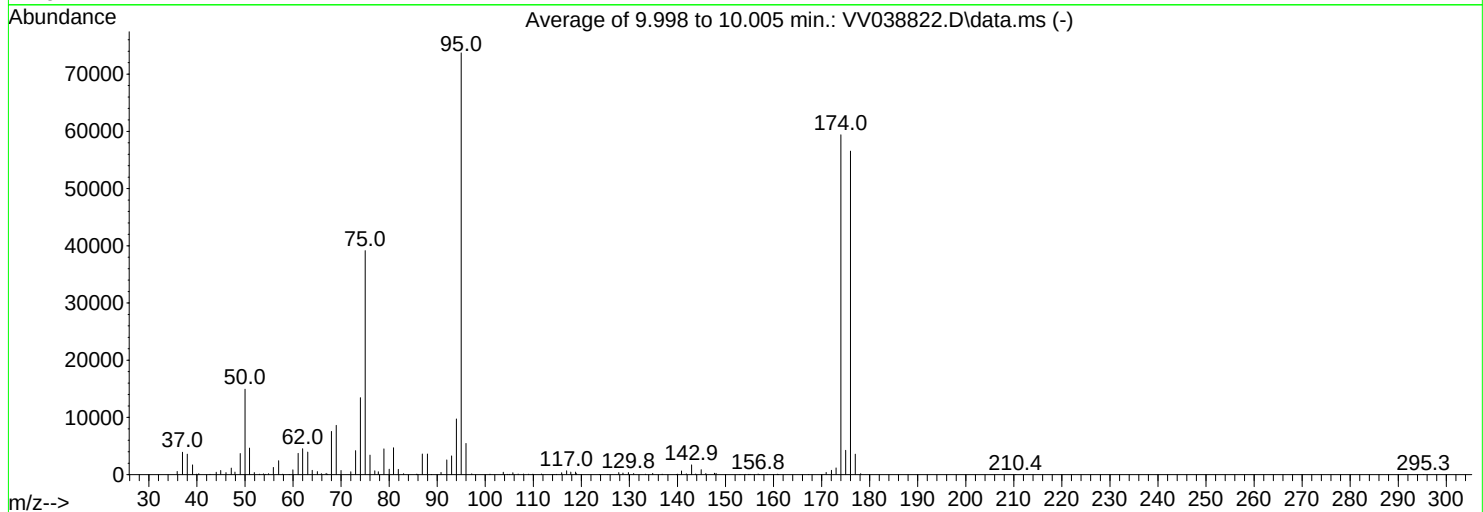


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV062725\  
Data File : VV038822.D  
Acq On : 27 Jun 2025 07:52  
Operator : SY/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V062725W.M  
Title : SW846 8260  
Last Update : Mon Jun 30 10:57:08 2025

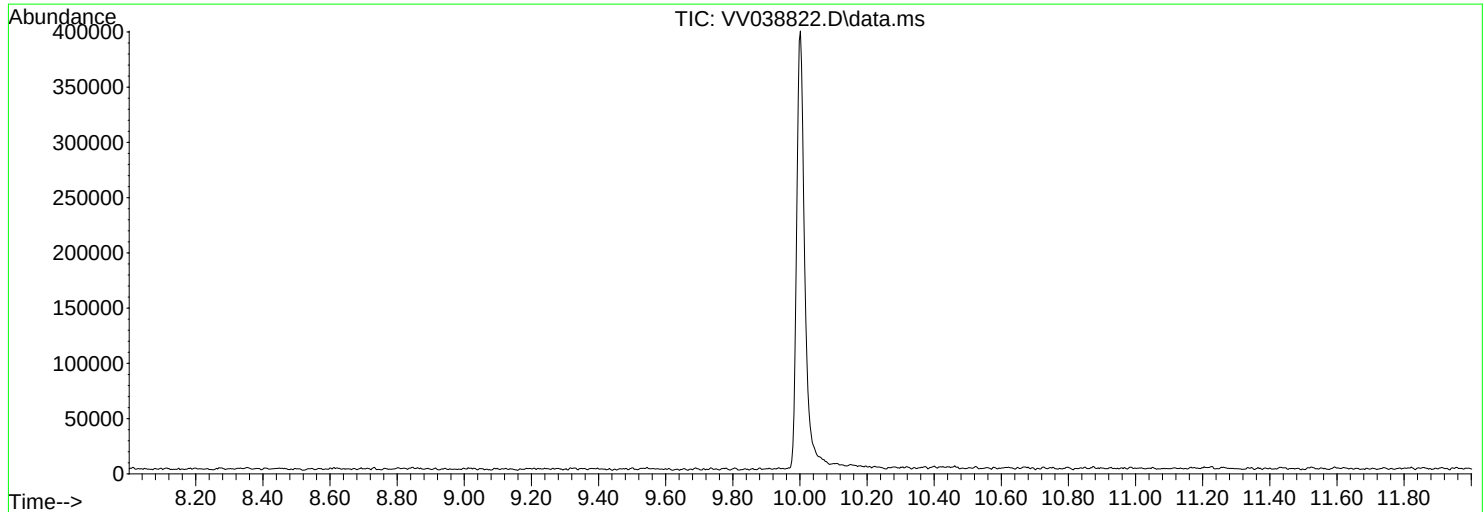

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.3         | 14929      | PASS                |
| 75             | 95              | 30              | 60              | 53.1         | 39141      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 73723      | PASS                |
| 96             | 95              | 5               | 9               | 7.4          | 5465       | PASS                |
| 173            | 174             | 0.00            | 2               | 2.0          | 1182       | PASS                |
| 174            | 95              | 50              | 100             | 80.6         | 59397      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 4257       | PASS                |
| 176            | 174             | 95              | 101             | 95.2         | 56555      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 3571       | PASS                |