

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062818\
 Data File : VV006489.D
 Acq On : 28 Jun 2018 15:02
 Operator : SY/MD
 Sample : J3766-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ST2

Quant Time: Jun 29 03:58:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 29 03:51:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	311756	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	278858	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	122550	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	117391	5.73	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	114.60%
7) Chloroethane-d5	1.59	69	94696	5.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.60%
11) 1,1-Dichloroethene-d2	2.13	63	152524	4.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.00%
20) 2-Butanone-d5	3.98	46	213058	55.47	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.94%
24) Chloroform-d	4.41	84	177281	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.09	65	88412	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.20%
32) Benzene-d6	5.11	84	401816	5.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.80%
36) 1,2-Dichloropropane-d6	6.12	67	116946	5.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.00%
41) Toluene-d8	7.37	98	359578	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
43) trans-1,3-Dichloropropene-	7.67	79	36694	4.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.20%
46) 2-Hexanone-d5	8.14	63	153851	48.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.46%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	64240	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	123978	5.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.80%


Target Compounds					Ovalue
13) Acetone	2.23	43	11172	4.75	ug/L 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062818\
Data File : VV006489.D
Acq On : 28 Jun 2018 15:02
Operator : SY/MD
Sample : J3766-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ST2

Quant Time: Jun 29 03:58:37 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 29 03:51:20 2018
Response via : Initial Calibration

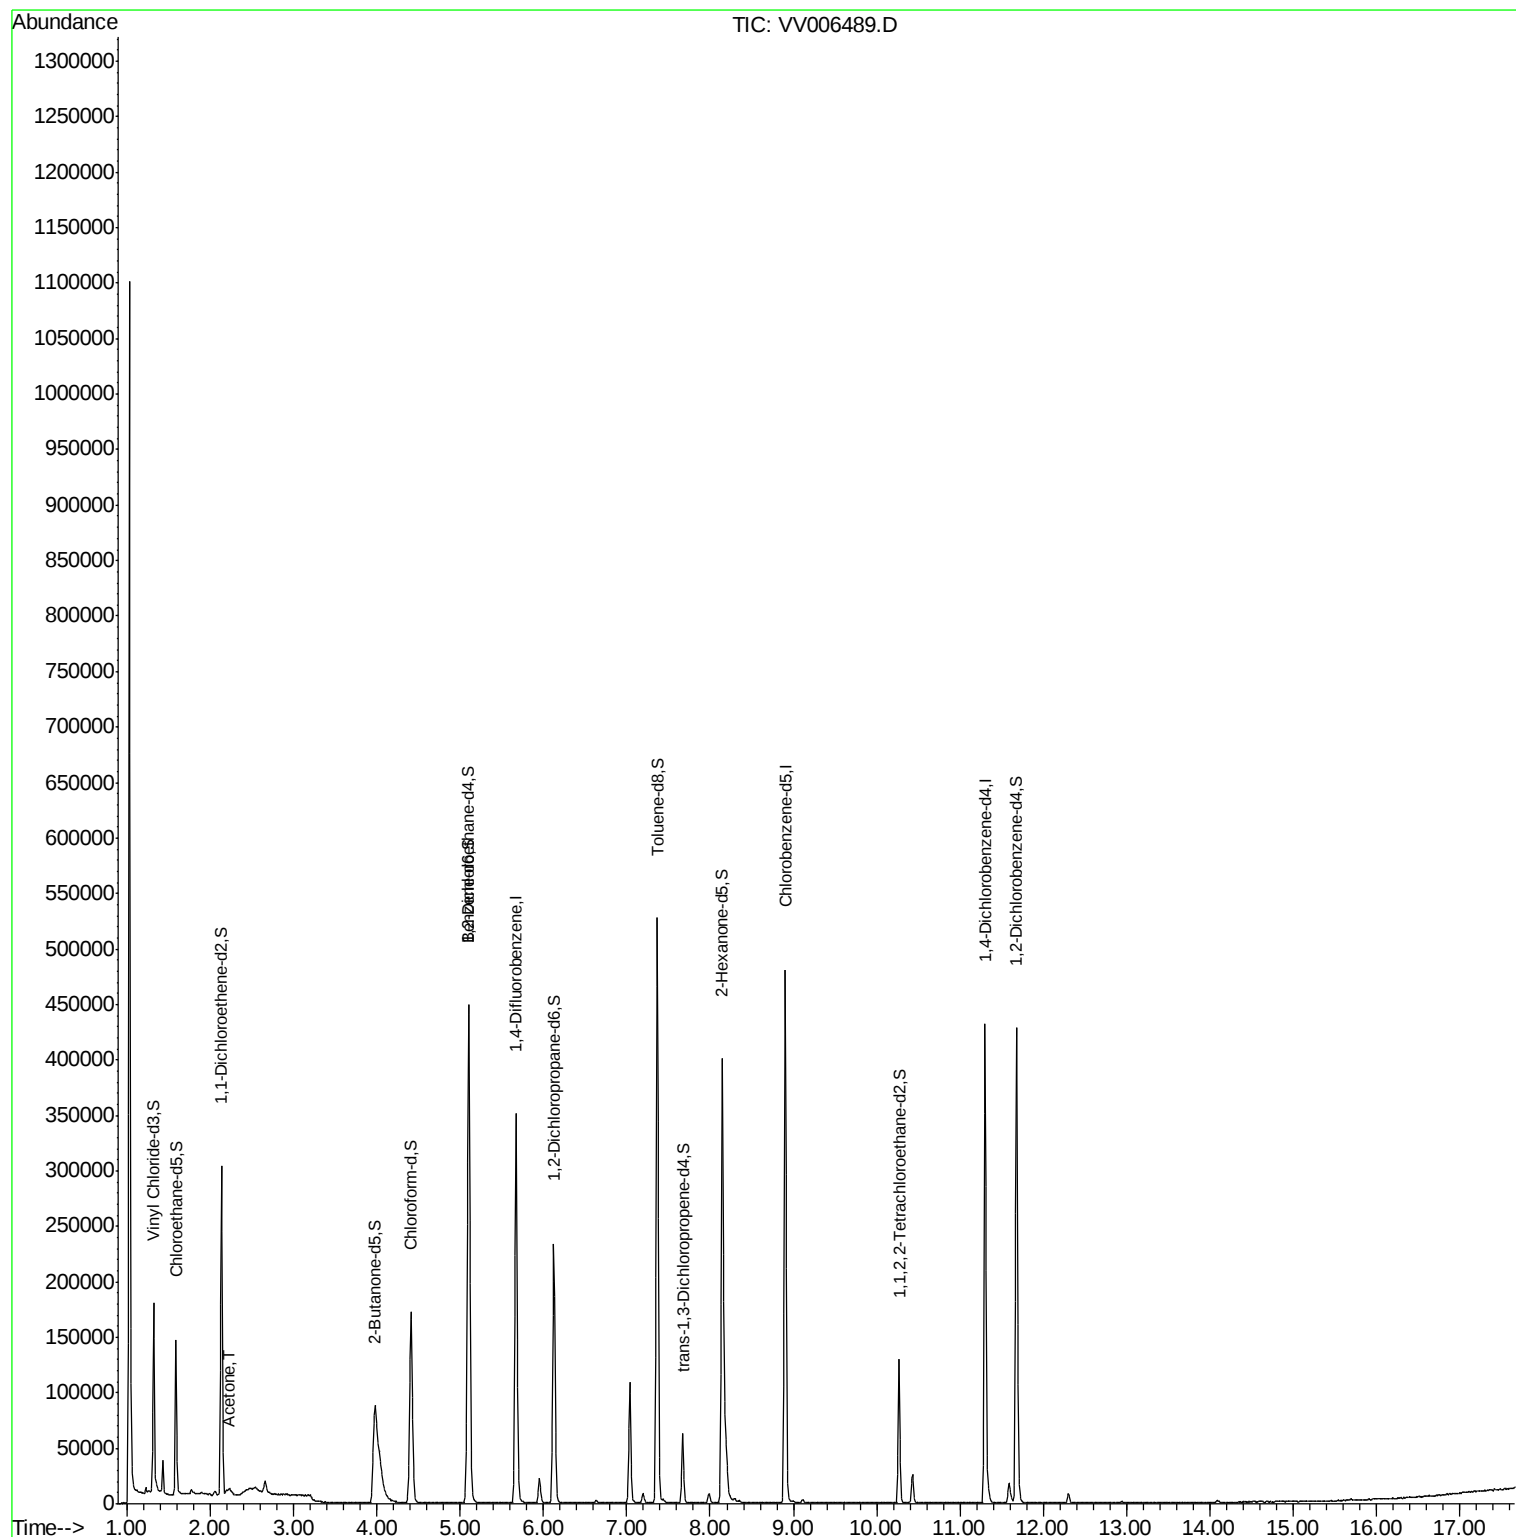

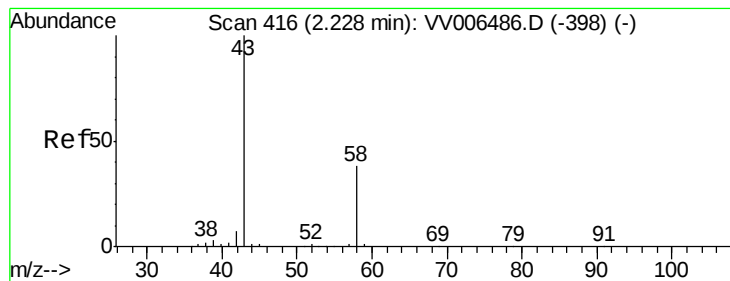

#13

Acetone

Concen: 4.75 ug/L

RT: 2.23 min Scan# 416

Delta R.T. 0.00 min

Lab File: VV006489.D

Acq: 28 Jun 2018 15:02

Instrument :
MSVOA_V
ClientSampleId :
C0ST2

Tot Ion: 43 Resp: 11172

Ion Ratio Lower Upper

43 100

58 32.7 0.0 77.4

