

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062818\
 Data File : VV006498.D
 Acq On : 28 Jun 2018 19:18
 Operator : SY/MD
 Sample : J3766-06
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ST6

Quant Time: Jun 29 04:20:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 29 03:51:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	302716	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	276548	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	119242	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	107161	5.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.60%
7) Chloroethane-d5	1.58	69	86870	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.40%
11) 1,1-Dichloroethene-d2	2.13	63	141487	4.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.20%
20) 2-Butanone-d5	3.98	46	199701	53.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.08%
24) Chloroform-d	4.41	84	165296	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.09	65	82027	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.10	84	371364	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
36) 1,2-Dichloropropane-d6	6.12	67	109442	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.37	98	331993	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
43) trans-1,3-Dichloropropene-	7.67	79	31369	3.97	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.40%
46) 2-Hexanone-d5	8.14	63	141585	45.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.44%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60862	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	114441	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.23	43	9356	4.09 ug/L	77
34) Trichloroethene	5.97	95	7063	0.30 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062818\
Data File : VV006498.D
Acq On : 28 Jun 2018 19:18
Operator : SY/MD
Sample : J3766-06
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ST6

Quant Time: Jun 29 04:20:36 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 29 03:51:20 2018
Response via : Initial Calibration

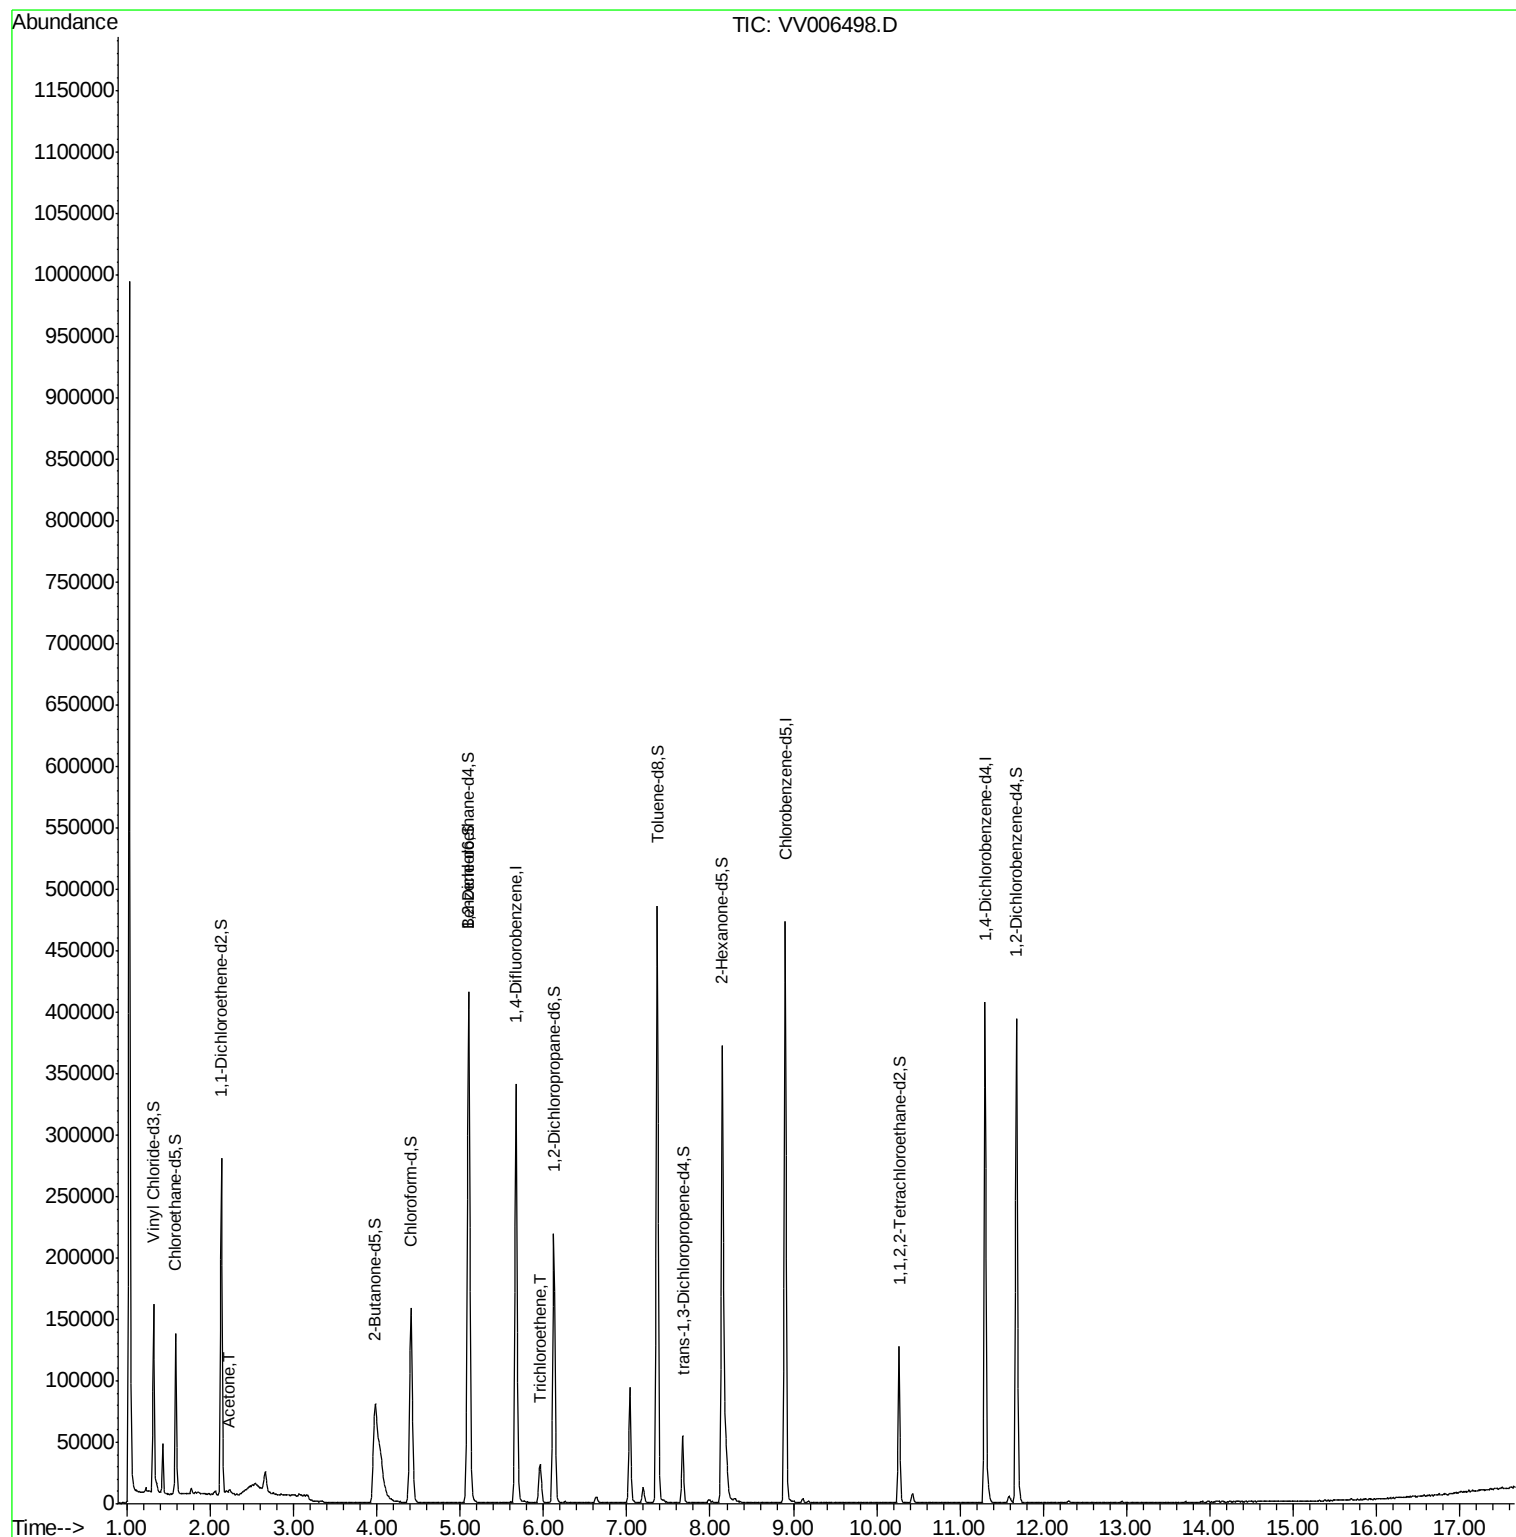

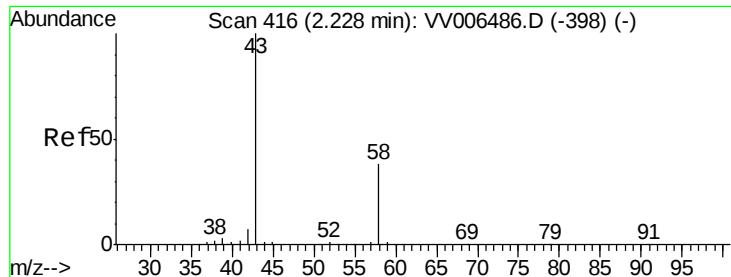

#13

Acetone

Concen: 4.09 ug/L

RT: 2.23 min Scan# 416

Delta R.T. 0.00 min

Lab File: VV006498.D

Acq: 28 Jun 2018 19:18





Instrument :
MSVOA_V
ClientSampleId :
C0ST6

Tot Ion: 43 Resp: 9356

Ion Ratio Lower Upper

43 100

58 24.7 0.0 77.4

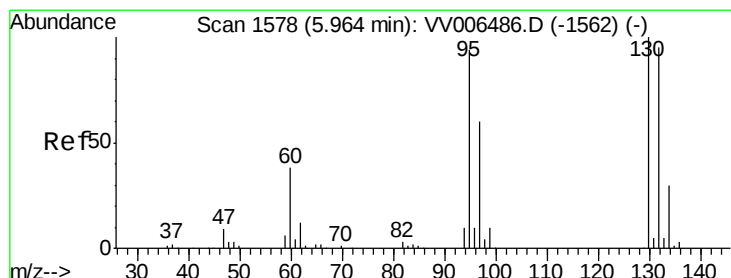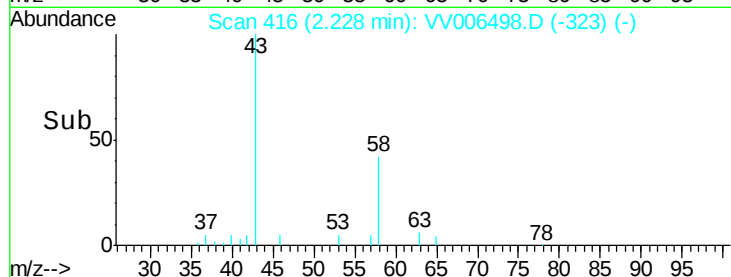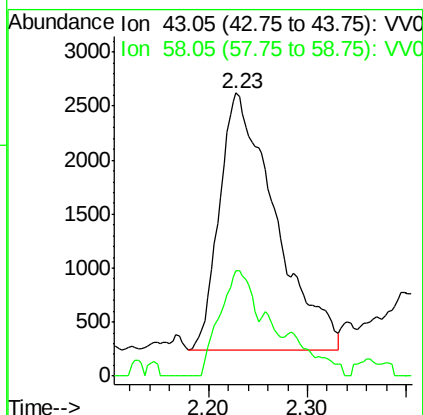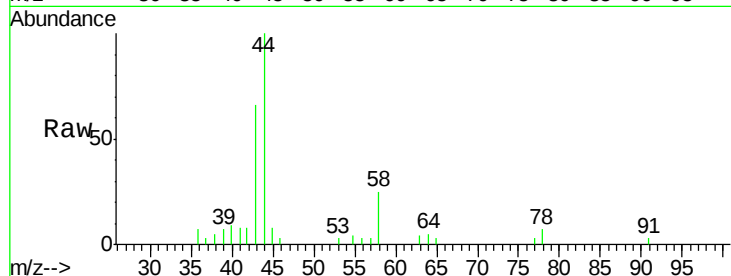

#34

Trichloroethene

Concen: 0.30 ug/L

RT: 5.97 min Scan# 1579

Delta R.T. 0.00 min

Lab File: VV006498.D

Acq: 28 Jun 2018 19:18

Tgt Ion: 95 Resp: 7063

Ion Ratio Lower Upper

95 100

97 70.4 44.6 82.8

132 118.7 70.1 130.1

130 121.1 73.3 136.1

