


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062818\
 Data File : VV006485.D
 Acq On : 28 Jun 2018 09:06
 Operator : SY/MD
 Sample : BFB62
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 29 23:41:20 2018

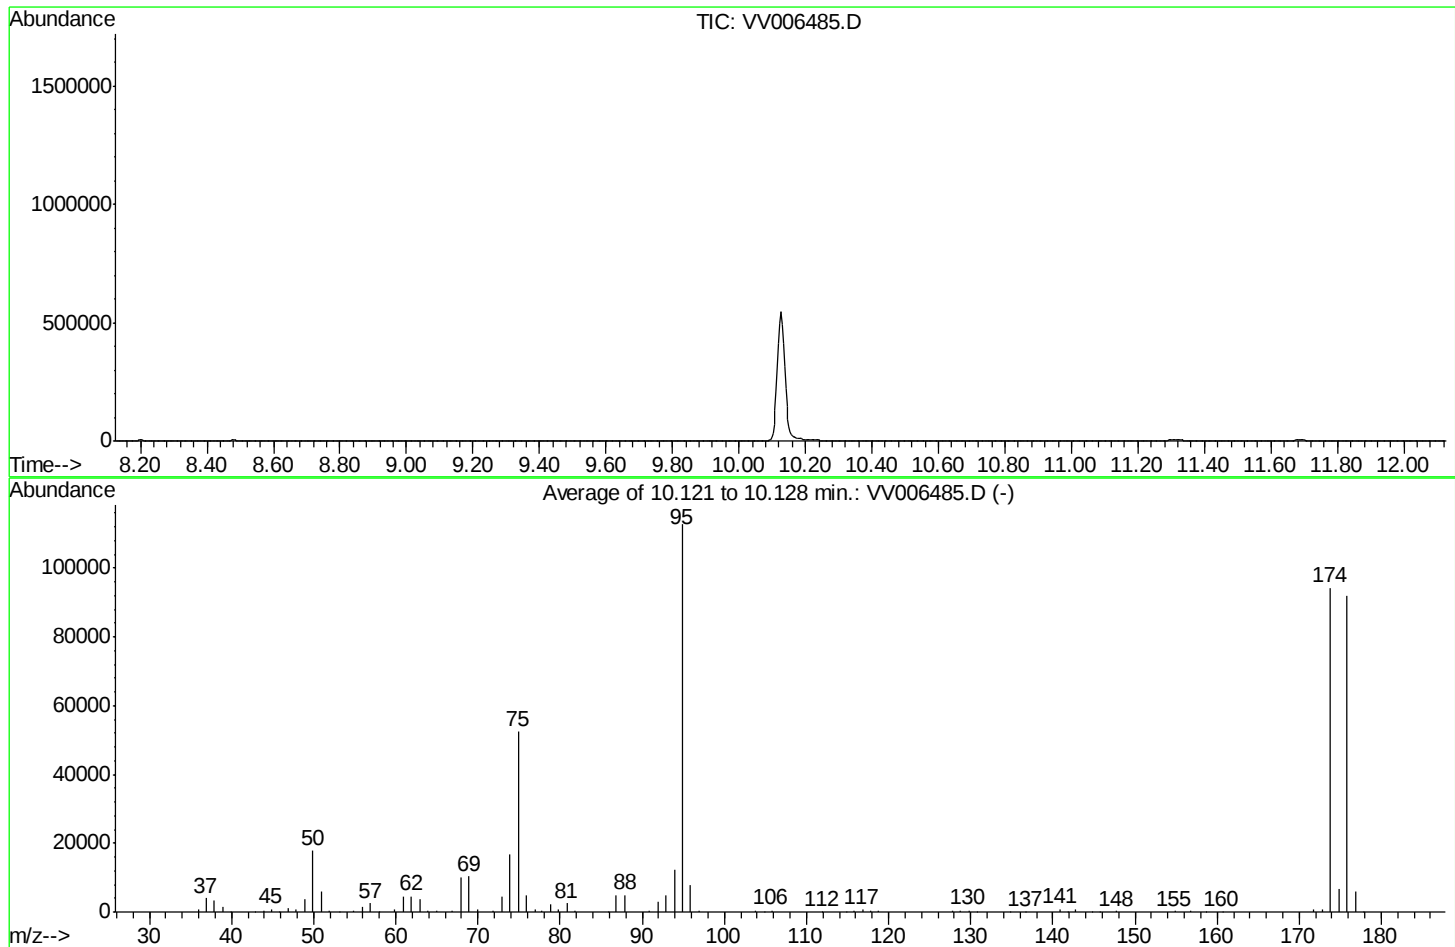

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	17813	PASS
75	95	30	80	46.4	52317	PASS
95	95	100	100	100.0	112736	PASS
96	95	5	9	6.9	7727	PASS
173	174	0.00	2	0.8	732	PASS
174	95	50	120	83.7	94370	PASS
175	174	5	9	7.1	6737	PASS
176	174	95	101	97.3	91776	PASS
177	176	5	9	6.6	6026	PASS

Scan 2859 (10.083 min): VV006485.D
BFB62

m/z	Abundance
35.90	426.0
37.90	217.0
39.80	140.0
43.80	565.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	1117.0
36.90	3756.0
37.90	3616.0
38.90	1399.0
39.80	268.0
42.80	140.0
43.90	1047.0
44.90	760.0
45.80	109.0
46.80	1253.0
47.80	589.0
48.90	3475.0
49.90	17104.0
50.90	5682.0
51.90	228.0
54.80	231.0
55.90	1261.0
56.90	2375.0
57.90	131.0
59.90	872.0
60.90	4217.0
61.90	4307.0
62.90	3420.0
63.90	416.0
64.90	399.0
66.80	335.0
67.90	9541.0
68.90	9891.0
69.90	818.0
71.80	512.0
72.90	4050.0
73.90	16112.0
74.90	49856.0
76.00	4474.0
76.90	717.0
77.80	502.0
78.80	2379.0
79.90	719.0
80.80	2451.0
81.80	553.0
85.80	130.0
86.90	4645.0
87.90	4827.0
90.80	376.0
91.90	2816.0
92.90	4677.0
93.90	11392.0
94.90	106976.0
95.90	7393.0
96.90	357.0
103.90	324.0
104.80	109.0
105.70	358.0
115.80	292.0
116.80	596.0
117.80	313.0
118.80	478.0
127.70	259.0
128.70	192.0
129.80	375.0
130.80	167.0
134.80	175.0
136.70	167.0
140.90	806.0
142.80	767.0
144.80	154.0
145.70	152.0
147.80	234.0
154.90	217.0
156.80	210.0
158.70	110.0
160.60	101.0
171.80	618.0
172.90	702.0
173.80	87320.0
174.90	6429.0
175.80	84616.0
176.90	5756.0
177.80	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	1167.0
36.90	4062.0
37.90	3837.0
38.90	1489.0
39.80	281.0
42.80	153.0
43.90	1071.0
44.90	780.0
45.90	101.0
46.90	1347.0
47.80	604.0
48.90	3772.0
49.90	18400.0
50.90	6062.0
51.90	250.0
53.10	104.0
54.80	267.0
55.90	1403.0
56.90	2533.0
57.90	151.0
59.90	912.0
60.90	4583.0
61.90	4652.0
62.90	3716.0
63.90	443.0
64.90	490.0
66.80	356.0
67.90	10342.0
68.90	10607.0
69.90	905.0
71.80	535.0
72.90	4437.0
73.90	17344.0
74.90	54016.0
75.90	4845.0
76.90	721.0
77.80	547.0
78.80	2465.0
79.80	854.0
80.80	2643.0
81.80	579.0
85.80	120.0
86.80	4983.0
87.90	5141.0
90.80	393.0
91.90	3108.0
92.90	4877.0
93.90	12654.0
94.90	116344.0
95.90	8015.0
96.90	369.0
103.80	363.0
104.80	116.0
105.80	388.0
114.90	103.0
115.80	318.0
116.80	695.0
117.80	333.0
118.80	548.0
127.70	287.0
128.70	221.0
129.80	425.0
130.80	195.0
134.80	167.0
136.70	188.0
140.90	879.0
141.80	103.0
142.80	827.0
144.70	159.0
145.70	171.0
147.80	245.0
154.90	237.0
156.80	229.0
160.60	116.0
171.80	635.0
172.90	763.0
173.80	97280.0
174.80	6993.0
175.80	94752.0
176.90	6211.0
177.80	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.90	1187.0
36.90	3970.0
37.90	3702.0
38.90	1470.0
39.90	289.0
42.80	146.0
43.90	1018.0
44.80	764.0
46.90	1312.0
47.80	597.0
48.90	3740.0
49.90	17936.0
50.90	5780.0
51.90	246.0
54.80	284.0
55.90	1395.0
56.90	2474.0
57.90	142.0
59.90	823.0
60.90	4487.0
61.90	4570.0
62.90	3671.0
63.90	449.0
64.90	536.0
66.80	324.0
67.90	10220.0
68.90	10467.0
69.90	882.0
71.80	536.0
72.90	4427.0
73.90	17256.0
74.90	53080.0
75.90	4739.0
76.90	692.0
77.80	553.0
78.80	2364.0
79.80	899.0
80.80	2585.0
81.80	562.0
85.80	131.0
86.80	4950.0
87.90	4954.0
90.80	345.0
91.90	3027.0
92.90	4636.0
93.90	12842.0
94.90	114888.0
95.90	7773.0
96.90	286.0
103.80	340.0
104.80	145.0
105.80	390.0
111.90	104.0
115.80	310.0
116.80	679.0
117.90	326.0
118.80	551.0
127.80	320.0
128.80	215.0
129.80	444.0
130.80	200.0
134.70	158.0
136.70	193.0
140.90	846.0
141.90	104.0
142.80	862.0
144.70	151.0
145.70	193.0
147.80	250.0
154.90	247.0
156.80	225.0
160.60	110.0
171.80	624.0
172.90	732.0
173.80	98512.0
174.90	6791.0
175.80	95960.0
176.90	6113.0
177.80	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62