


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062918\
Data File : VV006500.D
Acq On : 29 Jun 2018 10:06
Operator : SY/MD
Sample : BFB63
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jun 30 02:15:06 2018

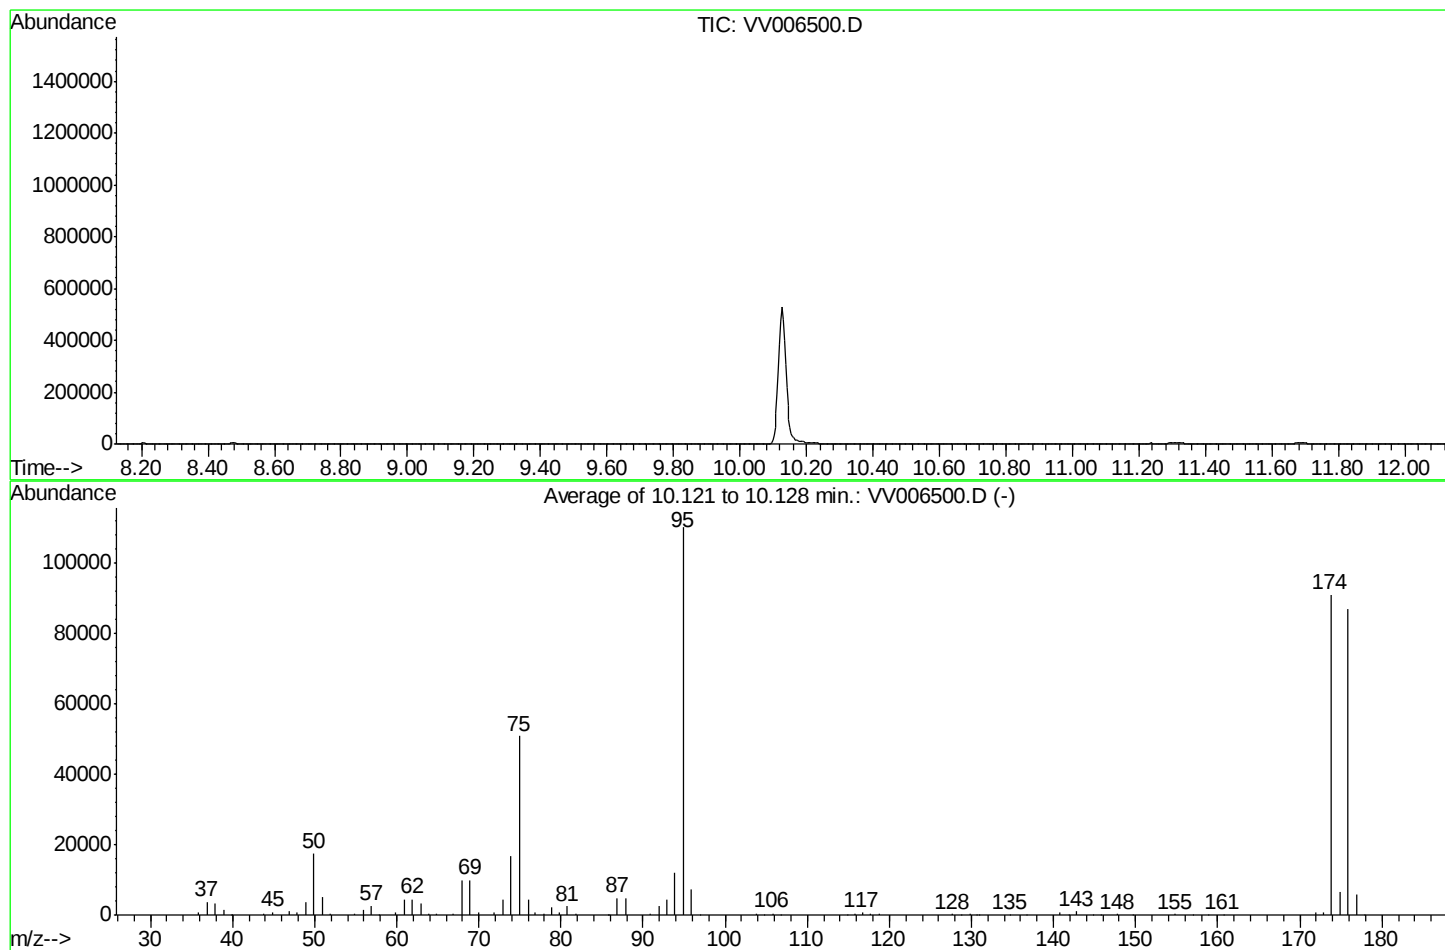

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	17469	PASS
75	95	30	80	46.2	50962	PASS
95	95	100	100	100.0	110240	PASS
96	95	5	9	6.5	7203	PASS
173	174	0.00	2	0.8	688	PASS
174	95	50	120	82.7	91130	PASS
175	174	5	9	7.0	6400	PASS
176	174	95	101	95.5	87016	PASS
177	176	5	9	6.8	5940	PASS

Scan 2858 (10.080 min): vv006500.D
BFB63

m/z	Abundance
39.90	172.0
43.80	666.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.90	684.0
36.90	3528.0
37.90	3080.0
38.90	1254.0
39.80	175.0
40.00	177.0
43.80	1056.0
44.90	752.0
46.90	1144.0
47.80	571.0
48.90	3618.0
49.90	16664.0
50.90	5039.0
52.00	180.0
54.80	228.0
55.90	1343.0
56.90	2493.0
57.80	121.0
59.90	835.0
60.90	4230.0
61.90	4348.0
62.90	3151.0
63.90	361.0
64.90	446.0
66.80	284.0
67.90	9361.0
68.90	9440.0
69.90	830.0
71.90	572.0
72.90	4200.0
73.90	15942.0
74.90	47800.0
76.00	4165.0
76.90	578.0
78.00	355.0
78.80	2120.0
79.80	623.0
80.80	2266.0
81.70	520.0
85.70	153.0
86.80	4575.0
87.90	4385.0
90.80	308.0
91.90	2502.0
92.90	4132.0
93.90	11243.0
94.90	103520.0
95.90	6925.0
96.90	146.0
103.80	333.0
105.80	386.0
106.70	130.0
114.80	119.0
115.80	276.0
116.70	597.0
117.70	375.0
118.80	442.0
127.70	337.0
128.80	158.0
129.80	328.0
130.70	123.0
134.70	167.0
136.70	114.0
140.80	731.0
141.80	128.0
142.80	946.0
144.80	142.0
145.80	110.0
147.80	213.0
154.80	216.0
156.90	122.0
160.70	101.0
172.00	613.0
172.90	650.0
173.80	82832.0
174.90	6027.0
175.80	79208.0
176.90	5434.0
177.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.90	726.0
36.90	3850.0
37.90	3356.0
38.90	1348.0
40.00	226.0
43.90	1051.0
44.90	890.0
46.90	1222.0
47.80	584.0
48.90	3935.0
49.90	18080.0
50.90	5329.0
51.90	231.0
54.80	253.0
55.90	1406.0
56.90	2649.0
57.80	136.0
59.90	934.0
60.90	4495.0
61.90	4674.0
62.90	3491.0
63.90	394.0
64.90	480.0
66.80	329.0
67.90	10267.0
68.90	10308.0
69.90	836.0
71.90	580.0
72.90	4578.0
73.90	17440.0
74.90	52624.0
76.00	4537.0
76.80	623.0
77.90	407.0
78.80	2290.0
79.80	711.0
80.80	2485.0
81.70	561.0
85.90	149.0
86.90	5066.0
87.80	4964.0
90.80	381.0
91.90	2682.0
92.90	4526.0
93.90	12284.0
94.90	113936.0
95.90	7440.0
96.90	177.0
103.80	381.0
104.70	127.0
105.80	406.0
106.70	137.0
114.80	132.0
115.90	307.0
116.70	635.0
117.70	427.0
118.80	469.0
127.70	372.0
128.80	165.0
129.80	349.0
130.70	149.0
134.80	187.0
136.70	113.0
140.80	810.0
141.90	149.0
142.80	1041.0
144.80	153.0
145.80	140.0
147.80	230.0
149.70	101.0
154.80	242.0
156.90	151.0
158.80	109.0
160.70	105.0
171.90	728.0
172.90	717.0
173.80	93880.0
174.90	6564.0
175.80	89840.0
176.90	6121.0
177.80	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.90	721.0
36.90	3839.0
37.90	3280.0
38.90	1341.0
39.90	261.0
43.90	1015.0
44.90	879.0
46.90	1168.0
47.80	537.0
48.90	3890.0
49.90	17664.0
50.90	5176.0
51.90	253.0
54.90	287.0
55.90	1378.0
56.90	2607.0
57.90	149.0
59.90	909.0
60.90	4470.0
61.90	4501.0
62.90	3517.0
63.90	394.0
64.90	526.0
66.80	342.0
67.90	10163.0
68.90	10271.0
69.90	810.0
71.90	531.0
72.90	4460.0
73.90	17016.0
74.90	52464.0
76.00	4474.0
76.80	598.0
77.90	446.0
78.80	2282.0
79.80	775.0
80.80	2433.0
81.80	562.0
85.90	150.0
86.90	5073.0
87.80	4945.0
90.80	389.0
91.90	2693.0
92.90	4544.0
93.90	12186.0
94.90	113264.0
95.90	7245.0
96.90	208.0
103.80	403.0
104.80	153.0
105.80	416.0
106.70	108.0
114.80	102.0
115.90	279.0
116.80	616.0
117.80	419.0
118.80	431.0
127.70	342.0
128.80	159.0
129.80	330.0
130.90	159.0
134.80	195.0
136.70	121.0
140.80	816.0
141.90	136.0
142.80	1016.0
144.80	128.0
145.80	142.0
147.80	204.0
149.70	106.0
154.80	242.0
156.90	153.0
158.80	105.0
171.80	771.0
172.90	698.0
173.80	96680.0
174.90	6610.0
175.80	92000.0
176.90	6267.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63