

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017230.D
 Acq On : 29 Jun 2020 11:00
 Operator : SY/MD
 Sample : L3118-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	80	rBV	147170	153992	11.15%	1.455%
2	1.579	145	152	164	rBV	118068	137290	9.94%	1.297%
3	2.122	312	321	346	rVB	288391	444187	32.17%	4.196%
4	2.505	438	440	442	rBV2	1589	793	0.06%	0.007%
5	2.592	465	467	470	rVB3	1080	553	0.04%	0.005%
6	2.611	471	473	477	rBV5	1111	1002	0.07%	0.009%
7	2.749	513	516	518	rVB3	1216	635	0.05%	0.006%
8	3.138	635	637	639	rBV2	759	415	0.03%	0.004%
9	3.151	639	641	643	rBV3	1177	474	0.03%	0.004%
10	3.280	675	681	682	rBV5	909	775	0.06%	0.007%
11	3.341	697	700	703	rBV3	1069	789	0.06%	0.007%
12	3.486	743	745	751	rVB6	1675	1502	0.11%	0.014%
13	3.508	751	752	755	rBV2	839	451	0.03%	0.004%
14	3.537	759	761	764	rVV3	991	571	0.04%	0.005%
15	3.650	794	796	798	rVB3	1026	415	0.03%	0.004%
16	3.717	811	817	820	rBV6	1381	1346	0.10%	0.013%
17	3.907	866	876	912	rBV	95323	281490	20.39%	2.659%
18	4.261	982	986	987	rBV2	1859	1164	0.08%	0.011%
19	4.376	1004	1022	1046	rBV	230125	574125	41.58%	5.423%
20	4.553	1075	1077	1079	rBV4	1152	529	0.04%	0.005%
21	4.640	1102	1104	1108	rVB3	1003	711	0.05%	0.007%
22	4.814	1155	1158	1160	rBV3	556	458	0.03%	0.004%
23	4.961	1202	1204	1206	rBV3	1278	629	0.05%	0.006%
24	5.074	1222	1239	1261	rBV2	535720	1380742	100.00%	13.042%
25	5.386	1333	1336	1338	rBV4	1277	751	0.05%	0.007%
26	5.450	1352	1356	1357	rBV2	1303	874	0.06%	0.008%
27	5.476	1362	1364	1365	rBV2	1059	516	0.04%	0.005%
28	5.566	1390	1392	1398	rVB7	1027	848	0.06%	0.008%
29	5.640	1400	1415	1440	rBV	437692	874081	63.31%	8.256%
30	5.929	1495	1505	1517	rBV8	11063	23478	1.70%	0.222%
31	6.093	1542	1556	1578	rBV	310502	632246	45.79%	5.972%
32	6.309	1621	1623	1627	rBV4	1332	887	0.06%	0.008%
33	6.331	1627	1630	1632	rVV4	1153	563	0.04%	0.005%
34	6.637	1720	1725	1727	rBV4	2065	1859	0.13%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017230.D
 Acq On : 29 Jun 2020 11:00
 Operator : SY/MD
 Sample : L3118-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.743	1756	1758	1761	rBV3	852	584	0.04%	0.006%
36	6.833	1784	1786	1791	rVB5	839	454	0.03%	0.004%
37	7.006	1830	1840	1859	rBV	179535	319384	23.13%	3.017%
38	7.338	1931	1943	1962	rBV	645835	1110043	80.39%	10.485%
39	7.579	2016	2018	2021	rBV3	922	497	0.04%	0.005%
40	7.643	2027	2038	2057	rBV	133024	224145	16.23%	2.117%
41	7.749	2069	2071	2073	rBV3	824	406	0.03%	0.004%
42	7.916	2119	2123	2125	rBV3	1060	849	0.06%	0.008%
43	8.106	2172	2182	2205	rBV	340628	607009	43.96%	5.734%
44	8.379	2266	2267	2271	rBV4	948	554	0.04%	0.005%
45	8.518	2308	2310	2312	rVB2	1154	427	0.03%	0.004%
46	8.540	2312	2317	2320	rBV6	1966	1837	0.13%	0.017%
47	8.829	2401	2407	2408	rBV4	1193	1162	0.08%	0.011%
48	8.871	2409	2420	2442	rVV	635171	1041901	75.46%	9.841%
49	9.032	2468	2470	2472	rBV4	1203	702	0.05%	0.007%
50	9.083	2481	2486	2488	rBV3	1706	1587	0.11%	0.015%
51	9.116	2492	2496	2498	rBV5	1583	1228	0.09%	0.012%
52	9.145	2503	2505	2507	rBV2	1159	553	0.04%	0.005%
53	9.238	2532	2534	2537	rVB4	1286	603	0.04%	0.006%
54	9.669	2665	2668	2671	rBV2	814	631	0.05%	0.006%
55	9.691	2671	2675	2677	rBV3	1462	1161	0.08%	0.011%
56	9.762	2694	2697	2701	rVB4	1125	840	0.06%	0.008%
57	9.781	2701	2703	2708	rVB3	1451	1027	0.07%	0.010%
58	9.807	2708	2711	2712	rBV2	1184	717	0.05%	0.007%
59	9.913	2740	2744	2747	rBV5	1075	891	0.06%	0.008%
60	10.032	2777	2781	2784	rBV4	1055	784	0.06%	0.007%
61	10.051	2784	2787	2789	rVB2	969	450	0.03%	0.004%
62	10.116	2805	2807	2808	rBV	886	462	0.03%	0.004%
63	10.145	2813	2816	2820	rVB4	1460	1040	0.08%	0.010%
64	10.238	2832	2845	2863	rBV	411254	646322	46.81%	6.105%
65	10.395	2891	2894	2898	rBV4	1186	1031	0.07%	0.010%
66	10.450	2906	2911	2914	rBV8	1019	1177	0.09%	0.011%
67	10.534	2935	2937	2941	rVB4	1299	819	0.06%	0.008%
68	10.572	2945	2949	2953	rBV5	1078	793	0.06%	0.007%
69	10.598	2955	2957	2959	rBV3	1211	504	0.04%	0.005%
70	10.643	2967	2971	2973	rBV5	1053	766	0.06%	0.007%
71	10.714	2988	2993	2995	rVB3	1140	827	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017230.D
 Acq On : 29 Jun 2020 11:00
 Operator : SY/MD
 Sample : L3118-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.765	3005	3009	3010	rBV4	929	493	0.04%	0.005%
73	10.923	3056	3058	3060	rBV3	1604	762	0.06%	0.007%
74	11.090	3108	3110	3115	rVV4	832	613	0.04%	0.006%
75	11.167	3132	3134	3136	rBV3	823	493	0.04%	0.005%
76	11.270	3154	3166	3186	rBV	652366	1002980	72.64%	9.474%
77	11.466	3225	3227	3228	rBV	1119	528	0.04%	0.005%
78	11.527	3241	3246	3252	rVB5	1449	1837	0.13%	0.017%
79	11.566	3256	3258	3261	rBV3	1361	693	0.05%	0.007%
80	11.646	3270	3283	3304	rBV	684287	1069368	77.45%	10.101%
81	11.759	3316	3318	3321	rBV4	964	558	0.04%	0.005%
82	11.977	3381	3386	3391	rBV6	1606	1573	0.11%	0.015%
83	12.000	3391	3393	3395	rVB2	974	401	0.03%	0.004%
84	12.151	3438	3440	3441	rBV2	917	437	0.03%	0.004%
85	12.247	3467	3470	3473	rBV2	1293	841	0.06%	0.008%
86	12.273	3476	3478	3480	rVV2	936	452	0.03%	0.004%
87	12.289	3480	3483	3486	rVV3	835	467	0.03%	0.004%
88	12.575	3567	3572	3573	rBV4	1385	997	0.07%	0.009%
89	12.771	3630	3633	3636	rBV3	892	806	0.06%	0.008%
90	12.807	3642	3644	3646	rBV3	881	544	0.04%	0.005%
91	13.051	3718	3720	3723	rBV3	765	549	0.04%	0.005%
92	13.067	3723	3725	3729	rVV3	1273	779	0.06%	0.007%
93	13.212	3767	3770	3773	rBV5	980	718	0.05%	0.007%
94	13.382	3821	3823	3827	rVB4	1527	779	0.06%	0.007%
95	13.704	3920	3923	3924	rBV3	1134	631	0.05%	0.006%
96	13.730	3927	3931	3932	rBV3	769	488	0.04%	0.005%
97	13.855	3968	3970	3973	rVB4	1345	403	0.03%	0.004%
98	13.948	3997	3999	4001	rBV2	1272	429	0.03%	0.004%
99	14.022	4020	4022	4025	rBV2	1101	795	0.06%	0.008%
100	14.318	4109	4114	4116	rBV4	1376	1259	0.09%	0.012%


Sum of corrected areas: 10586981

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017230.D
Acq On : 29 Jun 2020 11:00
Operator : SY/MD
Sample : L3118-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

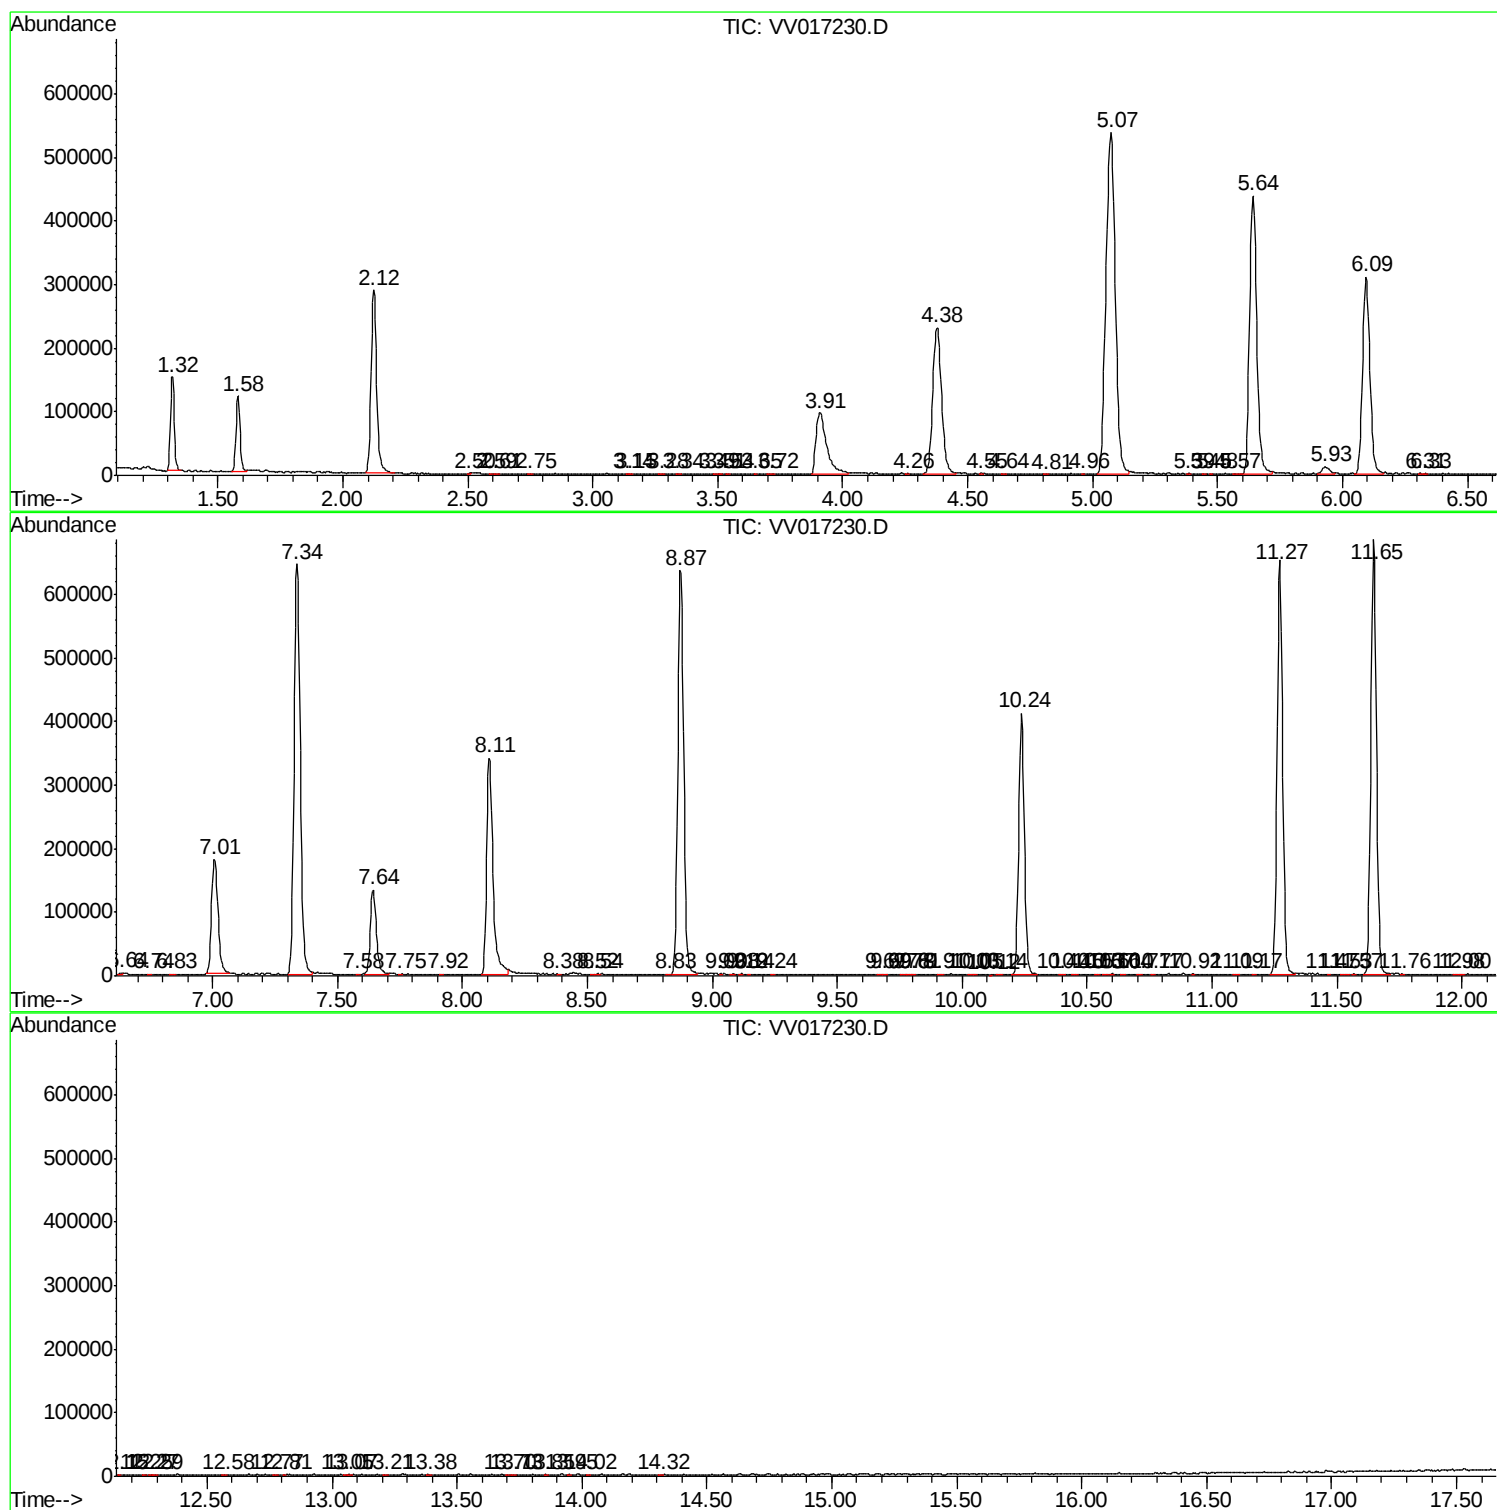

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017230.D
Acq On : 29 Jun 2020 11:00
Operator : SY/MD
Sample : L3118-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017230.D
Acq On : 29 Jun 2020 11:00
Operator : SY/MD
Sample : L3118-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc