

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017234.D
 Acq On : 29 Jun 2020 12:33
 Operator : SY/MD
 Sample : L3133-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	153468	164059	11.79%	1.554%
2	1.579	145	152	162	rBV	129171	143398	10.31%	1.358%
3	2.122	312	321	346	rVB	295540	448305	32.22%	4.245%
4	2.251	359	361	364	rBV4	1189	719	0.05%	0.007%
5	2.460	423	426	429	rBV3	1135	745	0.05%	0.007%
6	2.659	486	488	489	rBV	677	269	0.02%	0.003%
7	2.736	510	512	514	rVB3	782	181	0.01%	0.002%
8	2.826	538	540	542	rBV2	751	420	0.03%	0.004%
9	2.952	577	579	580	rBV2	1224	401	0.03%	0.004%
10	3.061	611	613	615	rBV2	1151	728	0.05%	0.007%
11	3.280	679	681	682	rBV	645	265	0.02%	0.003%
12	3.373	707	710	712	rBV3	936	494	0.04%	0.005%
13	3.453	732	735	737	rBV3	1347	911	0.07%	0.009%
14	3.550	763	765	767	rBV3	845	411	0.03%	0.004%
15	3.563	767	769	771	rVV3	824	324	0.02%	0.003%
16	3.601	779	781	784	rBV3	1121	527	0.04%	0.005%
17	3.643	792	794	795	rBV2	852	335	0.02%	0.003%
18	3.679	801	805	810	rBV6	1381	1299	0.09%	0.012%
19	3.823	849	850	853	rVB3	721	275	0.02%	0.003%
20	3.910	866	877	904	rBV	95408	277635	19.95%	2.629%
21	4.264	983	987	989	rBV3	1069	856	0.06%	0.008%
22	4.376	1004	1022	1044	rBV2	235061	580948	41.75%	5.501%
23	4.566	1079	1081	1083	rVB	1320	461	0.03%	0.004%
24	4.585	1083	1087	1089	rBV2	1502	1135	0.08%	0.011%
25	4.666	1108	1112	1115	rBV4	943	725	0.05%	0.007%
26	4.714	1124	1127	1129	rBV3	1069	712	0.05%	0.007%
27	4.820	1156	1160	1163	rBV5	1470	1270	0.09%	0.012%
28	4.884	1177	1180	1183	rVB3	1524	1009	0.07%	0.010%
29	4.945	1194	1199	1202	rBV7	1720	1686	0.12%	0.016%
30	4.978	1207	1209	1213	rVB4	1713	998	0.07%	0.009%
31	5.074	1220	1239	1263	rBV2	538152	1391405	100.00%	13.176%
32	5.640	1401	1415	1440	rBV	436072	866919	62.31%	8.209%
33	5.929	1495	1505	1520	rBV9	10557	22436	1.61%	0.212%
34	6.093	1543	1556	1579	rBV	307174	625872	44.98%	5.927%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017234.D
 Acq On : 29 Jun 2020 12:33
 Operator : SY/MD
 Sample : L3133-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.820	1781	1782	1784	rBV2	950	429	0.03%	0.004%
36	6.891	1802	1804	1811	rVB7	1162	1083	0.08%	0.010%
37	6.932	1815	1817	1818	rBV2	493	186	0.01%	0.002%
38	7.006	1829	1840	1860	rBV	182994	325061	23.36%	3.078%
39	7.338	1931	1943	1965	rBV	653406	1120655	80.54%	10.612%
40	7.585	2018	2020	2022	rBV	1505	998	0.07%	0.009%
41	7.643	2028	2038	2061	rVB	132545	227239	16.33%	2.152%
42	7.926	2120	2126	2128	rBV6	1547	1513	0.11%	0.014%
43	8.109	2173	2183	2208	rBV	326172	581859	41.82%	5.510%
44	8.675	2357	2359	2361	rVB3	835	172	0.01%	0.002%
45	8.691	2361	2364	2366	rBV4	1108	655	0.05%	0.006%
46	8.874	2409	2421	2443	rBV	639240	1033239	74.26%	9.784%
47	9.112	2490	2495	2499	rVB3	1863	1717	0.12%	0.016%
48	9.132	2499	2501	2507	rBV7	1657	1606	0.12%	0.015%
49	9.289	2548	2550	2554	rVB5	1823	865	0.06%	0.008%
50	9.405	2583	2586	2588	rBV2	1392	843	0.06%	0.008%
51	9.804	2706	2710	2711	rBV3	1402	1077	0.08%	0.010%
52	9.839	2716	2721	2724	rBV6	1282	1464	0.11%	0.014%
53	9.926	2745	2748	2749	rBV2	1291	651	0.05%	0.006%
54	10.128	2810	2811	2813	rBV	609	157	0.01%	0.001%
55	10.145	2813	2816	2819	rBV5	1479	1075	0.08%	0.010%
56	10.167	2821	2823	2827	rVB2	1146	592	0.04%	0.006%
57	10.186	2827	2829	2832	rBV4	1167	598	0.04%	0.006%
58	10.238	2832	2845	2861	rBV	406698	642243	46.16%	6.082%
59	10.389	2890	2892	2894	rBV3	959	642	0.05%	0.006%
60	10.418	2899	2901	2904	rVB4	1728	880	0.06%	0.008%
61	10.537	2933	2938	2941	rBV8	1353	1126	0.08%	0.011%
62	10.585	2950	2953	2958	rBV7	1636	1444	0.10%	0.014%
63	10.614	2958	2962	2963	rBV2	929	586	0.04%	0.006%
64	10.698	2986	2988	2989	rBV2	660	233	0.02%	0.002%
65	10.765	3006	3009	3013	rBV4	1056	958	0.07%	0.009%
66	10.919	3054	3057	3058	rBV2	841	466	0.03%	0.004%
67	10.997	3079	3081	3083	rBV3	970	471	0.03%	0.004%
68	11.270	3154	3166	3183	rBV	650670	991355	71.25%	9.388%
69	11.466	3224	3227	3228	rBV3	1051	662	0.05%	0.006%
70	11.646	3271	3283	3298	rBV	688672	1064838	76.53%	10.083%
71	11.948	3375	3377	3380	rBV3	1392	967	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017234.D
 Acq On : 29 Jun 2020 12:33
 Operator : SY/MD
 Sample : L3133-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.000	3390	3393	3395	rBV3	1306	849	0.06%	0.008%
73	12.032	3401	3403	3405	rBV2	1320	745	0.05%	0.007%
74	12.157	3440	3442	3447	rVB4	1512	964	0.07%	0.009%
75	12.469	3537	3539	3540	rBV	948	454	0.03%	0.004%
76	12.543	3560	3562	3563	rBV	963	422	0.03%	0.004%
77	13.022	3709	3711	3713	rBV2	713	339	0.02%	0.003%
78	13.160	3748	3754	3757	rBV5	1721	1816	0.13%	0.017%
79	13.437	3838	3840	3843	rVB4	1477	692	0.05%	0.007%
80	13.456	3843	3846	3849	rBV3	1268	753	0.05%	0.007%
81	13.611	3889	3894	3898	rBV6	1525	1828	0.13%	0.017%
82	13.903	3983	3985	3988	rBV4	1061	517	0.04%	0.005%
83	14.115	4049	4051	4053	rVB2	1237	471	0.03%	0.004%
84	14.128	4053	4055	4057	rBV3	1353	706	0.05%	0.007%
85	15.193	4383	4386	4388	rBV3	1562	912	0.07%	0.009%


Sum of corrected areas: 10560206

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017234.D
Acq On : 29 Jun 2020 12:33
Operator : SY/MD
Sample : L3133-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

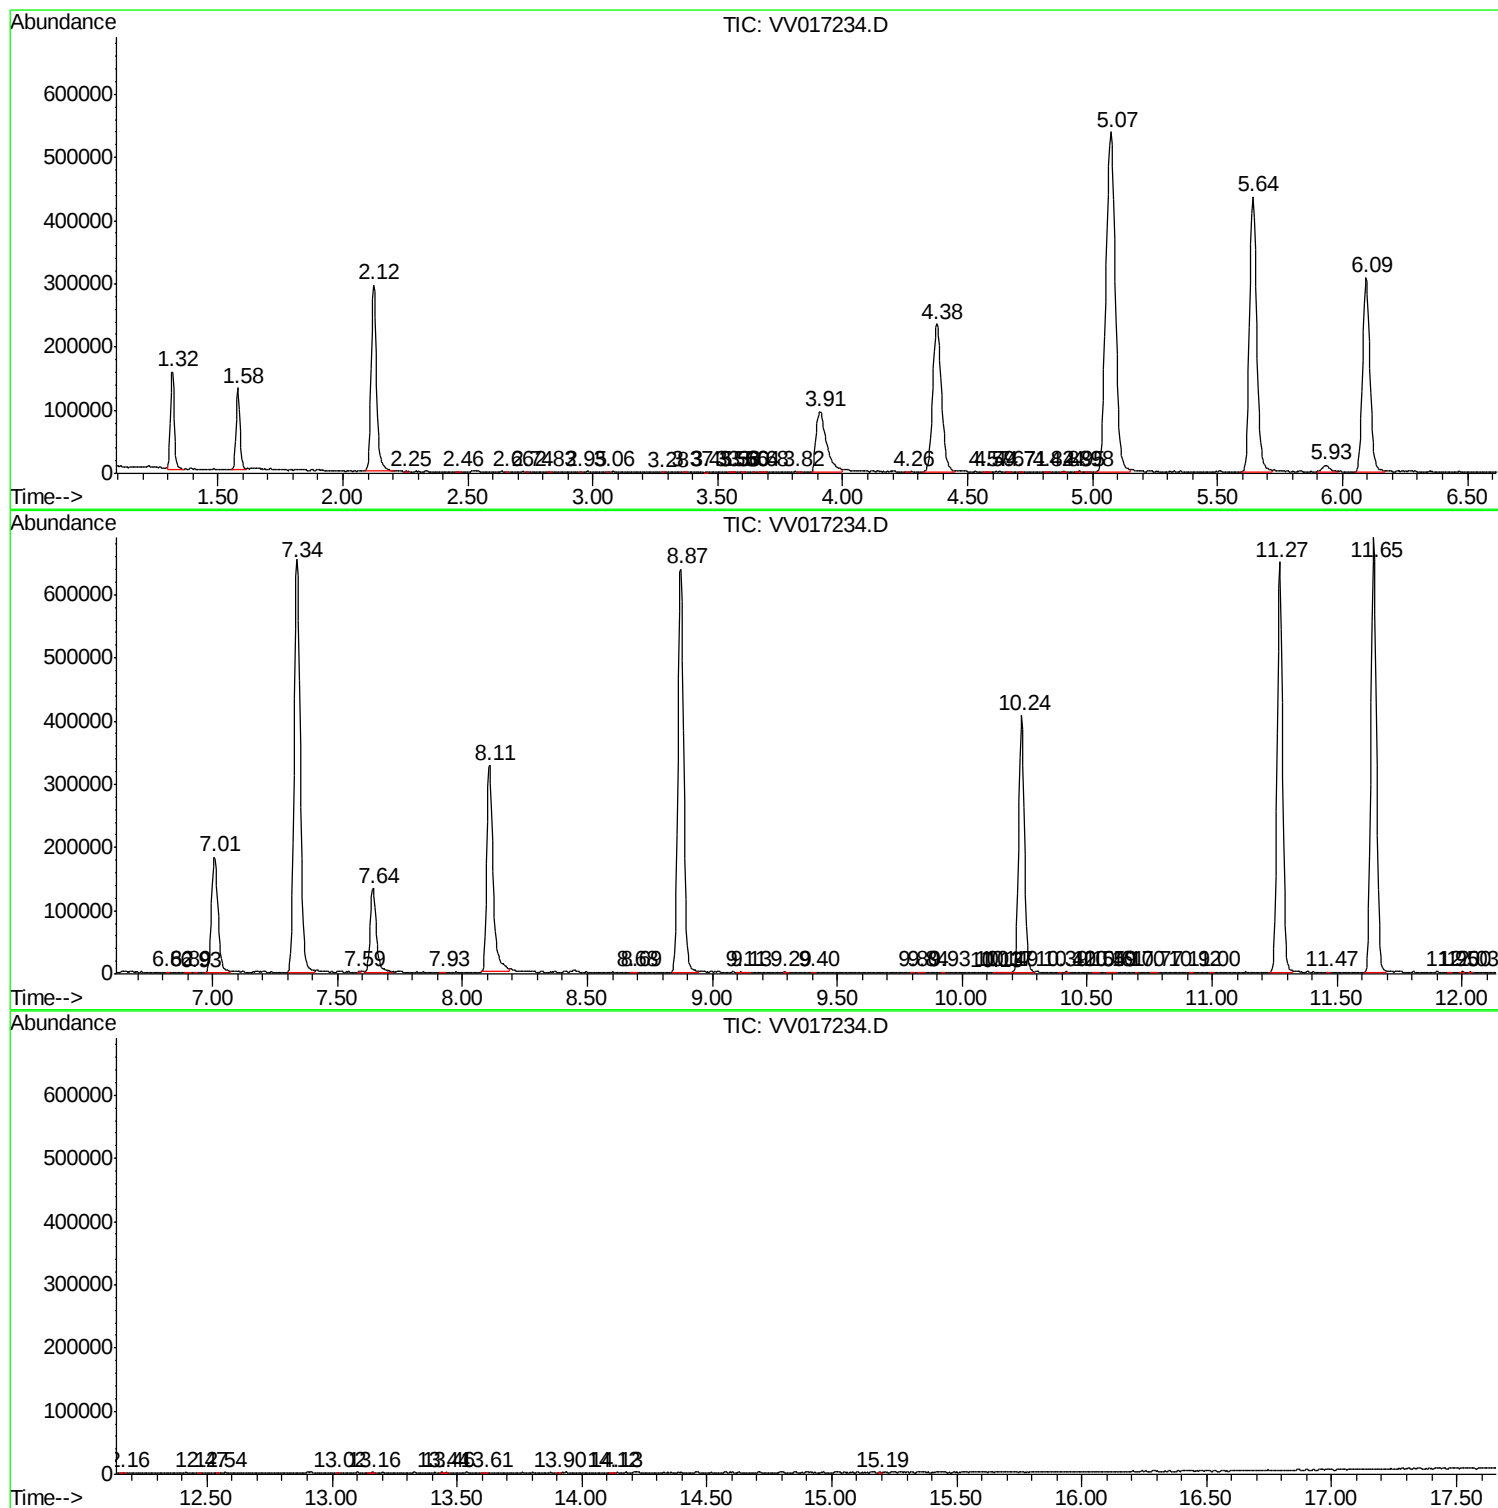

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017234.D
Acq On : 29 Jun 2020 12:33
Operator : SY/MD
Sample : L3133-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017234.D
Acq On : 29 Jun 2020 12:33
Operator : SY/MD
Sample : L3133-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc