

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017235.D
 Acq On : 29 Jun 2020 12:56
 Operator : SY/MD
 Sample : L3135-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q39

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	81	rVB	149032	154912	11.63%	1.511%
2	1.579	146	152	167	rVB	125125	139419	10.47%	1.360%
3	2.122	311	321	337	rBV	278502	424619	31.88%	4.142%
4	2.762	517	520	522	rBV3	1051	644	0.05%	0.006%
5	2.817	534	537	539	rBV4	979	504	0.04%	0.005%
6	2.878	553	556	557	rBV3	910	463	0.03%	0.005%
7	3.113	627	629	632	rBV3	1024	692	0.05%	0.007%
8	3.409	717	721	724	rVB5	942	742	0.06%	0.007%
9	3.428	724	727	730	rBV5	1039	841	0.06%	0.008%
10	3.553	763	766	768	rBV3	606	433	0.03%	0.004%
11	3.621	783	787	791	rBV6	1898	1736	0.13%	0.017%
12	3.733	819	822	826	rVB4	1502	1216	0.09%	0.012%
13	3.762	826	831	834	rBV6	1458	1087	0.08%	0.011%
14	3.788	836	839	844	rVB5	1208	1121	0.08%	0.011%
15	3.820	844	849	850	rBV3	1672	1106	0.08%	0.011%
16	3.910	864	877	907	rBV	90250	269672	20.25%	2.631%
17	4.325	1003	1006	1007	rBV3	1254	773	0.06%	0.008%
18	4.376	1007	1022	1046	rVV	221922	544118	40.86%	5.308%
19	4.624	1097	1099	1101	rBV3	1105	571	0.04%	0.006%
20	4.675	1113	1115	1117	rBV3	1016	587	0.04%	0.006%
21	4.749	1136	1138	1140	rBV2	1059	630	0.05%	0.006%
22	4.798	1151	1153	1154	rBV2	871	396	0.03%	0.004%
23	4.855	1169	1171	1176	rBV4	1033	804	0.06%	0.008%
24	5.071	1221	1238	1265	rBV2	510456	1331820	100.00%	12.992%
25	5.261	1295	1297	1301	rBV4	1191	956	0.07%	0.009%
26	5.328	1314	1318	1320	rBV4	1324	1092	0.08%	0.011%
27	5.518	1375	1377	1381	rVB3	1192	735	0.06%	0.007%
28	5.537	1381	1383	1386	rBV4	839	470	0.04%	0.005%
29	5.560	1389	1390	1394	rBV4	903	453	0.03%	0.004%
30	5.640	1403	1415	1436	rBV	428547	851293	63.92%	8.304%
31	5.939	1497	1508	1526	rVB3	50133	106563	8.00%	1.040%
32	6.093	1542	1556	1580	rBV	296188	594395	44.63%	5.798%
33	6.328	1624	1629	1630	rBV5	919	755	0.06%	0.007%
34	6.389	1647	1648	1650	rBV2	968	406	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017235.D
 Acq On : 29 Jun 2020 12:56
 Operator : SY/MD
 Sample : L3135-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q39

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.495	1678	1681	1682	rBV3	1767	949	0.07%	0.009%
36	6.621	1718	1720	1722	rBV3	952	565	0.04%	0.006%
37	6.849	1789	1791	1795	rVB4	893	473	0.04%	0.005%
38	6.929	1813	1816	1820	rBV4	796	573	0.04%	0.006%
39	6.949	1820	1822	1826	rBV3	1220	850	0.06%	0.008%
40	7.006	1830	1840	1856	rVV2	170098	299485	22.49%	2.921%
41	7.254	1910	1917	1918	rBV5	1043	1156	0.09%	0.011%
42	7.338	1930	1943	1968	rBV	616745	1060583	79.63%	10.346%
43	7.643	2027	2038	2061	rBV2	127679	220818	16.58%	2.154%
44	7.794	2082	2085	2086	rBV3	1248	795	0.06%	0.008%
45	7.878	2108	2111	2114	rBV3	1228	664	0.05%	0.006%
46	7.891	2114	2115	2120	rBV4	946	563	0.04%	0.005%
47	7.958	2132	2136	2139	rBV5	1690	1642	0.12%	0.016%
48	8.109	2173	2183	2216	rBV	316688	572081	42.95%	5.581%
49	8.521	2307	2311	2312	rBV4	1439	976	0.07%	0.010%
50	8.672	2356	2358	2364	rVB7	1446	842	0.06%	0.008%
51	8.704	2364	2368	2370	rBV3	825	644	0.05%	0.006%
52	8.801	2396	2398	2401	rBV3	1015	560	0.04%	0.005%
53	8.875	2409	2421	2440	rBV	639869	1030167	77.35%	10.049%
54	9.077	2481	2484	2487	rBV5	1514	939	0.07%	0.009%
55	9.125	2496	2499	2505	rBV7	1715	1398	0.10%	0.014%
56	9.203	2521	2523	2526	rVB4	906	479	0.04%	0.005%
57	9.296	2549	2552	2555	rBV5	790	446	0.03%	0.004%
58	9.408	2581	2587	2590	rBV6	1427	1137	0.09%	0.011%
59	9.453	2597	2601	2604	rBV5	1117	947	0.07%	0.009%
60	9.498	2612	2615	2618	rBV4	1566	877	0.07%	0.009%
61	9.598	2644	2646	2649	rBV3	855	419	0.03%	0.004%
62	9.646	2658	2661	2662	rBV3	864	434	0.03%	0.004%
63	9.794	2703	2707	2710	rBV5	988	753	0.06%	0.007%
64	9.817	2712	2714	2719	rBV3	1077	680	0.05%	0.007%
65	10.116	2805	2807	2809	rBV3	1024	428	0.03%	0.004%
66	10.238	2832	2845	2865	rVV	389288	612641	46.00%	5.976%
67	10.341	2875	2877	2878	rBV2	1141	494	0.04%	0.005%
68	10.392	2890	2893	2894	rBV2	1218	668	0.05%	0.007%
69	10.479	2917	2920	2926	rBV6	1249	1152	0.09%	0.011%
70	10.534	2934	2937	2939	rBV4	903	552	0.04%	0.005%
71	10.588	2951	2954	2955	rBV3	1517	863	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017235.D
 Acq On : 29 Jun 2020 12:56
 Operator : SY/MD
 Sample : L3135-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q39

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.727	2995	2997	2999	rVB3	951	489	0.04%	0.005%
73	10.797	3015	3019	3022	rBV4	613	622	0.05%	0.006%
74	10.868	3038	3041	3042	rBV3	799	436	0.03%	0.004%
75	10.897	3048	3050	3056	rVB7	1323	1128	0.08%	0.011%
76	10.968	3069	3072	3075	rVB5	1572	887	0.07%	0.009%
77	11.067	3099	3103	3106	rBV5	929	779	0.06%	0.008%
78	11.270	3154	3166	3187	rBV	629382	969283	72.78%	9.455%
79	11.646	3272	3283	3303	rVB	645214	1004309	75.41%	9.797%
80	11.855	3344	3348	3350	rBV	1574	1006	0.08%	0.010%
81	11.926	3368	3370	3373	rBV4	1053	648	0.05%	0.006%
82	11.971	3380	3384	3385	rBV3	1164	795	0.06%	0.008%
83	12.035	3399	3404	3410	rBV8	1477	2015	0.15%	0.020%
84	12.106	3424	3426	3431	rVB5	721	545	0.04%	0.005%
85	12.260	3470	3474	3475	rBV3	1257	703	0.05%	0.007%
86	12.334	3494	3497	3502	rVB6	1497	1352	0.10%	0.013%
87	12.373	3507	3509	3512	rBV2	1179	1060	0.08%	0.010%
88	12.437	3526	3529	3530	rBV3	850	508	0.04%	0.005%
89	12.450	3530	3533	3534	rVV2	782	450	0.03%	0.004%
90	12.617	3583	3585	3587	rBV3	1126	606	0.05%	0.006%
91	12.807	3640	3644	3646	rVV5	1291	953	0.07%	0.009%
92	13.058	3720	3722	3724	rBV2	1132	722	0.05%	0.007%
93	13.315	3800	3802	3806	rBV4	1032	524	0.04%	0.005%
94	13.675	3912	3914	3916	rBV2	1015	632	0.05%	0.006%
95	13.710	3923	3925	3928	rVB4	1071	604	0.05%	0.006%
96	13.733	3928	3932	3937	rVB4	1133	1246	0.09%	0.012%
97	13.762	3937	3941	3942	rBV3	1472	904	0.07%	0.009%
98	14.061	4032	4034	4038	rBV5	1386	856	0.06%	0.008%
99	14.601	4200	4202	4204	rBV3	998	569	0.04%	0.006%
100	14.697	4230	4232	4235	rBV3	1464	918	0.07%	0.009%


Sum of corrected areas: 10251266

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017235.D
Acq On : 29 Jun 2020 12:56
Operator : SY/MD
Sample : L3135-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q39

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

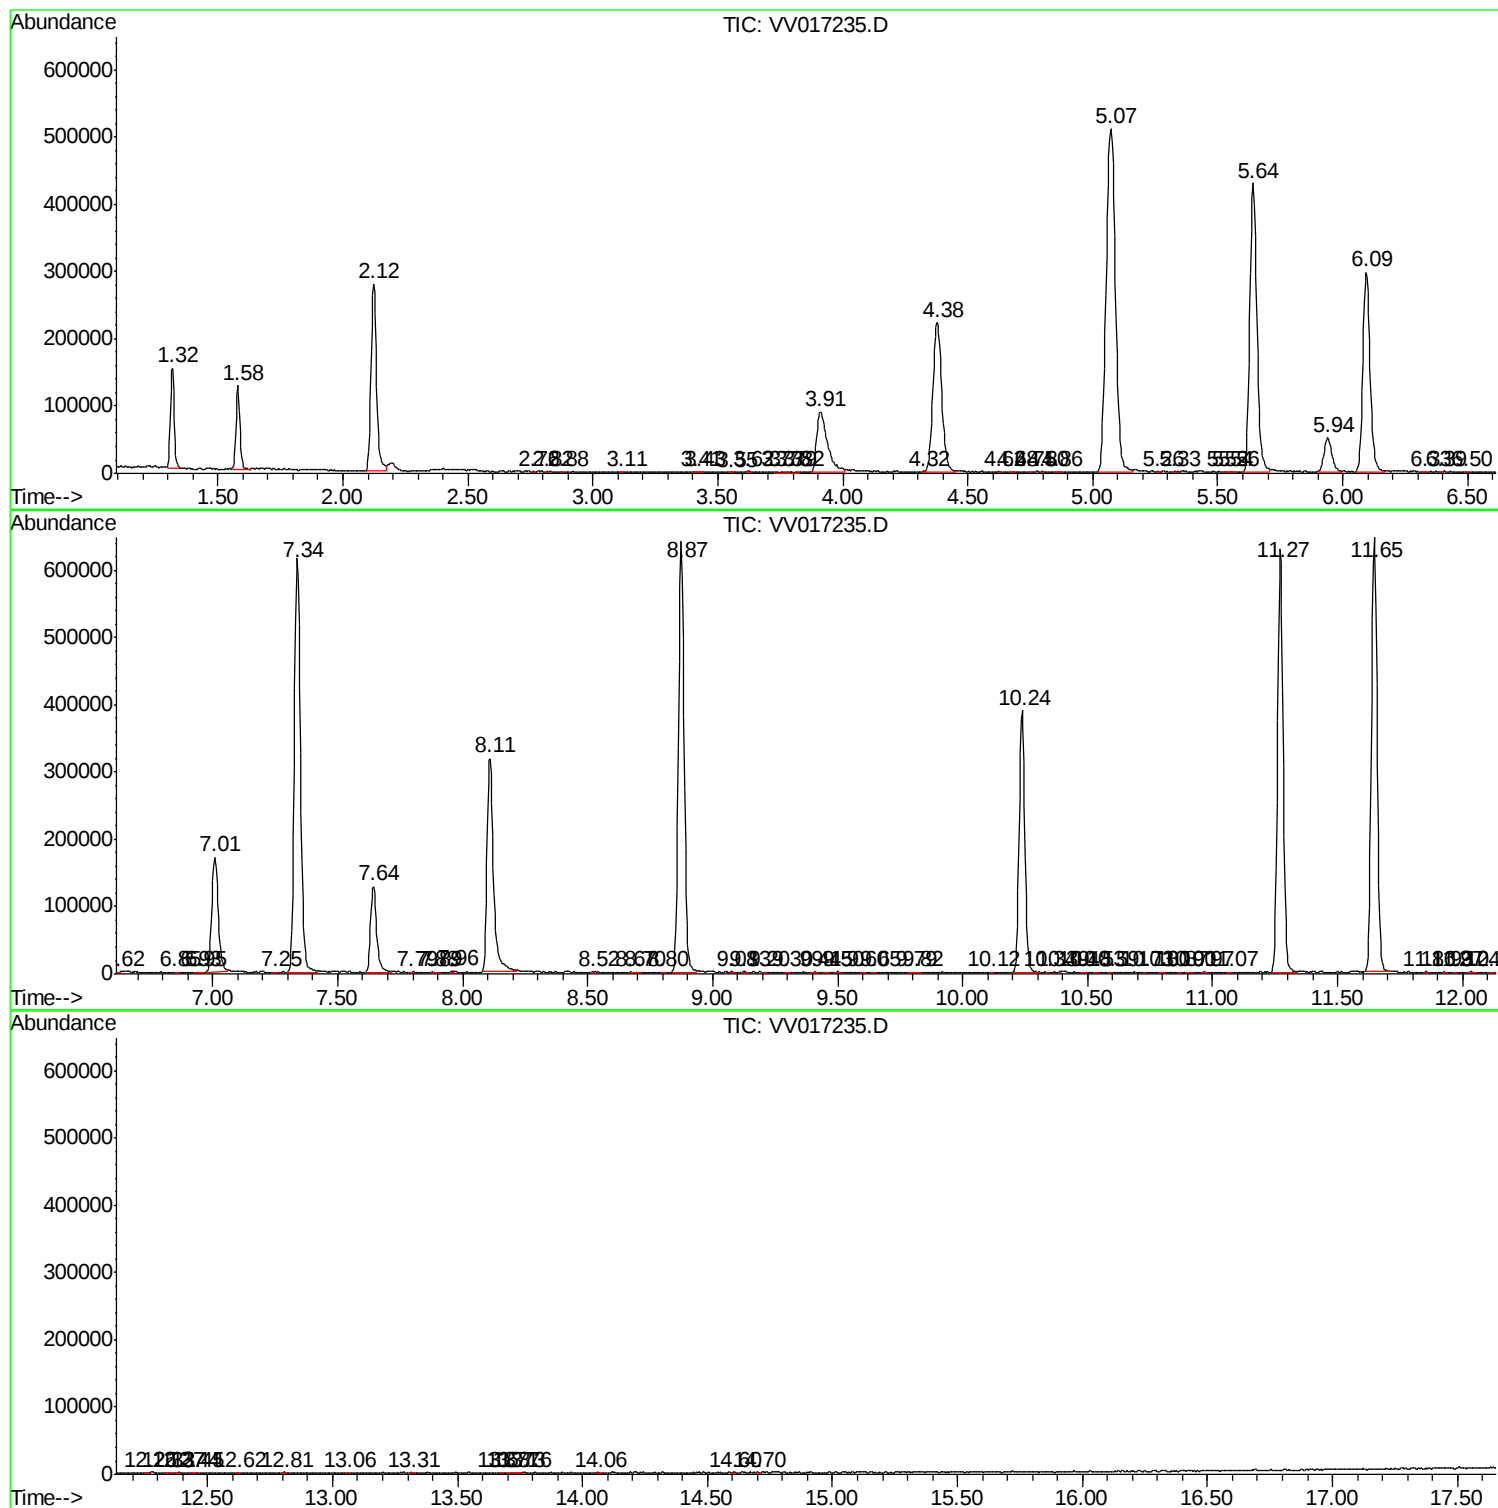

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017235.D
Acq On : 29 Jun 2020 12:56
Operator : SY/MD
Sample : L3135-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q39

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017235.D
Acq On : 29 Jun 2020 12:56
Operator : SY/MD
Sample : L3135-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q39

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc