

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017241.D
 Acq On : 29 Jun 2020 15:15
 Operator : SY/MD
 Sample : L3135-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	134522	143786	11.11%	1.308%
2	1.579	145	152	160	rBV	112316	122119	9.44%	1.111%
3	2.122	312	321	333	rBV	260638	391477	30.25%	3.560%
4	2.930	570	572	574	rBV2	1200	510	0.04%	0.005%
5	2.962	578	582	584	rBV4	924	703	0.05%	0.006%
6	2.981	586	588	590	rBV3	919	509	0.04%	0.005%
7	3.036	603	605	607	rBV2	996	368	0.03%	0.003%
8	3.100	623	625	627	rVV2	1124	491	0.04%	0.004%
9	3.206	657	658	662	rBV3	1291	704	0.05%	0.006%
10	3.380	711	712	717	rVB4	1414	704	0.05%	0.006%
11	3.418	722	724	727	rVB2	878	433	0.03%	0.004%
12	3.454	732	735	736	rBV3	1098	629	0.05%	0.006%
13	3.528	754	758	759	rBV4	1105	738	0.06%	0.007%
14	3.637	791	792	795	rBV	1207	633	0.05%	0.006%
15	3.817	846	848	850	rBV3	1164	603	0.05%	0.005%
16	3.865	861	863	865	rBV3	1738	952	0.07%	0.009%
17	3.936	865	885	905	rBV2	178263	619725	47.89%	5.636%
18	4.315	1000	1003	1006	rVB5	910	430	0.03%	0.004%
19	4.376	1006	1022	1048	rBV2	221625	546190	42.21%	4.967%
20	4.592	1087	1089	1090	rBV	1080	471	0.04%	0.004%
21	4.727	1128	1131	1132	rBV	901	614	0.05%	0.006%
22	4.820	1158	1160	1161	rBV	890	379	0.03%	0.003%
23	4.897	1182	1184	1189	rVB5	824	667	0.05%	0.006%
24	4.946	1196	1199	1203	rBV4	1921	1505	0.12%	0.014%
25	5.074	1220	1239	1262	rBV2	497038	1294039	100.00%	11.768%
26	5.341	1320	1322	1323	rBV2	981	383	0.03%	0.003%
27	5.441	1351	1353	1356	rVB3	1172	515	0.04%	0.005%
28	5.457	1356	1358	1361	rBV4	1238	533	0.04%	0.005%
29	5.518	1372	1377	1382	rBV6	1477	1723	0.13%	0.016%
30	5.640	1403	1415	1441	rBV	405999	812808	62.81%	7.392%
31	5.939	1493	1508	1531	rBV	418254	830681	64.19%	7.554%
32	6.093	1544	1556	1578	rBV	285109	577799	44.65%	5.255%
33	6.212	1590	1593	1596	rBV5	2217	1800	0.14%	0.016%
34	6.392	1647	1649	1656	rVB6	2229	2294	0.18%	0.021%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017241.D
 Acq On : 29 Jun 2020 15:15
 Operator : SY/MD
 Sample : L3135-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.421	1656	1658	1659	rBV2	1870	768	0.06%	0.007%
36	6.463	1669	1671	1672	rBV2	775	371	0.03%	0.003%
37	6.791	1770	1773	1775	rBV4	829	418	0.03%	0.004%
38	6.826	1781	1784	1787	rBV2	1014	967	0.07%	0.009%
39	6.884	1798	1802	1804	rBV3	1195	1124	0.09%	0.010%
40	7.007	1830	1840	1858	rBV	167106	293942	22.72%	2.673%
41	7.338	1931	1943	1962	rBV	596993	1017609	78.64%	9.254%
42	7.640	2027	2037	2057	rBV	120746	210623	16.28%	1.915%
43	7.775	2077	2079	2081	rBV3	1053	353	0.03%	0.003%
44	7.846	2099	2101	2103	rBV3	1058	510	0.04%	0.005%
45	8.000	2146	2149	2152	rBV4	1442	918	0.07%	0.008%
46	8.068	2166	2170	2172	rBV5	1000	788	0.06%	0.007%
47	8.106	2173	2182	2212	rVV	295826	550908	42.57%	5.010%
48	8.614	2338	2340	2345	rBV4	895	794	0.06%	0.007%
49	8.669	2352	2357	2362	rBV6	1247	1320	0.10%	0.012%
50	8.695	2363	2365	2370	rVB4	790	495	0.04%	0.005%
51	8.801	2396	2398	2400	rBV2	1041	517	0.04%	0.005%
52	8.875	2407	2421	2435	rBV	605086	984186	76.06%	8.950%
53	9.087	2484	2487	2491	rVB4	1739	1086	0.08%	0.010%
54	9.257	2537	2540	2541	rBV3	1105	520	0.04%	0.005%
55	9.305	2552	2555	2556	rBV	1175	705	0.05%	0.006%
56	9.450	2597	2600	2602	rBV2	1193	777	0.06%	0.007%
57	9.711	2676	2681	2689	rVB8	1251	1521	0.12%	0.014%
58	9.826	2714	2717	2719	rVV2	1087	744	0.06%	0.007%
59	9.968	2759	2761	2766	rBV3	1161	1106	0.09%	0.010%
60	10.119	2805	2808	2810	rBV4	1041	570	0.04%	0.005%
61	10.238	2833	2845	2857	rBV	390469	599654	46.34%	5.453%
62	10.344	2876	2878	2880	rBV2	1111	776	0.06%	0.007%
63	10.373	2885	2887	2889	rVV3	1032	488	0.04%	0.004%
64	10.595	2951	2956	2959	rBV5	2039	1849	0.14%	0.017%
65	10.643	2968	2971	2973	rBV2	887	509	0.04%	0.005%
66	10.669	2977	2979	2982	rVB3	1161	574	0.04%	0.005%
67	10.736	2997	3000	3004	rBV5	767	770	0.06%	0.007%
68	10.756	3004	3006	3010	rVB4	1384	791	0.06%	0.007%
69	10.839	3030	3032	3035	rBV3	1055	515	0.04%	0.005%
70	10.878	3041	3044	3047	rBV5	1721	1078	0.08%	0.010%
71	10.948	3062	3066	3067	rBV3	949	742	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017241.D
 Acq On : 29 Jun 2020 15:15
 Operator : SY/MD
 Sample : L3135-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.987	3075	3078	3083	rBV4	874	624	0.05%	0.006%
73	11.067	3101	3103	3109	rBV5	715	698	0.05%	0.006%
74	11.125	3118	3121	3123	rBV3	1256	652	0.05%	0.006%
75	11.270	3154	3166	3185	rBV	613158	926843	71.62%	8.429%
76	11.466	3224	3227	3229	rBV3	1339	882	0.07%	0.008%
77	11.556	3248	3255	3265	rBV4	13382	22457	1.74%	0.204%
78	11.646	3272	3283	3300	rVB	623282	985315	76.14%	8.960%
79	11.894	3358	3360	3361	rBV2	1031	385	0.03%	0.004%
80	11.939	3372	3374	3376	rBV3	1334	839	0.06%	0.008%
81	12.106	3424	3426	3427	rBV3	1259	432	0.03%	0.004%
82	12.125	3430	3432	3437	rBV4	1110	980	0.08%	0.009%
83	12.231	3463	3465	3469	rBV5	1243	949	0.07%	0.009%
84	12.370	3506	3508	3513	rVB4	1046	779	0.06%	0.007%
85	12.434	3525	3528	3531	rBV3	1333	943	0.07%	0.009%
86	12.534	3556	3559	3563	rBV4	1148	1060	0.08%	0.010%
87	12.627	3585	3588	3591	rBV3	1153	837	0.06%	0.008%
88	12.727	3617	3619	3622	rBV3	839	661	0.05%	0.006%
89	12.884	3666	3668	3670	rBV3	1464	825	0.06%	0.008%
90	13.000	3701	3704	3707	rBV2	1236	584	0.05%	0.005%
91	13.019	3707	3710	3712	rBV3	1482	1064	0.08%	0.010%
92	13.119	3739	3741	3744	rBV4	1042	623	0.05%	0.006%
93	13.315	3799	3802	3803	rBV3	1032	574	0.04%	0.005%
94	13.350	3811	3813	3817	rVV3	1078	503	0.04%	0.005%
95	13.379	3817	3822	3828	rVB7	1694	2297	0.18%	0.021%
96	13.653	3904	3907	3910	rBV3	1238	885	0.07%	0.008%
97	13.759	3937	3940	3944	rBV3	1094	814	0.06%	0.007%
98	13.890	3979	3981	3986	rBV3	1482	927	0.07%	0.008%
99	14.193	4072	4075	4080	rVB6	1695	1592	0.12%	0.014%
100	15.530	4489	4491	4493	rBV3	1729	923	0.07%	0.008%


Sum of corrected areas: 10996248

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017241.D
Acq On : 29 Jun 2020 15:15
Operator : SY/MD
Sample : L3135-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

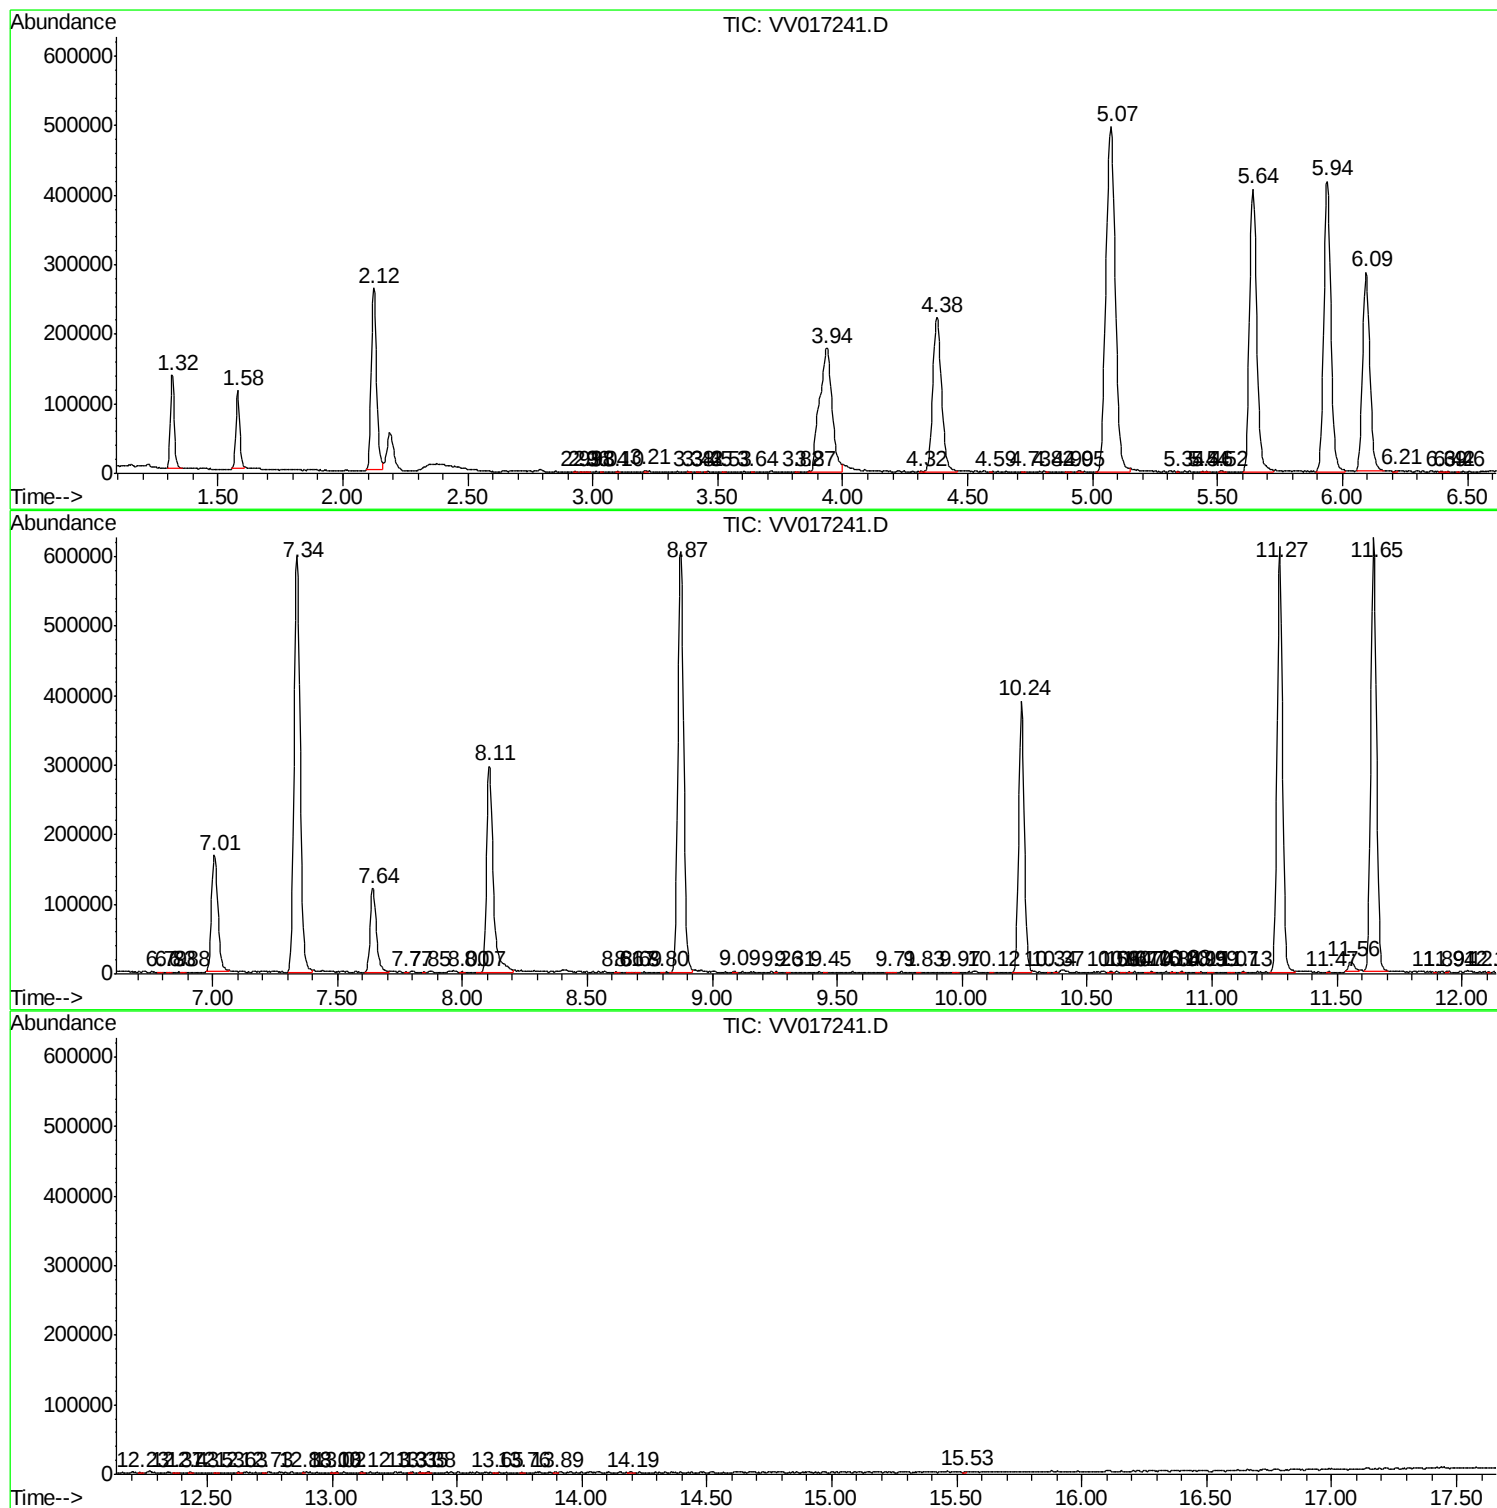

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017241.D
Acq On : 29 Jun 2020 15:15
Operator : SY/MD
Sample : L3135-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q57

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017241.D
Acq On : 29 Jun 2020 15:15
Operator : SY/MD
Sample : L3135-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q57

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc