

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017242.D
 Acq On : 29 Jun 2020 15:39
 Operator : SY/MD
 Sample : L3135-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	83	rVB	135380	144573	11.34%	1.205%
2	1.579	145	152	161	rVB	106938	114892	9.01%	0.957%
3	2.123	312	321	333	rBV	259636	385758	30.27%	3.214%
4	3.020	596	600	603	rBV4	1399	925	0.07%	0.008%
5	3.068	610	615	617	rBV4	1257	1233	0.10%	0.010%
6	3.097	622	624	628	rVB3	774	568	0.04%	0.005%
7	3.409	718	721	724	rVB5	1317	810	0.06%	0.007%
8	3.672	797	803	806	rBV5	1321	1301	0.10%	0.011%
9	3.698	809	811	816	rVB5	1441	869	0.07%	0.007%
10	3.724	816	819	822	rBV3	1100	826	0.06%	0.007%
11	3.856	857	860	864	rBV6	1328	1201	0.09%	0.010%
12	3.939	864	886	925	rVV2	359256	1118223	87.74%	9.318%
13	4.377	1007	1022	1046	rBV2	219808	536424	42.09%	4.470%
14	4.637	1101	1103	1107	rVB4	1081	681	0.05%	0.006%
15	4.746	1135	1137	1141	rBV3	1125	874	0.07%	0.007%
16	4.817	1154	1159	1160	rBV4	889	821	0.06%	0.007%
17	4.930	1190	1194	1198	rVB5	1748	1480	0.12%	0.012%
18	4.949	1198	1200	1202	rBV3	1185	656	0.05%	0.005%
19	5.071	1221	1238	1260	rBV2	495601	1274473	100.00%	10.620%
20	5.338	1318	1321	1324	rBV4	1152	701	0.06%	0.006%
21	5.383	1333	1335	1338	rBV4	1054	806	0.06%	0.007%
22	5.640	1403	1415	1437	rBV	418835	830656	65.18%	6.922%
23	5.939	1494	1508	1534	rBV	647631	1265558	99.30%	10.546%
24	6.093	1544	1556	1576	rVB	282330	570166	44.74%	4.751%
25	6.450	1665	1667	1673	rVV5	1212	905	0.07%	0.008%
26	6.518	1684	1688	1690	rBV3	1136	861	0.07%	0.007%
27	6.537	1690	1694	1695	rBV3	1019	657	0.05%	0.005%
28	6.592	1710	1711	1714	rBV3	1420	882	0.07%	0.007%
29	6.817	1778	1781	1785	rVB3	1560	1023	0.08%	0.009%
30	6.846	1788	1790	1793	rVB2	1431	814	0.06%	0.007%
31	7.007	1829	1840	1857	rBV	165114	296369	23.25%	2.470%
32	7.338	1931	1943	1962	rBV	586152	1002186	78.64%	8.351%
33	7.643	2028	2038	2056	rBV	119375	204638	16.06%	1.705%
34	7.749	2068	2071	2073	rBV3	1569	756	0.06%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017242.D
 Acq On : 29 Jun 2020 15:39
 Operator : SY/MD
 Sample : L3135-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.775	2076	2079	2080	rBV3	1233	554	0.04%	0.005%
36	7.875	2108	2110	2113	rBV2	891	629	0.05%	0.005%
37	7.910	2119	2121	2123	rBV3	1083	554	0.04%	0.005%
38	8.106	2170	2182	2215	rBV	315365	581868	45.66%	4.849%
39	8.563	2322	2324	2328	rBV3	1314	707	0.06%	0.006%
40	8.646	2347	2350	2352	rBV4	1001	605	0.05%	0.005%
41	8.871	2408	2420	2442	rBV	621078	1012861	79.47%	8.440%
42	9.090	2484	2488	2490	rBV3	992	880	0.07%	0.007%
43	9.209	2521	2525	2527	rBV4	924	749	0.06%	0.006%
44	9.412	2584	2588	2589	rBV3	1577	1192	0.09%	0.010%
45	9.582	2637	2641	2645	rVB5	1398	1474	0.12%	0.012%
46	9.608	2645	2649	2650	rBV3	1288	754	0.06%	0.006%
47	9.765	2694	2698	2699	rBV4	1244	880	0.07%	0.007%
48	9.987	2766	2767	2772	rVB3	1272	675	0.05%	0.006%
49	10.010	2772	2774	2777	rBV3	953	628	0.05%	0.005%
50	10.035	2778	2782	2788	rBV8	2075	2064	0.16%	0.017%
51	10.238	2833	2845	2863	rVV	391381	607226	47.65%	5.060%
52	10.306	2863	2866	2870	rVB4	1875	1200	0.09%	0.010%
53	10.389	2888	2892	2894	rBV3	1640	1092	0.09%	0.009%
54	10.473	2915	2918	2922	rBV3	953	923	0.07%	0.008%
55	10.572	2946	2949	2951	rBV3	1451	845	0.07%	0.007%
56	10.675	2979	2981	2985	rBV3	943	628	0.05%	0.005%
57	10.826	3025	3028	3029	rBV4	1311	792	0.06%	0.007%
58	10.871	3039	3042	3043	rBV2	1074	648	0.05%	0.005%
59	10.945	3063	3065	3069	rVB3	896	596	0.05%	0.005%
60	11.064	3099	3102	3105	rVB4	1189	748	0.06%	0.006%
61	11.084	3107	3108	3111	rBV2	1199	750	0.06%	0.006%
62	11.116	3116	3118	3121	rVB3	1310	847	0.07%	0.007%
63	11.151	3121	3129	3131	rBV5	1772	1769	0.14%	0.015%
64	11.209	3144	3147	3151	rBV4	990	754	0.06%	0.006%
65	11.270	3154	3166	3185	rBV	630787	965459	75.75%	8.045%
66	11.460	3222	3225	3228	rVB3	1542	803	0.06%	0.007%
67	11.556	3246	3255	3271	rBV5	15049	33800	2.65%	0.282%
68	11.646	3272	3283	3299	rVB	639563	980766	76.95%	8.172%
69	11.955	3377	3379	3381	rBV2	1198	686	0.05%	0.006%
70	12.023	3394	3400	3407	rVB8	2661	3060	0.24%	0.025%
71	12.077	3415	3417	3419	rBV2	1417	617	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017242.D
 Acq On : 29 Jun 2020 15:39
 Operator : SY/MD
 Sample : L3135-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.186	3449	3451	3453	rBV3	1083	553	0.04%	0.005%
73	12.621	3582	3586	3588	rBV3	828	715	0.06%	0.006%
74	12.791	3637	3639	3643	rBV4	917	628	0.05%	0.005%
75	12.900	3671	3673	3676	rBV3	1305	711	0.06%	0.006%
76	12.958	3685	3691	3693	rBV5	1471	1552	0.12%	0.013%
77	13.006	3702	3706	3710	rVB5	1244	1298	0.10%	0.011%
78	13.029	3710	3713	3716	rBV4	1256	1127	0.09%	0.009%
79	13.209	3766	3769	3771	rBV3	1558	950	0.07%	0.008%
80	13.376	3816	3821	3825	rBV7	1202	1367	0.11%	0.011%
81	13.473	3849	3851	3852	rBV	1334	604	0.05%	0.005%
82	13.511	3859	3863	3865	rBV4	822	644	0.05%	0.005%
83	13.543	3871	3873	3878	rVV4	948	834	0.07%	0.007%
84	13.707	3922	3924	3925	rBV	1314	591	0.05%	0.005%
85	13.759	3934	3940	3942	rBV7	1132	1048	0.08%	0.009%
86	13.775	3942	3945	3948	rVV4	1195	816	0.06%	0.007%
87	13.884	3973	3979	3983	rBV6	898	1027	0.08%	0.009%
88	14.141	4056	4059	4061	rBV3	1405	792	0.06%	0.007%
89	14.154	4061	4063	4069	rVV4	1387	1186	0.09%	0.010%
90	14.331	4115	4118	4120	rBV3	1388	1126	0.09%	0.009%
91	14.434	4146	4150	4156	rBV7	1253	1445	0.11%	0.012%
92	14.473	4160	4162	4165	rBV4	907	682	0.05%	0.006%
93	14.559	4187	4189	4192	rBV2	1223	583	0.05%	0.005%
94	14.678	4223	4226	4229	rBV4	1353	1010	0.08%	0.008%
95	14.727	4238	4241	4244	rVB4	981	555	0.04%	0.005%
96	14.765	4251	4253	4256	rBV4	1029	722	0.06%	0.006%
97	14.794	4256	4262	4264	rBV7	1460	1394	0.11%	0.012%
98	14.865	4282	4284	4287	rBV3	1236	899	0.07%	0.007%
99	15.128	4362	4366	4367	rBV3	1092	628	0.05%	0.005%
100	15.283	4412	4414	4417	rBV2	920	740	0.06%	0.006%


Sum of corrected areas: 12000876

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017242.D
Acq On : 29 Jun 2020 15:39
Operator : SY/MD
Sample : L3135-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

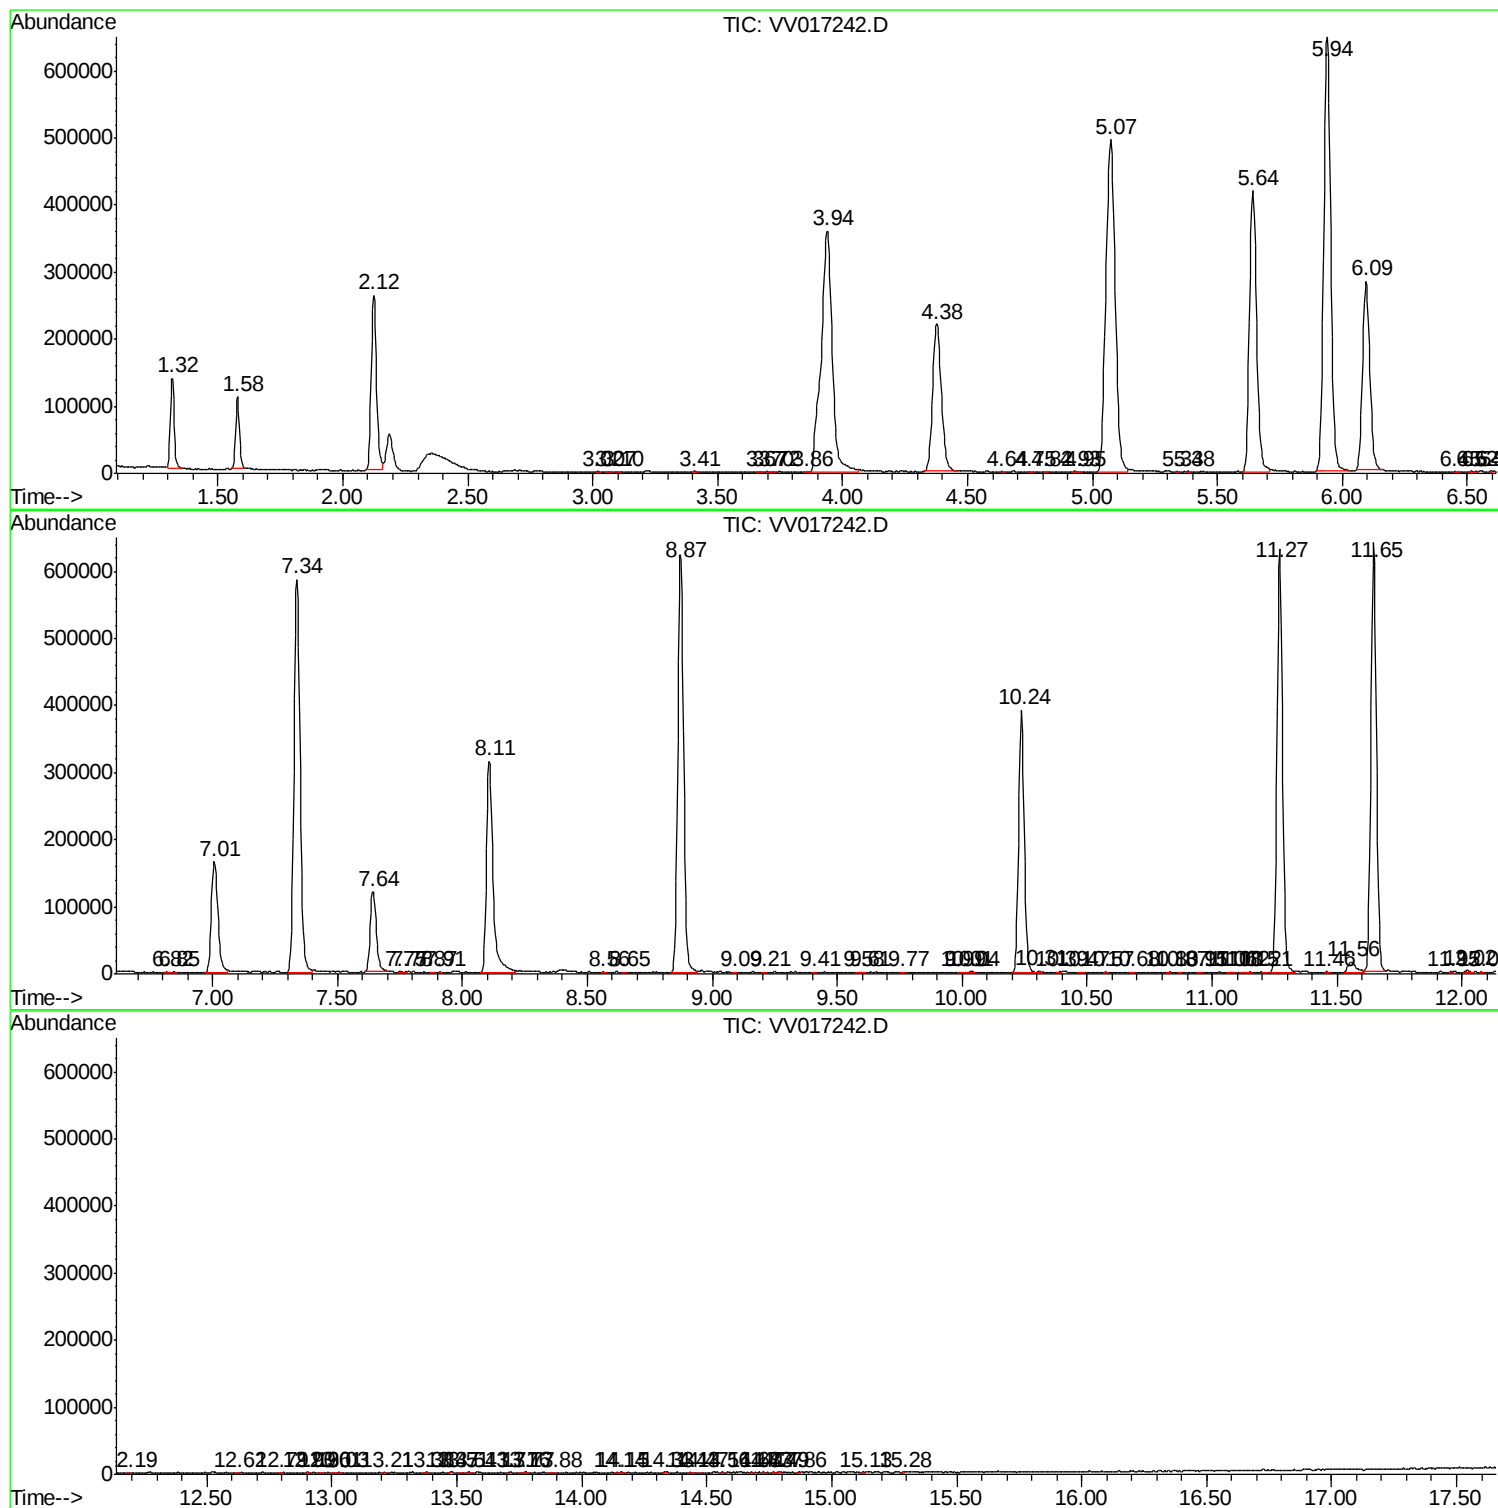

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017242.D
Acq On : 29 Jun 2020 15:39
Operator : SY/MD
Sample : L3135-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q58

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017242.D
Acq On : 29 Jun 2020 15:39
Operator : SY/MD
Sample : L3135-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q58

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc