

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017243.D
 Acq On : 29 Jun 2020 16:02
 Operator : SY/MD
 Sample : L3135-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB	136617	144111	11.13%	1.403%
2	1.579	145	152	160	rBV	111265	120841	9.33%	1.176%
3	2.122	312	321	335	rBV	258680	392913	30.34%	3.824%
4	2.627	475	478	480	rBV4	1094	755	0.06%	0.007%
5	3.045	603	608	611	rBV4	1051	979	0.08%	0.010%
6	3.109	625	628	635	rVB7	1080	1224	0.09%	0.012%
7	3.145	635	639	641	rBV4	814	701	0.05%	0.007%
8	3.245	668	670	673	rBV3	1497	877	0.07%	0.009%
9	3.392	712	716	719	rVB3	1040	819	0.06%	0.008%
10	3.409	719	721	725	rVB3	1229	645	0.05%	0.006%
11	3.437	725	730	732	rBV5	1457	1434	0.11%	0.014%
12	3.534	757	760	763	rVB4	1550	930	0.07%	0.009%
13	3.553	763	766	768	rBV3	820	621	0.05%	0.006%
14	3.598	776	780	783	rBV4	934	964	0.07%	0.009%
15	3.643	791	794	798	rBV3	1363	1051	0.08%	0.010%
16	3.698	809	811	814	rBV3	1259	672	0.05%	0.007%
17	3.907	865	876	908	rVV	93014	307387	23.74%	2.992%
18	4.248	979	982	985	rVB4	1189	649	0.05%	0.006%
19	4.328	1000	1007	1008	rBV	5021	3880	0.30%	0.038%
20	4.376	1009	1022	1045	rVB	220313	535767	41.38%	5.215%
21	4.772	1141	1145	1150	rVB7	1641	1598	0.12%	0.016%
22	4.839	1163	1166	1168	rBV2	1223	797	0.06%	0.008%
23	4.981	1207	1210	1213	rBV2	1263	953	0.07%	0.009%
24	5.071	1216	1238	1263	rBV2	498925	1294824	100.00%	12.603%
25	5.280	1300	1303	1308	rBV6	1241	1068	0.08%	0.010%
26	5.312	1311	1313	1317	rBV5	1221	837	0.06%	0.008%
27	5.415	1342	1345	1348	rBV4	1429	1158	0.09%	0.011%
28	5.640	1403	1415	1439	rBV	430815	849118	65.58%	8.264%
29	5.939	1492	1508	1527	rBV3	134210	284605	21.98%	2.770%
30	6.093	1543	1556	1577	rBV	280471	578899	44.71%	5.634%
31	6.305	1618	1622	1626	rVB7	1090	1071	0.08%	0.010%
32	6.601	1712	1714	1719	rVB5	1129	1072	0.08%	0.010%
33	6.630	1719	1723	1725	rBV4	2269	1893	0.15%	0.018%
34	6.711	1745	1748	1752	rVB5	1808	1265	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017243.D
 Acq On : 29 Jun 2020 16:02
 Operator : SY/MD
 Sample : L3135-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.791	1768	1773	1776	rBV4	1406	1314	0.10%	0.013%
36	6.897	1802	1806	1808	rBV4	1452	1054	0.08%	0.010%
37	6.942	1818	1820	1826	rVB5	1570	1052	0.08%	0.010%
38	7.006	1826	1840	1856	rBV	166744	298802	23.08%	2.908%
39	7.338	1930	1943	1962	rBV	582240	1011309	78.10%	9.843%
40	7.566	2012	2014	2019	rBV5	1371	1431	0.11%	0.014%
41	7.643	2028	2038	2053	rBV	120072	201491	15.56%	1.961%
42	7.762	2072	2075	2077	rBV4	1704	1024	0.08%	0.010%
43	7.878	2107	2111	2112	rBV4	856	710	0.05%	0.007%
44	7.907	2118	2120	2122	rBV3	1299	669	0.05%	0.007%
45	8.013	2150	2153	2156	rBV4	1375	1065	0.08%	0.010%
46	8.035	2158	2160	2164	rBV3	1158	789	0.06%	0.008%
47	8.106	2172	2182	2222	rBV	302985	571709	44.15%	5.564%
48	8.524	2308	2312	2313	rBV3	1225	790	0.06%	0.008%
49	8.543	2316	2318	2321	rVV2	1457	761	0.06%	0.007%
50	8.563	2321	2324	2329	rVV5	749	728	0.06%	0.007%
51	8.662	2350	2355	2358	rBV5	1252	1163	0.09%	0.011%
52	8.711	2365	2370	2374	rBV8	1283	1140	0.09%	0.011%
53	8.781	2388	2392	2396	rVB7	1401	1237	0.10%	0.012%
54	8.801	2396	2398	2401	rBV4	1017	743	0.06%	0.007%
55	8.871	2408	2420	2444	rBV	626130	1024328	79.11%	9.970%
56	9.148	2502	2506	2508	rBV5	1043	710	0.05%	0.007%
57	9.341	2563	2566	2570	rVB5	1650	1225	0.09%	0.012%
58	9.575	2637	2639	2642	rBV4	1268	788	0.06%	0.008%
59	9.820	2711	2715	2719	rBV3	1513	1168	0.09%	0.011%
60	10.022	2773	2778	2779	rBV3	1670	1184	0.09%	0.012%
61	10.080	2794	2796	2800	rBV5	1158	794	0.06%	0.008%
62	10.183	2826	2828	2833	rVB5	1280	851	0.07%	0.008%
63	10.238	2833	2845	2858	rBV	389711	603685	46.62%	5.876%
64	10.392	2889	2893	2895	rBV4	1228	875	0.07%	0.009%
65	10.501	2925	2927	2929	rBV2	1090	664	0.05%	0.006%
66	10.656	2972	2975	2976	rBV3	1156	660	0.05%	0.006%
67	10.784	3009	3015	3017	rBV6	1355	1396	0.11%	0.014%
68	10.823	3021	3027	3029	rBV6	1653	1633	0.13%	0.016%
69	10.987	3074	3078	3081	rBV3	1546	1226	0.09%	0.012%
70	11.009	3083	3085	3088	rVB4	1464	710	0.05%	0.007%
71	11.112	3114	3117	3118	rBV3	1208	615	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017243.D
 Acq On : 29 Jun 2020 16:02
 Operator : SY/MD
 Sample : L3135-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.183	3137	3139	3141	rBV3	1360	616	0.05%	0.006%
73	11.270	3152	3166	3183	rBV	631316	970194	74.93%	9.443%
74	11.431	3213	3216	3218	rBV4	1601	889	0.07%	0.009%
75	11.508	3238	3240	3245	rBV6	1123	1062	0.08%	0.010%
76	11.556	3245	3255	3265	rBV6	9726	20958	1.62%	0.204%
77	11.646	3272	3283	3300	rVB	628700	980628	75.73%	9.544%
78	11.961	3378	3381	3385	rVB5	1706	1212	0.09%	0.012%
79	11.984	3385	3388	3390	rBV2	1294	764	0.06%	0.007%
80	12.022	3398	3400	3402	rBV3	1545	689	0.05%	0.007%
81	12.254	3470	3472	3474	rBV3	1128	665	0.05%	0.006%
82	12.585	3572	3575	3577	rBV3	1473	950	0.07%	0.009%
83	12.849	3653	3657	3661	rBV4	1514	1209	0.09%	0.012%
84	12.887	3665	3669	3672	rBV3	1497	1188	0.09%	0.012%
85	12.926	3677	3681	3682	rBV2	1186	793	0.06%	0.008%
86	13.054	3717	3721	3724	rBV4	1168	1030	0.08%	0.010%
87	13.135	3739	3746	3750	rBV8	1577	1782	0.14%	0.017%
88	13.276	3786	3790	3791	rBV3	934	735	0.06%	0.007%
89	13.308	3798	3800	3804	rVB3	1275	787	0.06%	0.008%
90	13.379	3816	3822	3824	rBV5	756	671	0.05%	0.007%
91	13.402	3826	3829	3831	rBV2	1192	693	0.05%	0.007%
92	13.421	3832	3835	3838	rVV3	1658	1020	0.08%	0.010%
93	13.572	3879	3882	3883	rBV4	1076	697	0.05%	0.007%
94	13.720	3926	3928	3933	rBV4	972	915	0.07%	0.009%
95	13.903	3980	3985	3988	rBV6	1512	1730	0.13%	0.017%
96	13.958	3997	4002	4003	rBV3	1280	1042	0.08%	0.010%
97	14.540	4180	4183	4184	rBV2	1019	733	0.06%	0.007%
98	15.250	4402	4404	4405	rBV	1610	660	0.05%	0.006%
99	15.331	4427	4429	4433	rBV4	1273	808	0.06%	0.008%
100	15.820	4577	4581	4584	rBV5	1456	1349	0.10%	0.013%


Sum of corrected areas: 10274340

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017243.D
Acq On : 29 Jun 2020 16:02
Operator : SY/MD
Sample : L3135-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

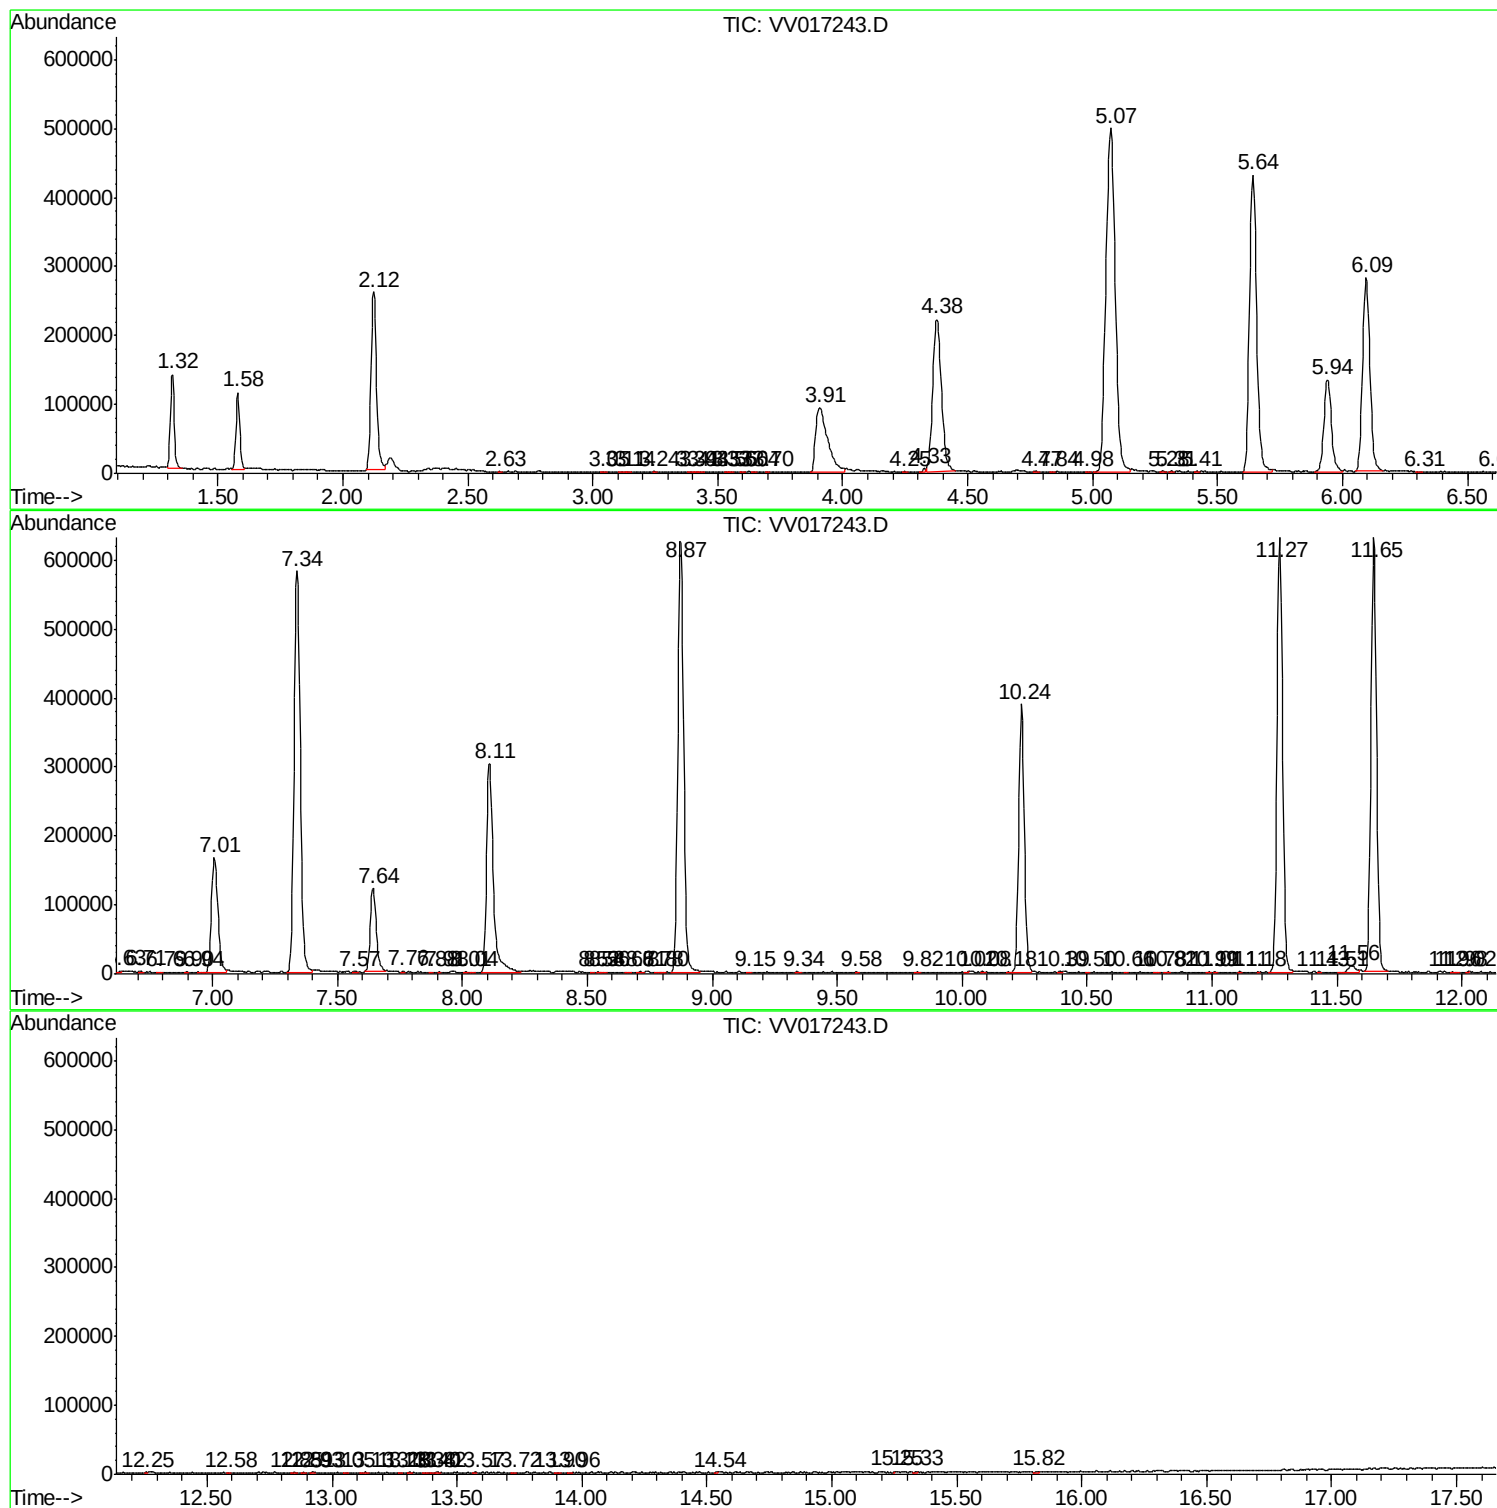

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017243.D
Acq On : 29 Jun 2020 16:02
Operator : SY/MD
Sample : L3135-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017243.D
Acq On : 29 Jun 2020 16:02
Operator : SY/MD
Sample : L3135-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q59

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc