

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017245.D
 Acq On : 29 Jun 2020 17:35
 Operator : SY/MD
 Sample : L3135-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	127699	133616	10.58%	1.361%
2	1.579	145	152	164	rVB	108010	120397	9.53%	1.227%
3	2.123	311	321	339	rBV	254547	387317	30.67%	3.947%
4	2.309	376	379	381	rBV4	1631	1302	0.10%	0.013%
5	2.634	478	480	483	rBV4	1097	457	0.04%	0.005%
6	2.926	568	571	574	rBV3	649	521	0.04%	0.005%
7	2.946	574	577	584	rBV7	1581	2006	0.16%	0.020%
8	3.007	593	596	600	rVB3	2041	1160	0.09%	0.012%
9	3.061	611	613	617	rVB2	1025	614	0.05%	0.006%
10	3.293	683	685	688	rBV3	912	674	0.05%	0.007%
11	3.309	688	690	692	rVV2	1497	697	0.06%	0.007%
12	3.377	708	711	716	rBV6	1603	1161	0.09%	0.012%
13	3.457	733	736	737	rBV3	914	485	0.04%	0.005%
14	3.512	750	753	755	rBV3	1182	559	0.04%	0.006%
15	3.605	780	782	787	rVV5	1035	824	0.07%	0.008%
16	3.663	798	800	801	rBV2	891	405	0.03%	0.004%
17	3.772	831	834	837	rVV4	769	591	0.05%	0.006%
18	3.872	861	865	866	rBV4	1499	1048	0.08%	0.011%
19	3.907	866	876	901	rVV	92745	257781	20.41%	2.627%
20	4.376	1008	1022	1045	rVB	210931	513826	40.68%	5.236%
21	4.640	1102	1104	1107	rVB3	2082	1083	0.09%	0.011%
22	4.656	1107	1109	1111	rBV3	1128	584	0.05%	0.006%
23	4.688	1116	1119	1121	rBV3	981	569	0.05%	0.006%
24	4.756	1138	1140	1141	rBV	996	461	0.04%	0.005%
25	4.830	1161	1163	1165	rVB3	1580	676	0.05%	0.007%
26	4.846	1165	1168	1171	rBV4	709	488	0.04%	0.005%
27	4.917	1186	1190	1193	rBV4	1327	1348	0.11%	0.014%
28	4.962	1202	1204	1207	rVB2	1029	490	0.04%	0.005%
29	5.071	1222	1238	1261	rBV2	489783	1262998	100.00%	12.869%
30	5.277	1300	1302	1306	rVB5	1391	989	0.08%	0.010%
31	5.303	1307	1310	1312	rBV4	903	563	0.04%	0.006%
32	5.319	1312	1315	1317	rBV4	1531	927	0.07%	0.009%
33	5.376	1331	1333	1337	rVB4	900	451	0.04%	0.005%
34	5.457	1356	1358	1363	rVB6	1505	1330	0.11%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017245.D
 Acq On : 29 Jun 2020 17:35
 Operator : SY/MD
 Sample : L3135-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.483	1363	1366	1368	rBV4	1242	839	0.07%	0.009%
36	5.640	1402	1415	1445	rBV	416299	833966	66.03%	8.498%
37	5.939	1495	1508	1525	rBV5	52932	117793	9.33%	1.200%
38	6.093	1543	1556	1577	rBV2	284951	575875	45.60%	5.868%
39	6.319	1622	1626	1628	rBV4	1063	789	0.06%	0.008%
40	6.383	1643	1646	1648	rBV4	1354	1062	0.08%	0.011%
41	6.515	1684	1687	1688	rBV	793	547	0.04%	0.006%
42	6.791	1771	1773	1776	rVB3	1059	422	0.03%	0.004%
43	6.807	1776	1778	1782	rBV3	1118	652	0.05%	0.007%
44	6.865	1794	1796	1798	rBV3	1315	695	0.06%	0.007%
45	7.007	1828	1840	1859	rBV	163349	294903	23.35%	3.005%
46	7.132	1877	1879	1881	rBV3	1098	420	0.03%	0.004%
47	7.264	1918	1920	1924	rBV5	1048	748	0.06%	0.008%
48	7.338	1931	1943	1964	rBV	574781	989589	78.35%	10.083%
49	7.595	2019	2023	2026	rBV3	1022	977	0.08%	0.010%
50	7.643	2028	2038	2057	rVV	117153	203500	16.11%	2.074%
51	8.036	2158	2160	2162	rVB3	1566	629	0.05%	0.006%
52	8.106	2173	2182	2216	rBV	314182	565902	44.81%	5.766%
53	8.740	2376	2379	2381	rBV	958	618	0.05%	0.006%
54	8.871	2409	2420	2442	rBV	610231	993919	78.70%	10.127%
55	9.171	2511	2513	2514	rBV2	1291	455	0.04%	0.005%
56	9.203	2519	2523	2525	rBV4	1028	670	0.05%	0.007%
57	9.344	2563	2567	2570	rBV4	1619	1197	0.09%	0.012%
58	9.643	2658	2660	2663	rVB2	1336	414	0.03%	0.004%
59	9.752	2692	2694	2700	rBV5	1077	794	0.06%	0.008%
60	9.833	2716	2719	2721	rBV2	915	681	0.05%	0.007%
61	9.859	2725	2727	2729	rBV2	996	443	0.04%	0.005%
62	9.926	2745	2748	2750	rBV2	1119	632	0.05%	0.006%
63	9.939	2750	2752	2754	rBV3	939	562	0.04%	0.006%
64	10.052	2784	2787	2788	rBV3	971	490	0.04%	0.005%
65	10.113	2803	2806	2811	rVB5	1451	1239	0.10%	0.013%
66	10.135	2811	2813	2816	rBV2	844	585	0.05%	0.006%
67	10.177	2824	2826	2829	rVB3	1147	569	0.05%	0.006%
68	10.193	2829	2831	2833	rBV3	898	560	0.04%	0.006%
69	10.238	2833	2845	2860	rVV	377632	602285	47.69%	6.137%
70	10.531	2933	2936	2937	rBV	857	505	0.04%	0.005%
71	10.682	2979	2983	2984	rBV3	866	610	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017245.D
 Acq On : 29 Jun 2020 17:35
 Operator : SY/MD
 Sample : L3135-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9Q80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.727	2995	2997	3001	rVB4	1298	739	0.06%	0.008%
73	10.749	3001	3004	3005	rBV2	983	525	0.04%	0.005%
74	10.846	3030	3034	3038	rBV5	1354	1393	0.11%	0.014%
75	11.122	3116	3120	3121	rBV3	986	707	0.06%	0.007%
76	11.174	3134	3136	3138	rBV2	954	565	0.04%	0.006%
77	11.270	3155	3166	3186	rBV	613418	933475	73.91%	9.512%
78	11.431	3214	3216	3218	rBV3	1218	424	0.03%	0.004%
79	11.531	3243	3247	3250	rBV5	817	834	0.07%	0.008%
80	11.646	3272	3283	3301	rVB	625364	964840	76.39%	9.831%
81	11.836	3339	3342	3343	rBV3	933	489	0.04%	0.005%
82	11.894	3357	3360	3364	rBV4	905	802	0.06%	0.008%
83	12.026	3399	3401	3403	rVB3	1496	567	0.04%	0.006%
84	12.039	3403	3405	3412	rVB5	1167	1192	0.09%	0.012%
85	12.068	3412	3414	3415	rBV2	1180	457	0.04%	0.005%
86	12.241	3465	3468	3469	rBV2	848	550	0.04%	0.006%
87	12.537	3556	3560	3564	rBV5	1582	1495	0.12%	0.015%
88	12.694	3606	3609	3610	rBV2	1070	478	0.04%	0.005%
89	12.704	3610	3612	3615	rVB3	1493	763	0.06%	0.008%
90	12.730	3615	3620	3624	rBV6	1226	1239	0.10%	0.013%
91	12.875	3661	3665	3668	rVB4	1340	947	0.07%	0.010%
92	12.900	3668	3673	3674	rBV5	958	721	0.06%	0.007%
93	13.222	3771	3773	3775	rBV3	1067	519	0.04%	0.005%
94	13.405	3827	3830	3834	rBV5	971	665	0.05%	0.007%
95	13.479	3852	3853	3855	rBV2	1186	589	0.05%	0.006%
96	13.604	3889	3892	3895	rBV2	1100	1041	0.08%	0.011%
97	13.694	3918	3920	3922	rVB2	1616	526	0.04%	0.005%
98	13.807	3951	3955	3957	rBV4	1399	972	0.08%	0.010%
99	13.836	3962	3964	3969	rBV6	1437	1128	0.09%	0.011%
100	14.810	4266	4267	4269	rBV2	1084	538	0.04%	0.005%


Sum of corrected areas: 9814114

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062920\
Data File : VV017245.D
Acq On : 29 Jun 2020 17:35
Operator : SY/MD
Sample : L3135-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9Q80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

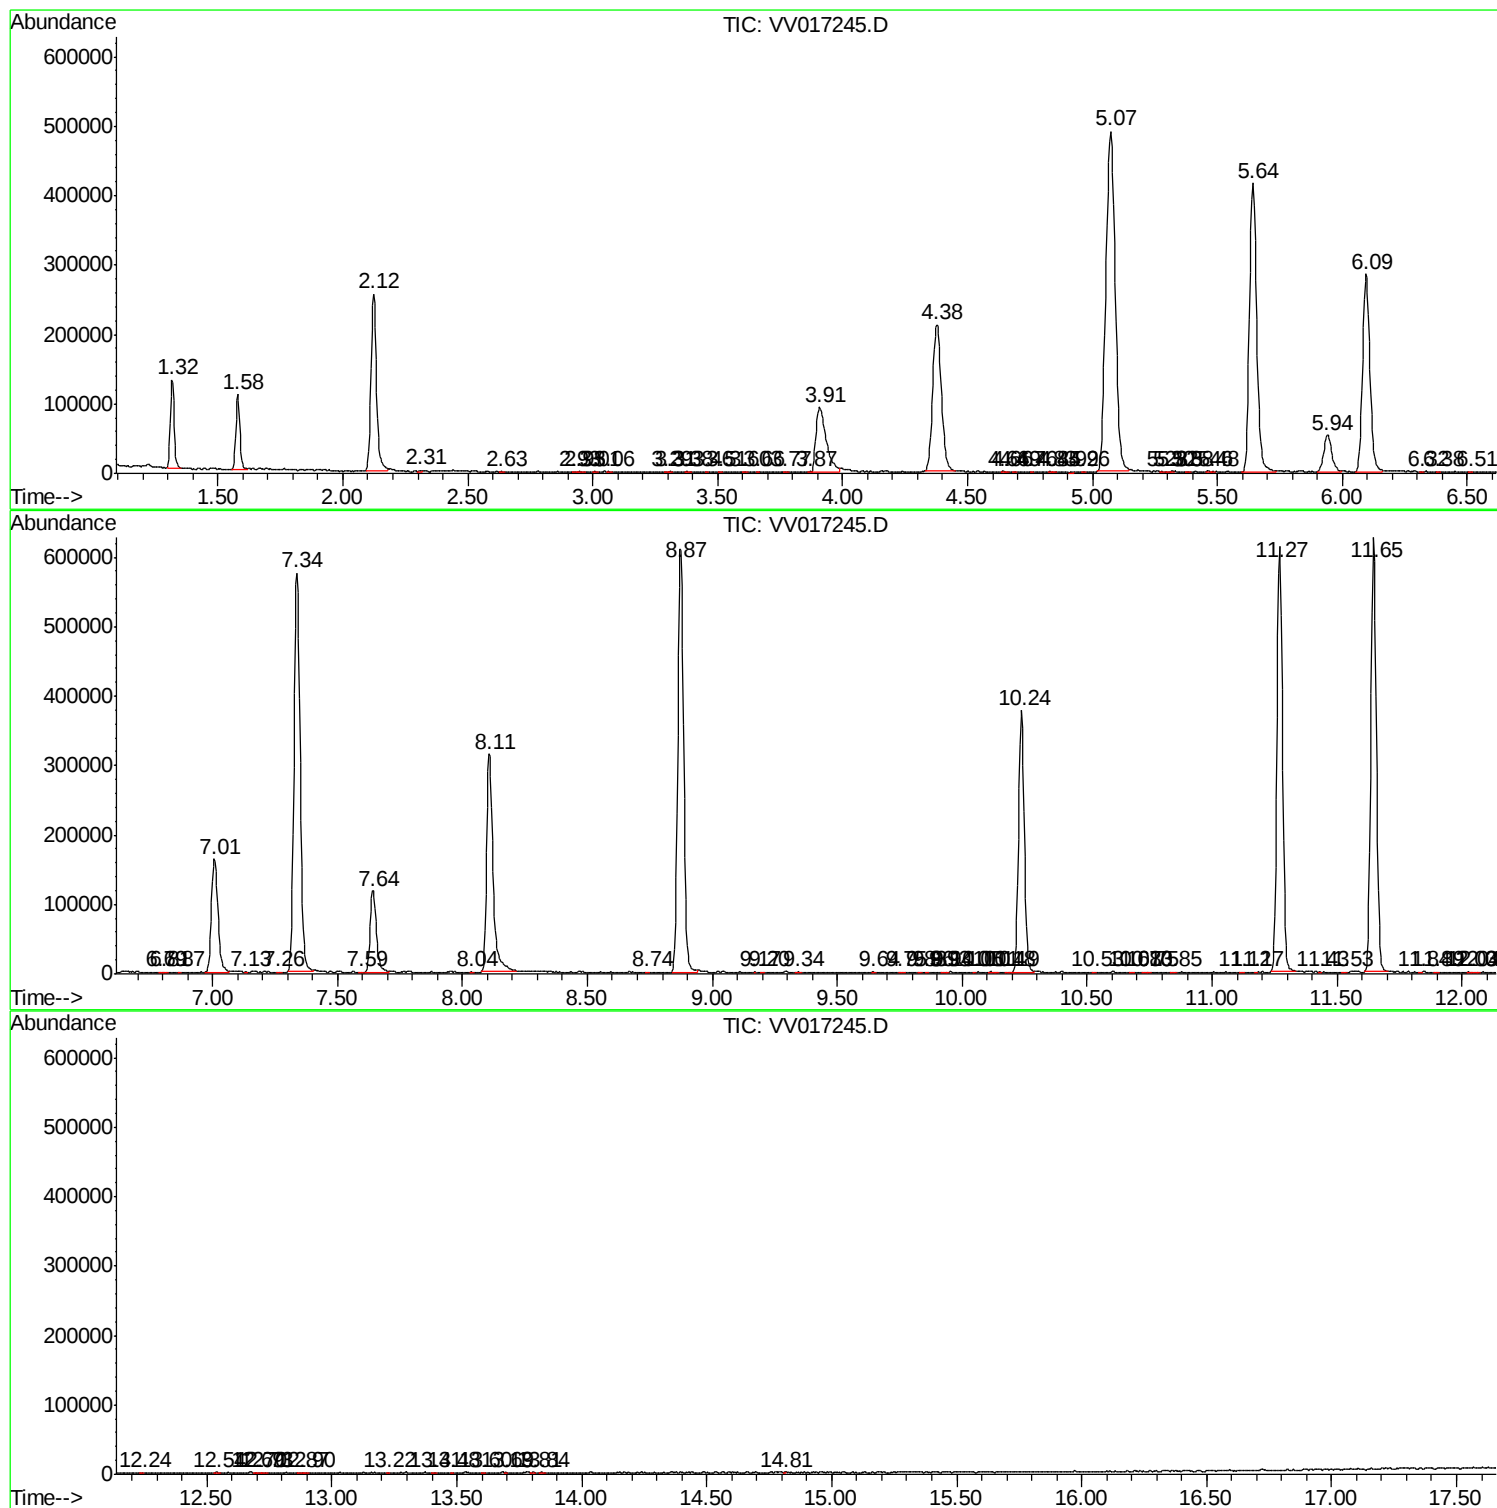

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017245.D
Acq On : 29 Jun 2020 17:35
Operator : SY/MD
Sample : L3135-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062920\
Data File : VV017245.D
Acq On : 29 Jun 2020 17:35
Operator : SY/MD
Sample : L3135-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9Q80

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
