


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062920\
 Data File : VV017225.D
 Acq On : 29 Jun 2020 08:46
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 30 12:05:50 2020

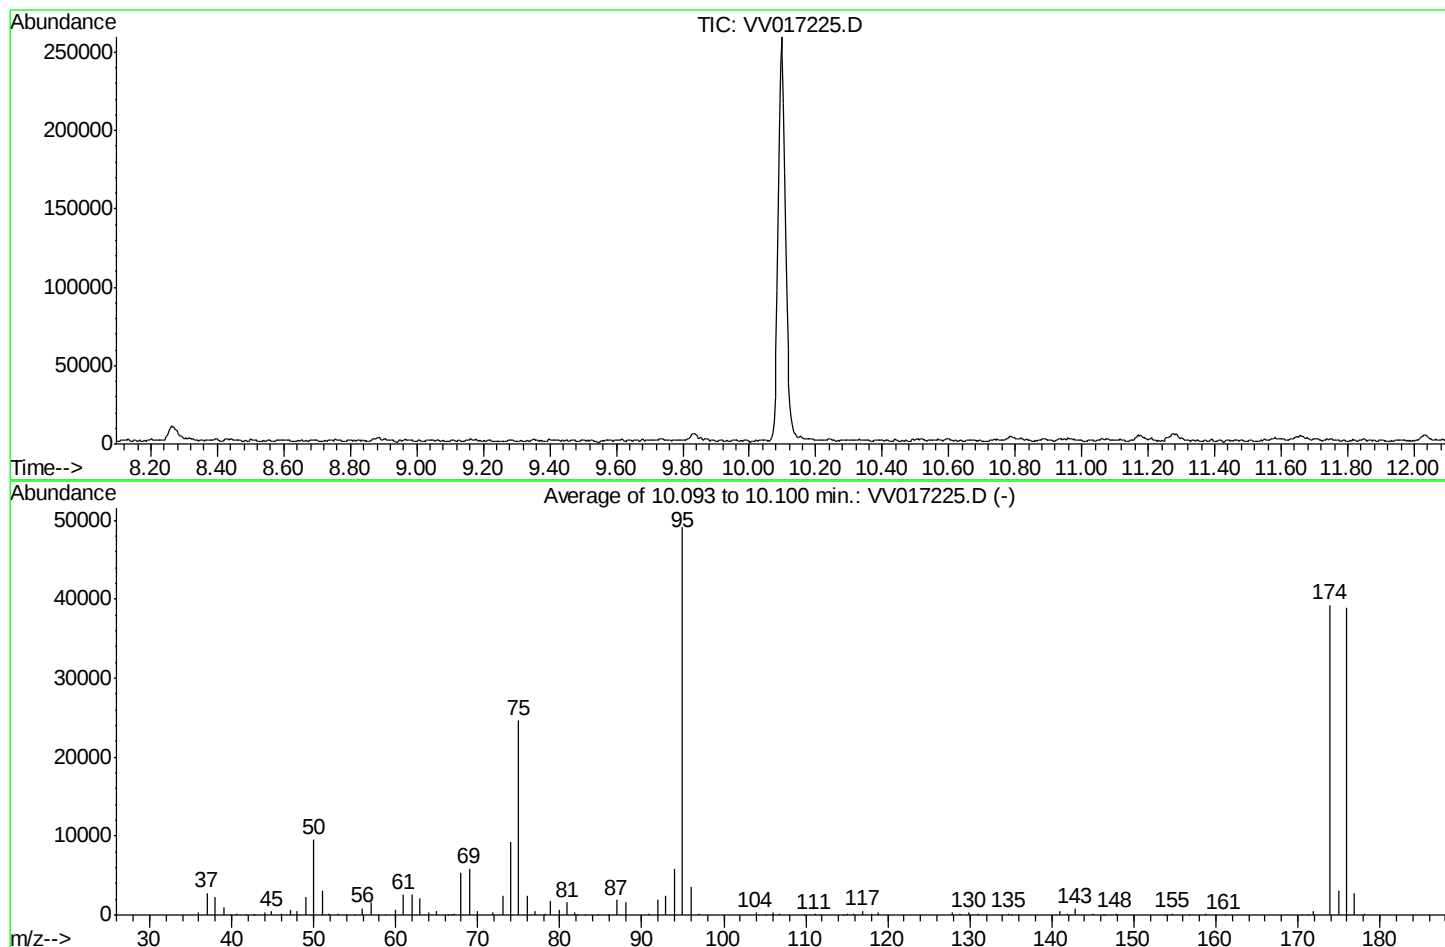

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	9533	PASS
75	95	30	80	50.1	24605	PASS
95	95	100	100	100.0	49128	PASS
96	95	5	9	7.2	3534	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.0	39282	PASS
175	174	5	9	7.8	3057	PASS
176	174	95	101	99.1	38917	PASS
177	176	5	9	7.0	2721	PASS

m/z	Abundance
36.00	498.0
37.00	2785.0
38.00	2327.0
39.00	1159.0
39.90	381.0
40.60	122.0
41.70	105.0
44.10	497.0
44.90	431.0
46.00	141.0
47.10	454.0
48.00	469.0
49.00	2408.0
50.00	9204.0
51.00	2924.0
51.90	198.0
52.90	144.0
53.80	116.0
54.80	185.0
55.90	906.0
57.00	1353.0
57.90	124.0
59.90	589.0
61.00	2551.0
62.00	2546.0
63.00	2129.0
63.90	266.0
65.00	495.0
66.40	120.0
67.20	171.0
68.00	5175.0
69.00	5707.0
70.00	458.0
71.90	282.0
73.00	2351.0
74.00	8878.0
75.00	24088.0
76.00	2494.0
77.10	448.0
78.90	1813.0
80.00	539.0
80.90	1564.0
81.90	411.0
82.10	422.0
83.10	147.0
85.80	110.0
86.90	1900.0
88.00	1544.0
90.90	221.0
92.00	1756.0
92.90	2245.0
94.00	5545.0
95.00	48112.0
96.00	3631.0
96.90	168.0
103.90	291.0
106.00	271.0
106.70	131.0
111.10	134.0
111.80	113.0
114.60	119.0
115.10	112.0
115.80	154.0
117.00	442.0
118.00	155.0
118.70	290.0
127.80	248.0
128.80	152.0
130.00	250.0
131.00	140.0
134.80	184.0
140.90	428.0
141.80	128.0
142.90	799.0
144.90	220.0
146.20	110.0
146.50	119.0
147.80	203.0
154.80	173.0
156.70	134.0
158.80	142.0
161.10	140.0
170.50	118.0
171.90	501.0
173.90	37032.0
174.90	2992.0
175.90	37224.0
176.90	2594.0
178.10	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	541.0
37.00	2917.0
38.00	2526.0
39.00	1180.0
39.90	411.0
40.70	111.0
42.60	125.0
44.00	513.0
44.90	477.0
46.00	141.0
47.10	637.0
48.00	540.0
49.00	2417.0
50.00	10025.0
51.00	3246.0
51.90	232.0
52.90	148.0
53.90	134.0
54.90	154.0
55.90	896.0
57.00	1672.0
57.90	133.0
58.70	119.0
60.00	740.0
61.00	2664.0
62.00	2577.0
63.00	2208.0
64.00	285.0
65.00	504.0
67.10	204.0
68.00	5610.0
69.00	6159.0
70.00	443.0
71.90	271.0
73.00	2593.0
74.00	9494.0
75.00	25400.0
76.00	2485.0
77.10	418.0
78.20	243.0
78.90	1778.0
80.00	605.0
80.90	1695.0
81.80	412.0
84.70	107.0
85.80	106.0
86.90	2028.0
88.00	1669.0
90.80	248.0
92.00	1919.0
93.00	2449.0
94.00	6040.0
95.00	51064.0
96.00	3720.0
96.90	177.0
103.90	332.0
105.00	106.0
106.00	314.0
106.70	128.0
109.80	107.0
111.20	160.0
114.60	115.0
115.00	145.0
115.80	169.0
117.00	543.0
117.90	187.0
118.70	359.0
127.80	260.0
128.90	151.0
129.90	273.0
131.00	149.0
134.80	205.0
135.00	191.0
140.90	517.0
141.90	159.0
142.90	821.0
145.00	242.0
147.80	190.0
154.70	184.0
156.70	103.0
158.80	172.0
170.30	115.0
171.20	132.0
171.90	567.0
173.90	40600.0
174.90	3136.0
175.90	40328.0
176.90	2860.0
178.10	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	537.0
37.00	2673.0
38.00	2442.0
39.00	1086.0
39.90	436.0
40.70	109.0
42.80	128.0
43.90	549.0
44.90	447.0
46.00	148.0
47.10	659.0
48.00	482.0
49.00	2092.0
50.00	9689.0
51.00	3170.0
51.90	261.0
53.00	141.0
55.00	185.0
56.00	823.0
57.00	1807.0
57.90	124.0
58.70	114.0
60.00	756.0
60.90	2425.0
62.00	2445.0
63.00	2026.0
64.10	313.0
65.00	479.0
66.90	250.0
68.00	5350.0
69.00	5809.0
70.00	373.0
71.90	244.0
73.00	2493.0
74.00	9184.0
75.00	24328.0
76.00	2171.0
77.00	378.0
78.20	293.0
78.90	1546.0
80.00	615.0
80.90	1593.0
81.80	371.0
84.70	117.0
87.00	1891.0
88.00	1651.0
90.90	246.0
92.00	2007.0
93.00	2535.0
94.00	6045.0
95.00	48208.0
96.00	3252.0
96.90	152.0
103.90	331.0
105.00	117.0
106.00	304.0
106.80	116.0
111.20	120.0
114.90	139.0
115.80	169.0
117.00	528.0
118.00	208.0
118.80	405.0
127.90	244.0
128.90	134.0
129.90	272.0
131.00	138.0
134.70	201.0
140.90	612.0
141.90	188.0
142.90	749.0
145.00	214.0
147.80	144.0
153.80	114.0
154.80	152.0
158.80	166.0
171.90	639.0
173.90	40216.0
175.00	3045.0
175.90	39200.0
176.90	2709.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
35.10	137.0
35.90	117.0
38.10	105.0
39.20	136.0
39.80	359.0
43.20	115.0
44.00	229.0
46.50	106.0
49.30	131.0
50.00	106.0
55.10	109.0
58.00	137.0
64.40	111.0
82.20	107.0
83.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95