


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062920\
 Data File : VV017249.D
 Acq On : 30 Jun 2020 09:24
 Operator : SY/MD
 Sample : BFB96
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB96

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 30 14:18:07 2020

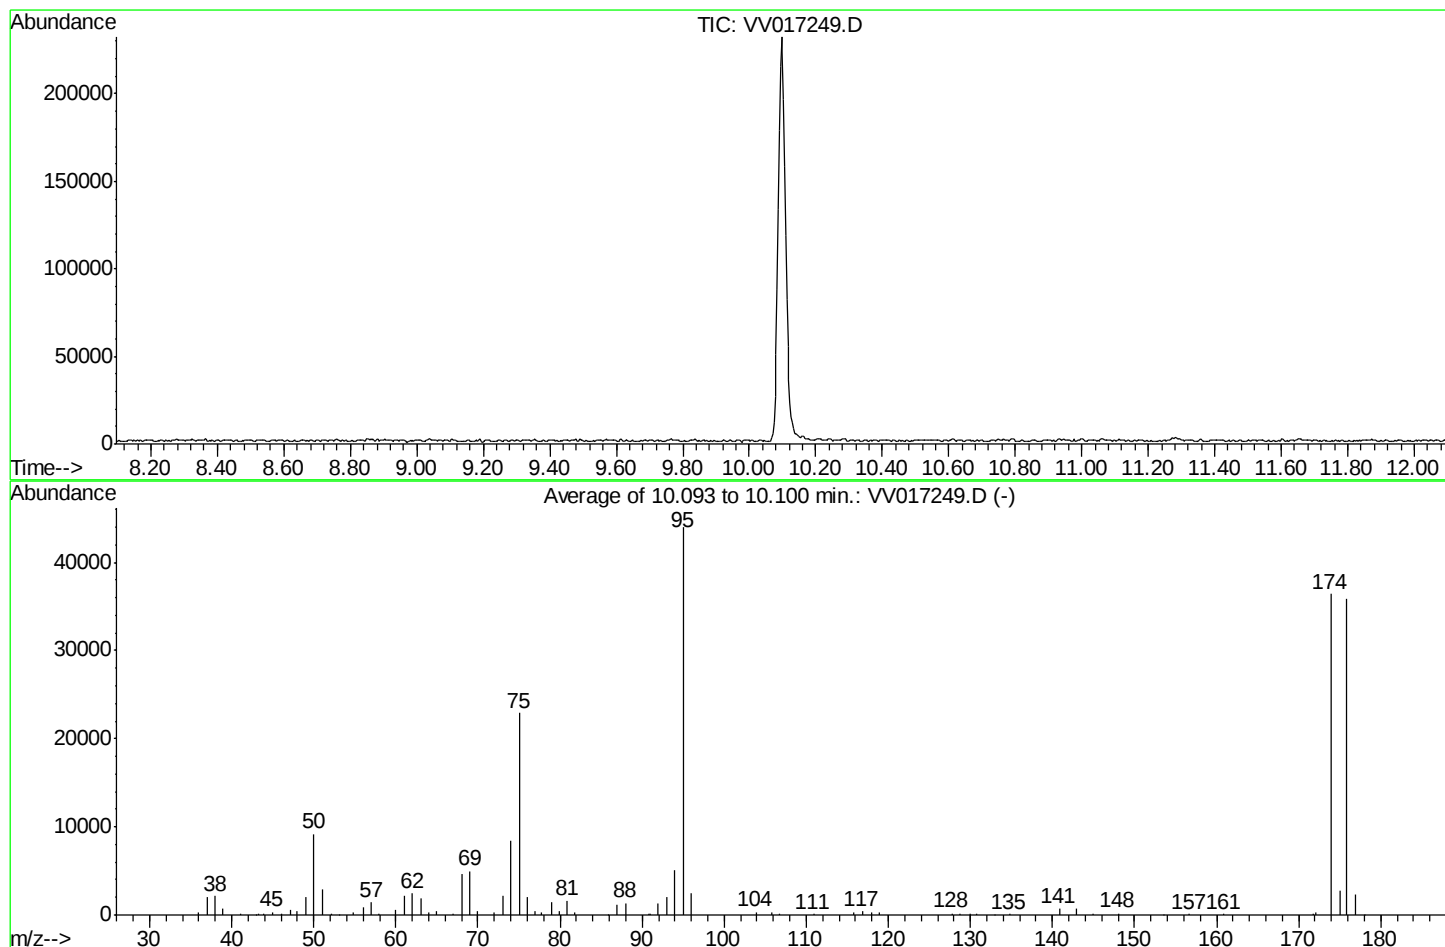

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	9207	PASS
75	95	30	80	52.1	22920	PASS
95	95	100	100	100.0	43973	PASS
96	95	5	9	5.7	2516	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.9	36442	PASS
175	174	5	9	7.6	2780	PASS
176	174	95	101	98.4	35874	PASS
177	176	5	9	6.6	2376	PASS

m/z	Abundance
35.90	348.0
37.00	2145.0
38.00	2196.0
39.00	869.0
39.90	285.0
41.20	133.0
43.20	234.0
44.10	533.0
45.00	359.0
46.10	167.0
47.20	514.0
47.90	414.0
49.00	1913.0
50.00	9068.0
51.00	3029.0
52.10	159.0
54.90	219.0
56.00	758.0
57.00	1289.0
60.00	573.0
61.00	2155.0
62.00	2293.0
63.10	1830.0
63.90	266.0
64.90	440.0
66.90	166.0
68.00	4612.0
69.00	5283.0
69.90	484.0
72.00	339.0
73.00	2142.0
74.00	8243.0
75.00	22464.0
76.00	1947.0
76.90	404.0
77.70	215.0
78.90	1451.0
79.80	439.0
80.90	1597.0
81.80	326.0
85.80	104.0
86.90	1312.0
87.90	1429.0
90.80	198.0
91.00	195.0
91.90	1213.0
93.00	1830.0
94.00	4855.0
95.00	41576.0
96.10	2597.0
103.90	322.0
105.80	235.0
110.90	164.0
115.80	287.0
116.90	396.0
117.90	262.0
119.00	212.0
127.70	206.0
128.70	124.0
129.90	131.0
130.80	126.0
132.90	108.0
134.70	125.0
140.80	773.0
142.90	587.0
144.90	153.0
148.00	163.0
172.10	527.0
174.00	34400.0
175.00	2688.0
175.90	33728.0
176.90	2166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
36.00	384.0
37.00	2128.0
38.00	2222.0
39.00	994.0
39.90	261.0
41.10	114.0
43.20	160.0
44.00	595.0
45.00	314.0
46.10	139.0
47.20	543.0
47.90	429.0
49.00	2106.0
50.00	9570.0
51.00	3047.0
52.10	184.0
53.10	104.0
54.80	247.0
56.00	908.0
57.00	1448.0
57.90	100.0
60.00	610.0
61.00	2321.0
62.00	2581.0
63.10	2071.0
64.00	274.0
65.00	420.0
66.90	170.0
68.00	4815.0
69.00	5140.0
69.90	453.0
71.80	353.0
73.00	2317.0
74.00	8952.0
75.00	23880.0
76.00	2047.0
76.90	388.0
77.80	238.0
78.90	1602.0
79.90	521.0
80.90	1642.0
81.80	331.0
86.90	1238.0
88.00	1418.0
90.80	206.0
91.90	1329.0
93.00	2016.0
94.00	5327.0
95.00	45568.0
96.10	2561.0
103.90	317.0
105.70	239.0
106.80	135.0
110.90	140.0
115.90	250.0
116.80	395.0
117.90	241.0
118.90	279.0
127.70	200.0
128.80	133.0
129.90	169.0
130.80	163.0
134.80	127.0
140.90	764.0
142.90	689.0
145.00	185.0
148.00	160.0
156.70	110.0
160.90	119.0
172.00	557.0
174.00	37680.0
175.00	2880.0
175.90	37208.0
177.00	2470.0
178.00	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
36.00	446.0
37.00	1937.0
38.00	2001.0
39.00	872.0
39.90	281.0
42.90	174.0
43.90	635.0
44.90	293.0
47.10	507.0
47.90	372.0
49.00	2152.0
50.00	8984.0
51.00	2808.0
52.20	198.0
53.20	107.0
54.80	242.0
56.00	894.0
57.00	1452.0
58.00	152.0
60.00	563.0
61.00	2252.0
62.00	2516.0
63.10	1981.0
64.00	283.0
65.10	470.0
66.90	164.0
68.00	4493.0
69.00	4422.0
69.90	421.0
71.90	327.0
73.00	2229.0
74.00	8138.0
75.00	22416.0
76.00	1905.0
76.90	355.0
77.80	234.0
78.90	1484.0
79.90	553.0
80.90	1567.0
81.90	330.0
86.90	1151.0
87.90	1286.0
90.90	200.0
92.00	1324.0
93.00	2130.0
94.00	5258.0
95.00	44776.0
96.00	2391.0
103.90	257.0
105.70	216.0
106.80	157.0
115.80	213.0
116.80	328.0
118.00	199.0
118.90	356.0
127.80	192.0
128.80	133.0
129.90	201.0
130.80	134.0
134.80	101.0
140.90	631.0
142.90	704.0
144.90	139.0
148.00	132.0
153.60	107.0
156.70	125.0
160.90	153.0
171.80	528.0
173.90	37248.0
175.00	2772.0
175.90	36688.0
177.00	2494.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
36.00	112.0
36.40	126.0
38.90	179.0
39.90	302.0
43.90	409.0
46.60	153.0
61.70	116.0
81.50	126.0
83.10	115.0
97.50	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96