


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062921\
 Data File : VV021570.D
 Acq On : 29 Jun 2021 09:14
 Operator : SY/MD
 Sample : BFB174
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB174

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis
 Last Update : Thu Jul 01 01:50:41 2021

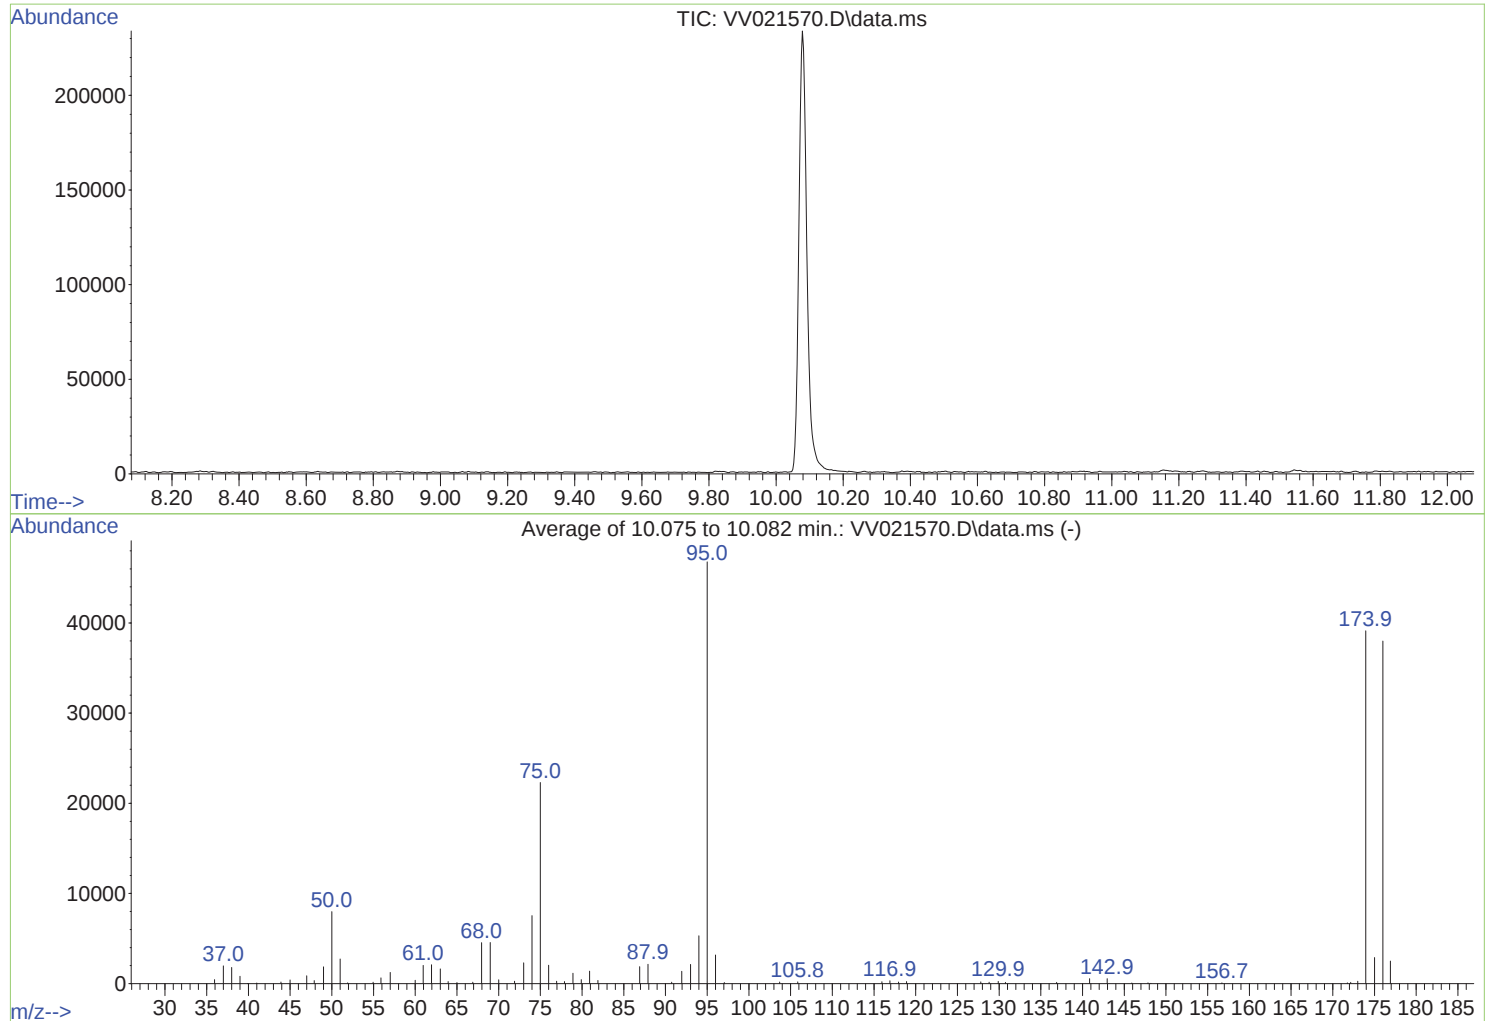

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	7989	PASS
75	95	30	80	47.7	22307	PASS
95	95	100	100	100.0	46776	PASS
96	95	5	9	6.8	3175	PASS
173	174	0.00	2	0.7	269	PASS
174	95	50	120	83.7	39133	PASS
175	174	5	9	7.4	2896	PASS
176	174	95	105	97.1	37987	PASS
177	176	5	10	6.6	2504	PASS

m/z	Abundance
39.90	196.0
43.00	107.0
43.90	674.0

Instrument :
MSVOA_V
ClientSampleId :
BFB174

m/z	Abundance
36.00	470.0
37.00	1951.0
38.00	1725.0
39.00	766.0
39.80	282.0
43.10	117.0
43.90	863.0
45.00	426.0
47.00	821.0
47.90	302.0
49.00	1867.0
50.00	8090.0
51.00	2770.0
51.90	163.0
55.00	168.0
55.90	655.0
57.00	1330.0
60.00	368.0
60.90	2054.0
62.00	2149.0
63.00	1533.0
64.00	217.0
65.00	107.0
66.90	140.0
67.90	4456.0
69.00	4554.0
70.00	446.0
71.90	276.0
73.00	2255.0
74.00	7371.0
75.00	21992.0
76.00	2135.0
77.00	278.0
77.90	193.0
78.90	1130.0
79.90	451.0
80.90	1438.0
81.90	331.0
86.90	1933.0
87.90	2151.0
90.90	173.0
91.90	1221.0
93.00	2042.0
94.00	5020.0
95.00	45896.0
96.00	3174.0
97.10	108.0
103.70	192.0
105.90	172.0
115.90	188.0
116.90	309.0
117.90	230.0
118.90	196.0
127.80	181.0
128.70	136.0
129.90	229.0
130.80	127.0
136.90	116.0
140.80	543.0
142.90	584.0
145.90	128.0
147.80	130.0
171.70	116.0
172.20	128.0
174.00	37984.0
175.00	2864.0
176.00	36376.0
176.90	2411.0

Instrument :
MSVOA_V
ClientSampleId :
BFB174

m/z	Abundance
35.90	447.0
37.00	2020.0
38.00	1832.0
39.00	836.0
39.90	206.0
41.00	106.0
43.90	850.0
45.00	426.0
47.00	914.0
47.90	362.0
49.00	1934.0
50.00	8149.0
51.00	2809.0
51.90	131.0
54.90	169.0
55.90	652.0
57.00	1281.0
60.00	366.0
61.00	2060.0
61.90	2145.0
63.00	1719.0
64.00	253.0
65.00	122.0
66.90	170.0
67.90	4696.0
69.00	4745.0
70.00	423.0
71.90	263.0
73.00	2463.0
74.00	7741.0
75.00	22952.0
76.00	2111.0
76.90	281.0
77.90	226.0
78.90	1167.0
79.90	441.0
80.90	1408.0
81.90	364.0
86.90	1865.0
87.90	2207.0
90.70	150.0
91.90	1427.0
93.00	2178.0
94.00	5460.0
95.00	48264.0
96.00	3248.0
97.00	148.0
103.70	197.0
105.80	204.0
115.90	233.0
116.90	327.0
117.90	190.0
118.90	225.0
127.80	196.0
128.80	169.0
129.90	271.0
130.80	144.0
136.90	147.0
140.90	571.0
142.90	586.0
145.90	112.0
147.90	119.0
156.70	136.0
171.80	140.0
172.20	143.0
173.00	400.0
173.90	40368.0
175.00	2995.0
176.00	39328.0
176.90	2598.0

Instrument :
MSVOA_V
ClientSampleId :
BFB174

m/z	Abundance
35.90	404.0
37.00	1929.0
38.00	1796.0
39.00	830.0
40.00	169.0
41.00	116.0
44.00	845.0
45.00	378.0
47.00	862.0
47.90	378.0
49.00	1806.0
50.00	7729.0
51.00	2634.0
54.90	147.0
55.90	629.0
57.00	1142.0
60.00	374.0
61.00	1971.0
61.90	2015.0
63.00	1649.0
63.90	243.0
65.00	131.0
66.90	168.0
68.00	4479.0
69.00	4406.0
70.00	395.0
71.90	245.0
73.00	2207.0
74.00	7510.0
75.00	21976.0
76.00	1888.0
77.00	244.0
77.90	252.0
78.90	1179.0
79.90	417.0
80.90	1289.0
81.90	365.0
86.90	1837.0
87.90	2101.0
90.70	150.0
92.00	1453.0
93.00	2183.0
94.00	5455.0
95.00	46168.0
96.00	3103.0
97.00	142.0
103.70	172.0
105.80	213.0
116.00	226.0
116.90	311.0
118.00	140.0
118.90	278.0
127.80	189.0
128.90	163.0
129.90	257.0
130.70	132.0
136.90	157.0
140.90	539.0
143.00	495.0
148.20	113.0
156.70	139.0
172.00	148.0
173.00	406.0
173.90	39048.0
175.00	2828.0
176.00	38256.0
176.90	2502.0

Instrument :
MSVOA_V
ClientSampleId :
BFB174