

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062923\
 Data File : VW031618.D
 Acq On : 29 Jun 2023 13:38
 Operator : SY/MD
 Sample : 03422-20ME
 Misc : 4.32g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46L7ME

Quant Time: Jun 30 04:27:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 30 04:25:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	236604	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	238783	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	124590	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	68222	43.325	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.640%
7) Chloroethane-d5	1.667	69	159	0.116	ug/L	0.13
Spiked Amount	50.000	Range	70 - 130	Recovery	=	0.240%#
11) 1,1-Dichloroethene-d2	2.047	65	34941	43.054	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.100%
21) 2-Butanone-d5	3.799	46	102163	80.124	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.120%
24) Chloroform-d	4.252	84	151751	38.480	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.960%
26) 1,2-Dichloroethane-d4	4.947	65	98802	40.043	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.080%
32) Benzene-d6	4.963	84	250136	37.216	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.440%
36) 1,2-Dichloropropane-d6	5.995	67	95698	40.172	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.340%
41) Toluene-d8	7.249	98	199857	32.403	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	64.800%#
43) trans-1,3-Dichloroprop...	7.561	79	41743	35.945	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.880%
47) 2-Hexanone-d5	8.043	63	74626	79.341	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.340%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	150491	41.853	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.700%
66) 1,2-Dichlorobenzene-d4	11.567	152	95091	40.040	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.080%
Target Compounds						Qvalue
13) Acetone	2.127	43	5477	4.353	ug/L	99
15) Methyl Acetate	2.381	43	30989	14.629	ug/L	96
61) 1,2,3-Trichloropropane	11.191	75	16190	6.579	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031618.D
Acq On : 29 Jun 2023 13:38
Operator : SY/MD
Sample : 03422-20ME
Misc : 4.32g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46L7ME

Quant Time: Jun 30 04:27:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 30 04:25:13 2023
Response via : Initial Calibration

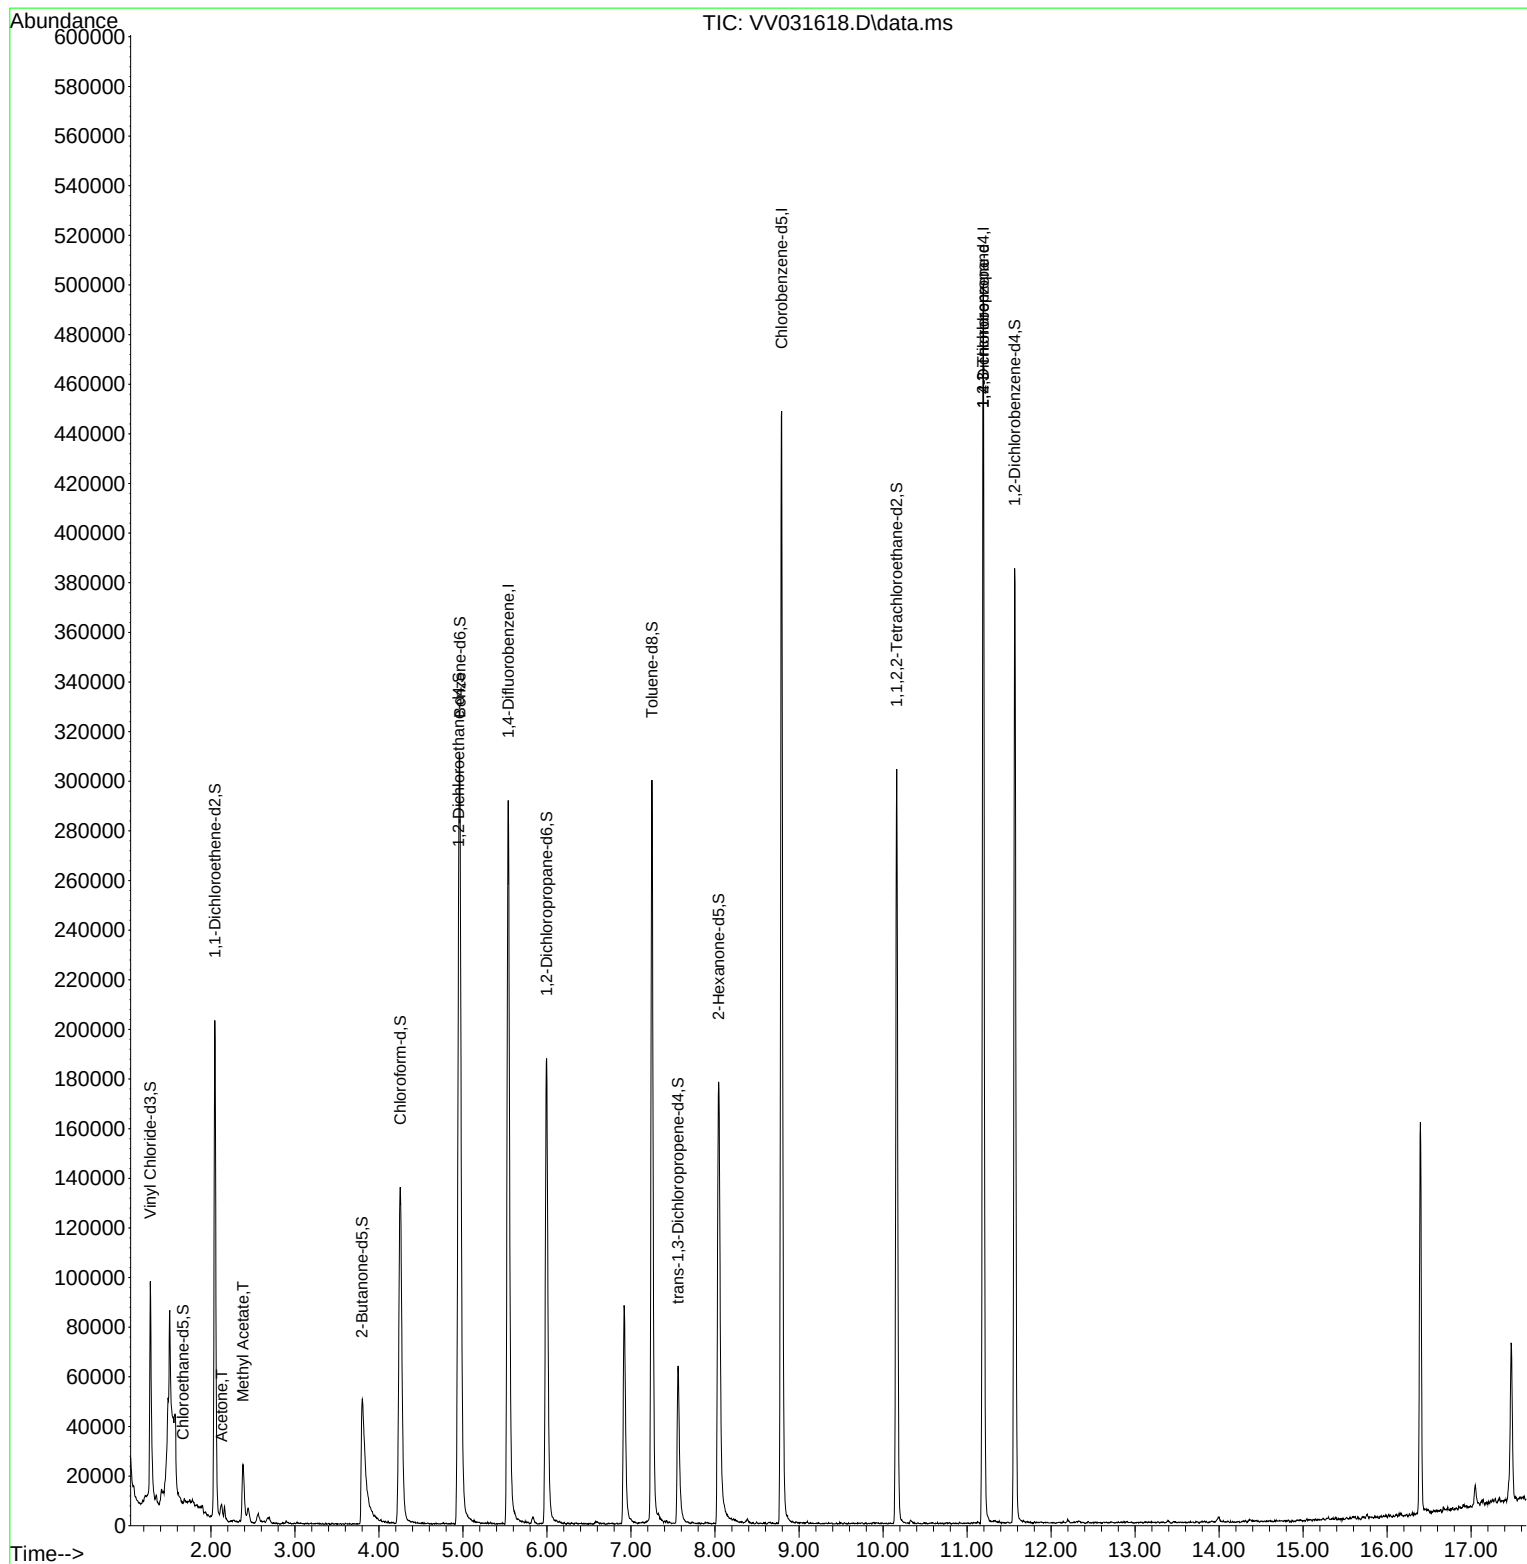

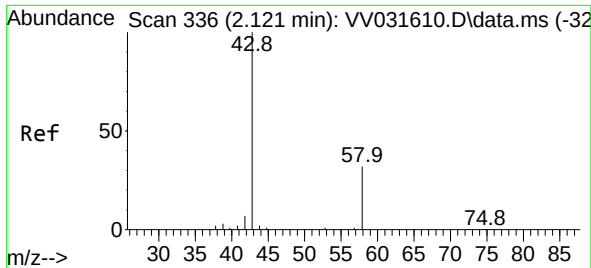

#13

Acetone

Concen: 4.353 ug/L

RT: 2.127 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV031618.D

Acq: 29 Jun 2023 13:38

Instrument :

MSVOA_V

ClientSampleId :





A46L7ME

Tgt Ion: 43 Resp: 5477

Ion Ratio Lower Upper

43 100

58 33.8 0.0 68.6

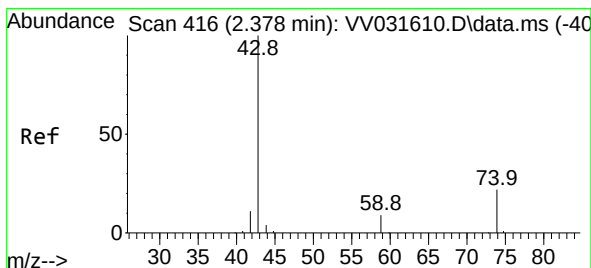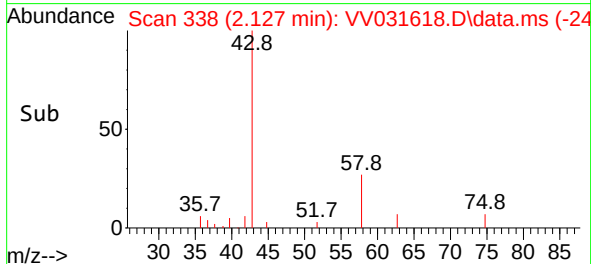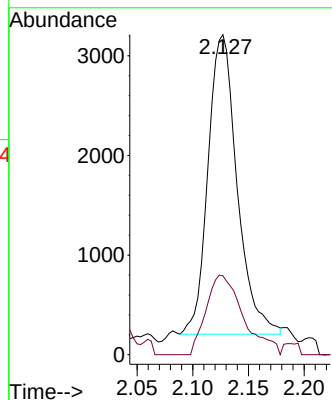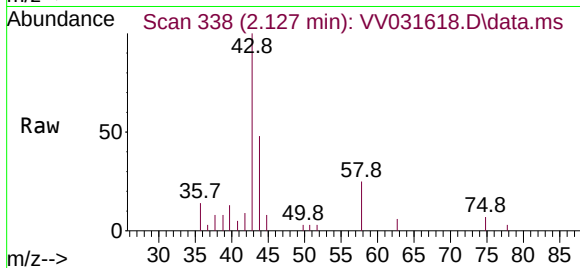

#15

Methyl Acetate

Concen: 14.629 ug/L

RT: 2.381 min Scan# 417

Delta R.T. 0.003 min

Lab File: VV031618.D




Acq: 29 Jun 2023 13:38


Tgt Ion: 43 Resp: 30989

Ion Ratio Lower Upper

43 100

74 20.4 17.8 26.6

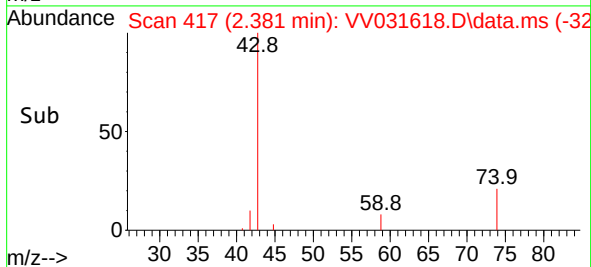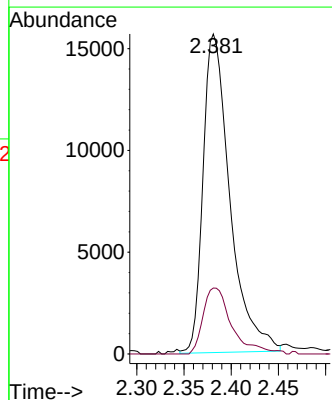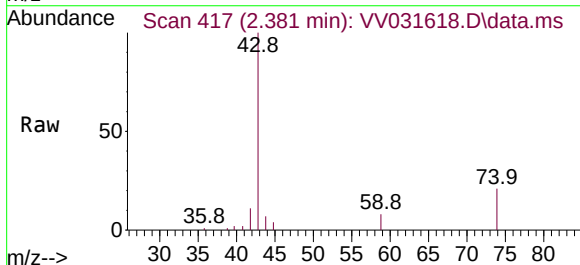

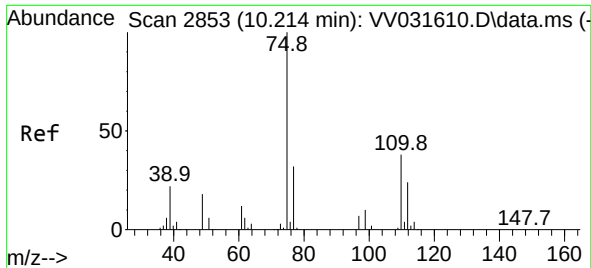

#61
 1,2,3-Trichloropropane
 Concen: 6.579 ug/L
 RT: 11.191 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV031618.D
 Acq: 29 Jun 2023 13:38

Instrument :
 MSVOA_V
 ClientSampleId :
 A46L7ME

Tgt Ion: 75 Resp: 16190
 Ion Ratio Lower Upper
 75 100
 77 36.3 25.4 38.0
 110 1.9 31.3 46.9#

