

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031619.D
 Acq On : 29 Jun 2023 14:01
 Operator : SY/MD
 Sample : 03422-03ME
 Misc : 4.76g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46J2ME

Quant Time: Jun 30 04:27:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 30 04:25:13 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.539	114	287822	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.793	117	281923	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.194	152	142906	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	104549	54.579	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	109.160%	
7) Chloroethane-d5		1.519	69	47040	28.144	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	56.280%#	
11) 1,1-Dichloroethene-d2		2.050	65	51766	52.435	ug/L	-0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.880%	
21) 2-Butanone-d5		3.802	46	172670	111.323	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.320%	
24) Chloroform-d		4.252	84	225736	47.054	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.100%	
26) 1,2-Dichloroethane-d4		4.947	65	148842	49.589	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.180%	
32) Benzene-d6		4.963	84	380769	47.983	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.960%	
36) 1,2-Dichloropropane-d6		5.992	67	142581	50.694	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.380%	
41) Toluene-d8		7.249	98	305006	41.884	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.760%	
43) trans-1,3-Dichloroprop...		7.558	79	61150	44.598	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.200%	
47) 2-Hexanone-d5		8.047	63	117626	105.921	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.920%	
56) 1,1,2,2-Tetrachloroeth...		10.162	84	215741	50.818	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.640%	
66) 1,2-Dichlorobenzene-d4		11.571	152	137001	50.293	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.580%	
Target Compounds						Qvalue	
15) Methyl Acetate		2.381	43	25022	9.710	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031619.D
Acq On : 29 Jun 2023 14:01
Operator : SY/MD
Sample : 03422-03ME
Misc : 4.76g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46J2ME

Quant Time: Jun 30 04:27:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 30 04:25:13 2023
Response via : Initial Calibration

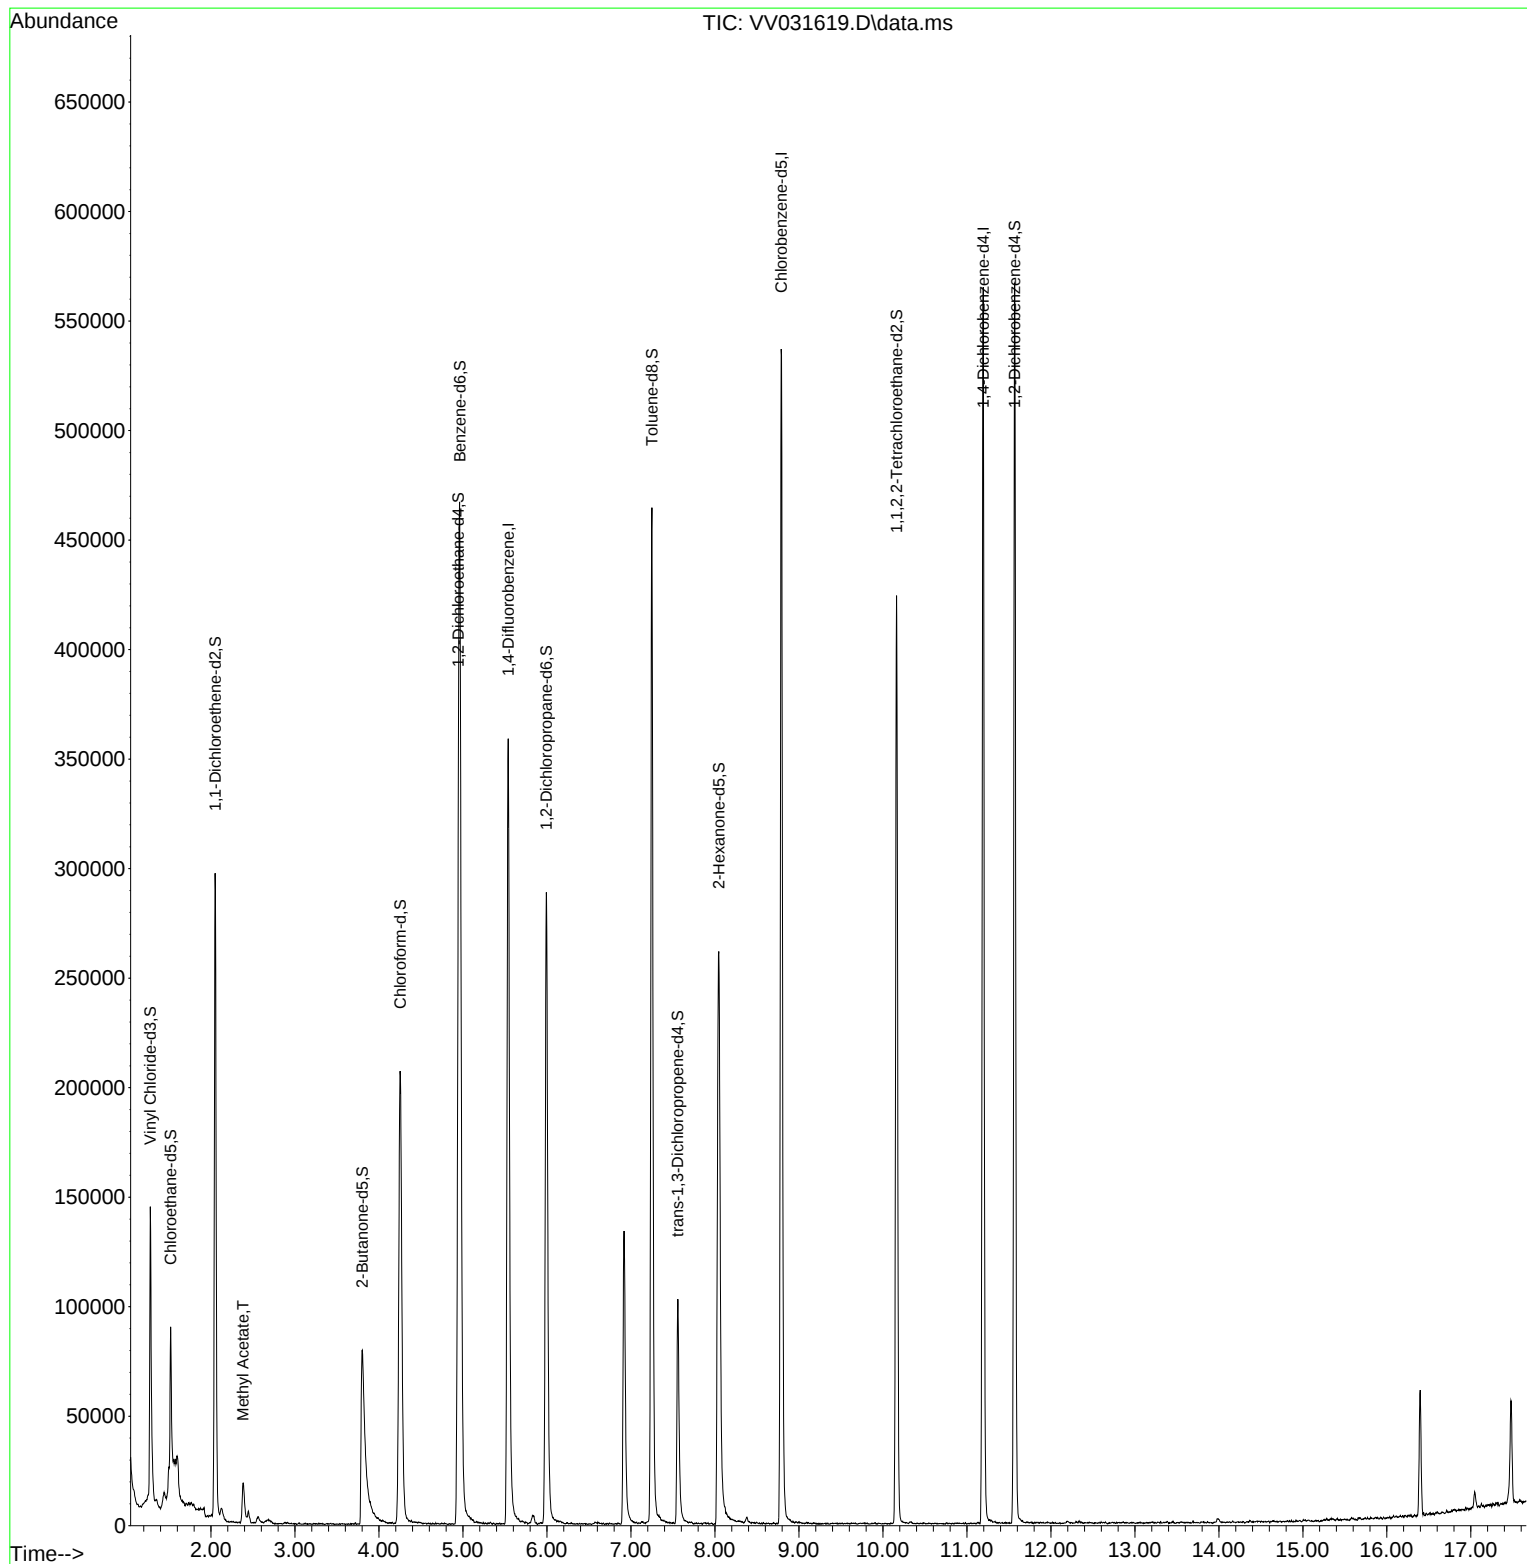

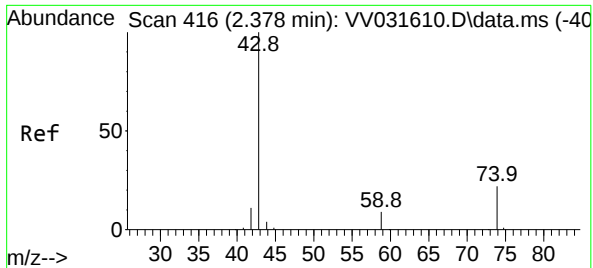

#15
Methyl Acetate
Concen: 9.710 ug/L
RT: 2.381 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV031619.D
Acq: 29 Jun 2023 14:01

Instrument :
MSVOA_V
ClientSampleId :
A46J2ME

Tgt Ion: 43 Resp: 25022
Ion Ratio Lower Upper
43 100
74 21.8 17.8 26.6

