

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031612.D
 Acq On : 29 Jun 2023 11:00
 Operator : SY/MD
 Sample : VV0629WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK363

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	96985	109108	14.37%	1.812%
2	1.532	147	153	165	rVB	91242	107641	14.17%	1.788%
3	2.063	308	318	333	rBV	214549	314690	41.44%	5.227%
4	3.310	704	706	708	rVB	311	130	0.02%	0.002%
5	3.371	722	725	728	rBV3	326	238	0.03%	0.004%
6	3.387	728	730	731	rBV3	208	80	0.01%	0.001%
7	3.648	808	811	813	rBV2	295	216	0.03%	0.004%
8	3.744	839	841	842	rBV2	125	60	0.01%	0.001%
9	3.793	846	856	890	rBV	60066	166686	21.95%	2.769%
10	4.256	984	1000	1022	rBV	133625	338745	44.61%	5.627%
11	4.545	1085	1090	1092	rBV2	364	352	0.05%	0.006%
12	4.715	1140	1143	1144	rBV	270	163	0.02%	0.003%
13	4.773	1159	1161	1167	rVB2	389	261	0.03%	0.004%
14	4.809	1168	1172	1176	rBV3	283	259	0.03%	0.004%
15	4.963	1202	1220	1250	rBV2	284249	759386	100.00%	12.614%
16	5.320	1328	1331	1332	rBV	367	161	0.02%	0.003%
17	5.339	1335	1337	1342	rBV2	266	205	0.03%	0.003%
18	5.397	1354	1355	1359	rBV	441	176	0.02%	0.003%
19	5.461	1372	1375	1378	rVB2	201	114	0.02%	0.002%
20	5.542	1387	1400	1423	rBV	234894	492406	64.84%	8.180%
21	5.789	1474	1477	1480	rBV3	382	307	0.04%	0.005%
22	5.831	1483	1490	1503	rVB9	1914	4007	0.53%	0.067%
23	5.918	1516	1517	1519	rBV9	157	77	0.01%	0.001%
24	5.995	1527	1541	1561	rBV	181126	373645	49.20%	6.207%
25	6.262	1622	1624	1626	rBV	244	99	0.01%	0.002%
26	6.336	1645	1647	1650	rBV2	186	73	0.01%	0.001%
27	6.400	1666	1667	1669	rVB	197	68	0.01%	0.001%
28	6.423	1669	1674	1678	rBV3	233	299	0.04%	0.005%
29	6.452	1680	1683	1686	rBV2	287	235	0.03%	0.004%
30	6.513	1701	1702	1703	rBV2	172	49	0.01%	0.001%
31	6.526	1703	1706	1707	rBV2	260	155	0.02%	0.003%
32	6.638	1738	1741	1743	rBV3	307	188	0.02%	0.003%
33	6.696	1757	1759	1761	rBV	188	104	0.01%	0.002%
34	6.799	1789	1791	1792	rBV	221	85	0.01%	0.001%
35	6.863	1809	1811	1812	rBV	149	47	0.01%	0.001%
36	6.918	1817	1828	1849	rBV2	84395	159363	20.99%	2.647%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031612.D
 Acq On : 29 Jun 2023 11:00
 Operator : SY/MD
 Sample : VV0629WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK363

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	7.101	1879	1885	1889	rBV4	630	657	0.09%	0.011%
38	7.194	1912	1914	1918	rBV2	446	328	0.04%	0.005%
39	7.249	1918	1931	1963	rBV	282785	510457	67.22%	8.479%
40	7.558	2017	2027	2047	rBV2	65652	117250	15.44%	1.948%
41	7.908	2135	2136	2138	rBV2	185	94	0.01%	0.002%
42	7.921	2138	2140	2143	rVB	538	229	0.03%	0.004%
43	7.953	2146	2150	2151	rBV	309	198	0.03%	0.003%
44	7.995	2160	2163	2164	rBV	275	130	0.02%	0.002%
45	8.030	2164	2174	2203	rBV	206297	377511	49.71%	6.271%
46	8.429	2294	2298	2303	rBV3	376	339	0.04%	0.006%
47	8.500	2317	2320	2322	rBV	378	207	0.03%	0.003%
48	8.789	2399	2410	2432	rBV	370066	616151	81.14%	10.235%
49	9.464	2613	2620	2624	rBV2	618	931	0.12%	0.015%
50	9.837	2734	2736	2740	rVB2	478	248	0.03%	0.004%
51	9.950	2768	2771	2775	rBV	267	209	0.03%	0.003%
52	10.030	2793	2796	2799	rBV2	286	229	0.03%	0.004%
53	10.159	2824	2836	2853	rBV	272625	428233	56.39%	7.114%
54	10.718	3006	3010	3013	rBV	382	405	0.05%	0.007%
55	11.011	3098	3101	3108	rBV3	497	524	0.07%	0.009%
56	11.191	3145	3157	3178	rBV	378791	591014	77.83%	9.818%
57	11.332	3198	3201	3204	rBV2	555	454	0.06%	0.008%
58	11.567	3262	3274	3295	rBV	352156	544317	71.68%	9.042%




Sum of corrected areas: 6019993

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031612.D
Acq On : 29 Jun 2023 11:00
Operator : SY/MD
Sample : VV0629WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK363

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

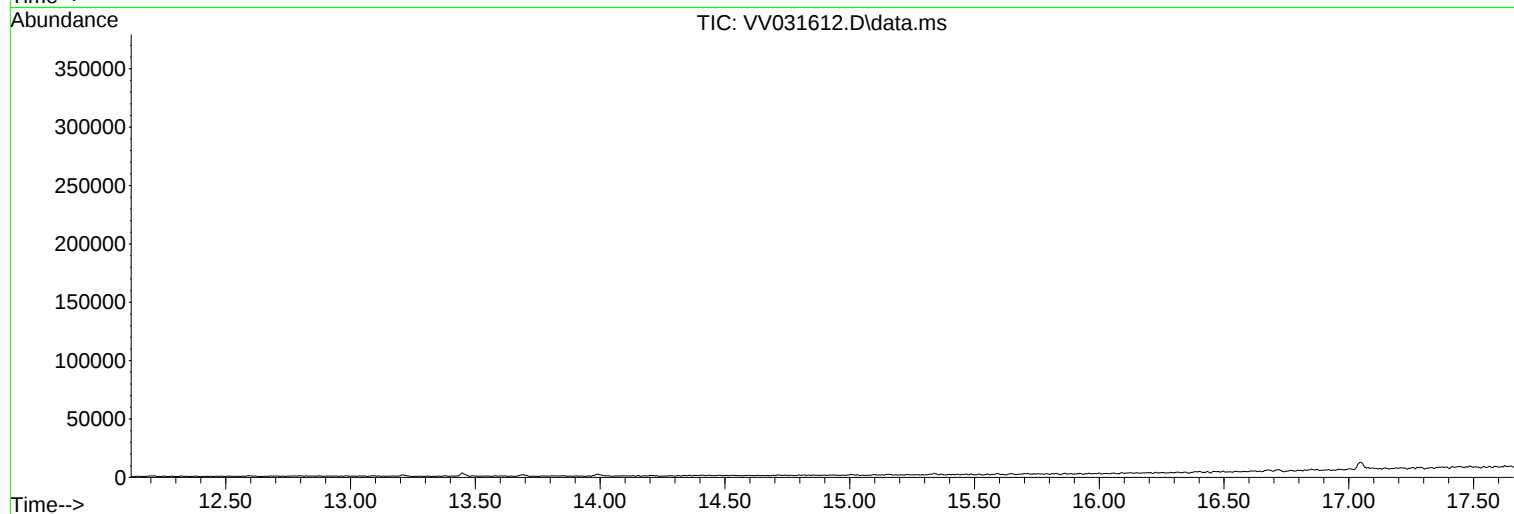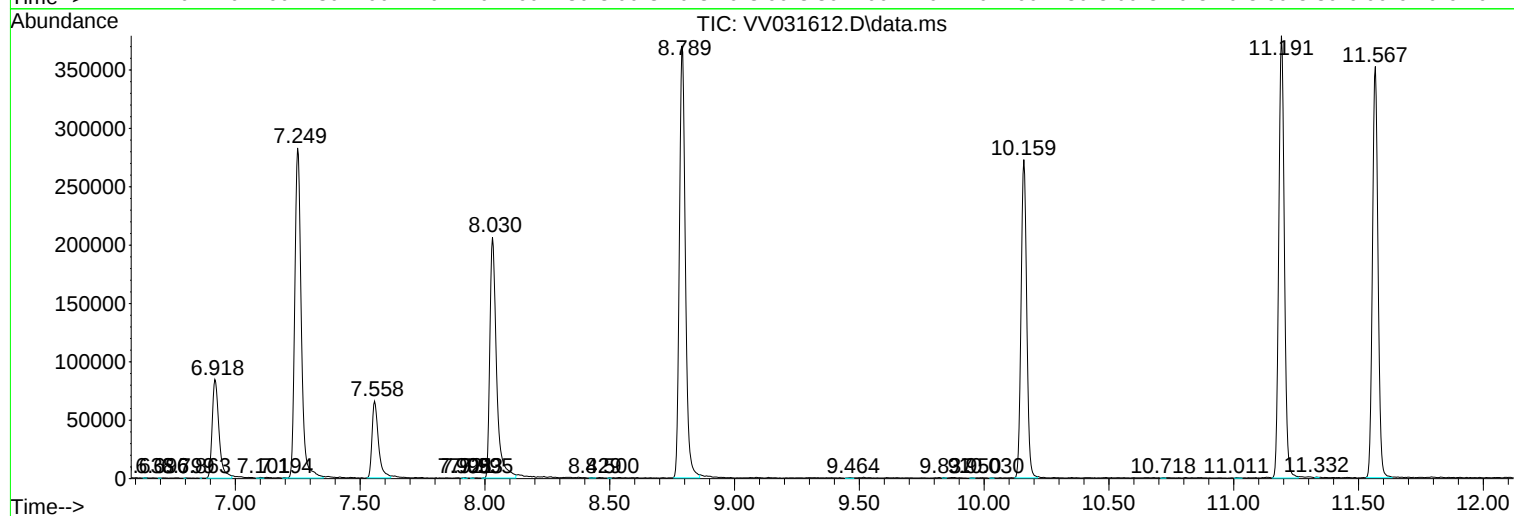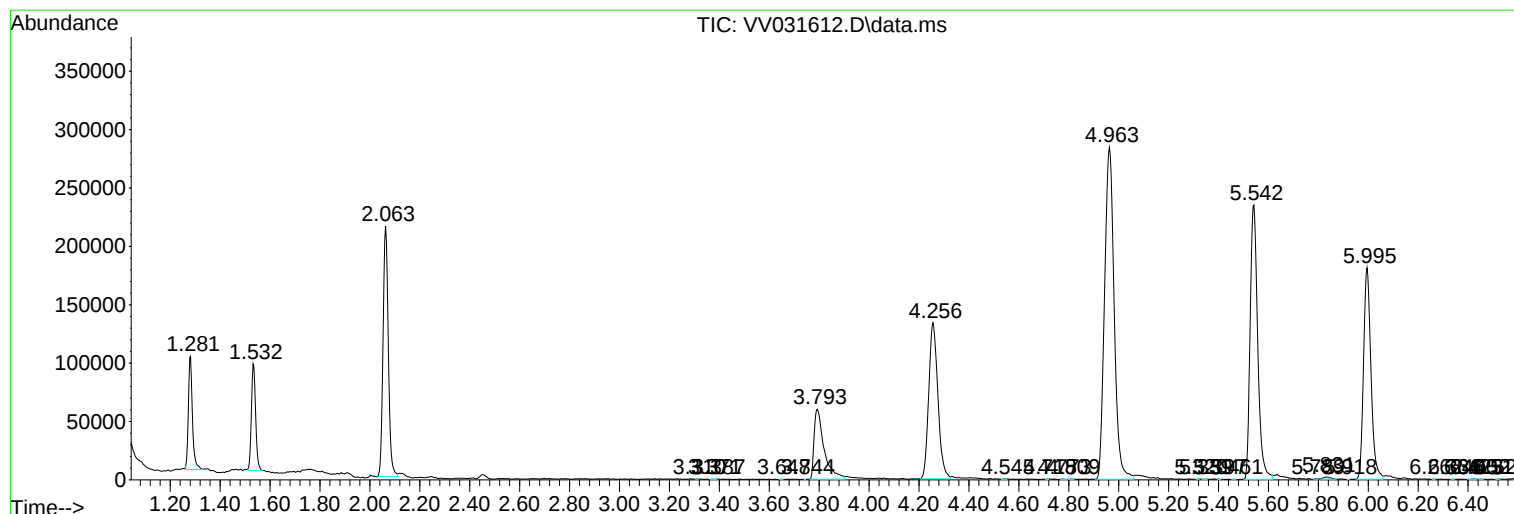

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031612.D
Acq On : 29 Jun 2023 11:00
Operator : SY/MD
Sample : VV0629WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK363

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031612.D
Acq On : 29 Jun 2023 11:00
Operator : SY/MD
Sample : VV0629WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK363

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------