

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031614.D
 Acq On : 29 Jun 2023 11:49
 Operator : SY/MD
 Sample : 03421-11ME
 Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46G7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	74592	97775	12.53%	1.542%
2	1.497	138	142	145	rBV	13992	14125	1.81%	0.223%
3	1.523	145	150	163	rVB	43057	53983	6.92%	0.852%
4	2.050	304	314	331	rVB	186041	271342	34.76%	4.280%
5	2.384	405	418	430	rBV	18667	37615	4.82%	0.593%
6	2.500	451	454	460	rBV4	366	330	0.04%	0.005%
7	2.561	462	473	481	rVV4	2170	4229	0.54%	0.067%
8	2.700	512	516	523	rVB4	1320	1456	0.19%	0.023%
9	2.886	569	574	583	rBV5	798	1168	0.15%	0.018%
10	2.918	583	584	590	rVV2	451	298	0.04%	0.005%
11	2.960	592	597	604	rBV4	459	523	0.07%	0.008%
12	3.002	604	610	614	rVB	308	360	0.05%	0.006%
13	3.040	620	622	627	rVB4	361	279	0.04%	0.004%
14	3.153	651	657	660	rVB4	422	417	0.05%	0.007%
15	3.278	692	696	699	rBV3	263	269	0.03%	0.004%
16	3.455	749	751	755	rVV2	404	287	0.04%	0.005%
17	3.497	759	764	766	rBV2	258	294	0.04%	0.005%
18	3.806	850	860	900	rBV	40899	149958	19.21%	2.365%
19	4.253	983	999	1025	rBV	120552	313031	40.11%	4.938%
20	4.429	1052	1054	1058	rVB3	409	268	0.03%	0.004%
21	4.494	1070	1074	1079	rVB3	302	317	0.04%	0.005%
22	4.539	1085	1088	1092	rBV3	356	362	0.05%	0.006%
23	4.635	1116	1118	1125	rVB2	327	310	0.04%	0.005%
24	4.732	1143	1148	1154	rVB3	486	529	0.07%	0.008%
25	4.960	1201	1219	1246	rBV2	272589	709444	90.89%	11.191%
26	5.433	1362	1366	1371	rBV	570	437	0.06%	0.007%
27	5.539	1385	1399	1422	rBV	264245	554163	71.00%	8.741%
28	5.744	1459	1463	1471	rVB3	448	579	0.07%	0.009%
29	5.799	1477	1480	1483	rVB3	438	318	0.04%	0.005%
30	5.831	1483	1490	1492	rBV5	1914	2441	0.31%	0.039%
31	5.896	1506	1510	1514	rBV	249	300	0.04%	0.005%
32	5.995	1526	1541	1564	rBV	164003	350479	44.90%	5.528%
33	6.117	1577	1579	1585	rVB2	497	419	0.05%	0.007%
34	6.179	1595	1598	1603	rVV2	502	300	0.04%	0.005%
35	6.204	1603	1606	1610	rVB3	348	257	0.03%	0.004%
36	6.436	1673	1678	1682	rBV3	511	524	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062923\
 Data File : VW031614.D
 Acq On : 29 Jun 2023 11:49
 Operator : SY/MD
 Sample : 03421-11ME
 Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46G7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.461	1682	1686	1687	rVV	436	290	0.04%	0.005%
38	6.535	1707	1709	1716	rBV2	375	332	0.04%	0.005%
39	6.597	1722	1728	1729	rBV2	347	289	0.04%	0.005%
40	6.918	1816	1828	1855	rBV	81030	160585	20.57%	2.533%
41	7.153	1898	1901	1902	rBV	584	309	0.04%	0.005%
42	7.204	1915	1917	1918	rBV2	625	310	0.04%	0.005%
43	7.249	1919	1931	1956	rBV	276232	503613	64.52%	7.944%
44	7.439	1988	1990	1995	rVB4	652	332	0.04%	0.005%
45	7.561	2017	2028	2050	rBV2	64559	128744	16.49%	2.031%
46	7.735	2080	2082	2086	rVB3	829	611	0.08%	0.010%
47	7.757	2086	2089	2094	rVB4	784	535	0.07%	0.008%
48	7.786	2095	2098	2100	rBV	488	308	0.04%	0.005%
49	8.050	2167	2180	2205	rBV2	142177	385037	49.33%	6.074%
50	8.378	2273	2282	2283	rBV6	1511	1794	0.23%	0.028%
51	8.413	2291	2293	2297	rVB2	637	358	0.05%	0.006%
52	8.715	2384	2387	2390	rVB3	600	369	0.05%	0.006%
53	8.735	2390	2393	2398	rVB4	463	294	0.04%	0.005%
54	8.793	2398	2411	2433	rBV	452965	780512	100.00%	12.312%
55	8.931	2452	2454	2457	rVB3	671	392	0.05%	0.006%
56	8.957	2458	2462	2463	rBV2	612	412	0.05%	0.006%
57	9.024	2479	2483	2486	rVB5	501	329	0.04%	0.005%
58	9.040	2486	2488	2493	rVB	455	314	0.04%	0.005%
59	9.230	2545	2547	2552	rVB3	614	440	0.06%	0.007%
60	9.490	2624	2628	2633	rBV4	704	619	0.08%	0.010%
61	9.574	2651	2654	2660	rVB3	425	382	0.05%	0.006%
62	9.741	2704	2706	2711	rBV2	378	291	0.04%	0.005%
63	9.841	2735	2737	2741	rBV2	396	306	0.04%	0.005%
64	9.989	2781	2783	2786	rBV3	543	316	0.04%	0.005%
65	10.162	2824	2837	2859	rBV	279790	468558	60.03%	7.391%
66	10.259	2865	2867	2873	rBV5	426	261	0.03%	0.004%
67	10.329	2883	2889	2891	rBV4	444	458	0.06%	0.007%
68	10.371	2898	2902	2904	rBV2	447	313	0.04%	0.005%
69	10.452	2921	2927	2931	rBV2	435	484	0.06%	0.008%
70	10.490	2931	2939	2944	rVB6	644	828	0.11%	0.013%
71	10.516	2944	2947	2951	rBV3	494	358	0.05%	0.006%
72	11.037	3107	3109	3113	rBV3	436	283	0.04%	0.004%
73	11.120	3131	3135	3136	rBV3	504	329	0.04%	0.005%
74	11.194	3146	3158	3180	rBV	479735	749219	95.99%	11.818%
75	11.381	3212	3216	3221	rBV3	467	419	0.05%	0.007%
76	11.567	3263	3274	3290	rBV	359868	570386	73.08%	8.997%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031614.D
 Acq On : 29 Jun 2023 11:49
 Operator : SY/MD
 Sample : 03421-11ME
 Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46G7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.661	3301	3303	3305	rBV2	552	370	0.05%	0.006%
78	11.828	3353	3355	3358	rVB3	885	418	0.05%	0.007%
79	12.024	3414	3416	3419	rVB2	553	381	0.05%	0.006%
80	12.130	3446	3449	3450	rBV3	431	268	0.03%	0.004%
81	12.172	3459	3462	3464	rBV2	476	369	0.05%	0.006%
82	12.747	3638	3641	3644	rVB3	749	428	0.05%	0.007%
83	12.789	3651	3654	3656	rBV2	441	266	0.03%	0.004%
84	12.876	3679	3681	3685	rVB	466	341	0.04%	0.005%
85	12.998	3717	3719	3722	rBV3	626	309	0.04%	0.005%
86	13.017	3722	3725	3727	rVB	441	278	0.04%	0.004%
87	13.268	3801	3803	3806	rBV	408	293	0.04%	0.005%
88	13.368	3831	3834	3835	rBV2	562	335	0.04%	0.005%
89	13.426	3849	3852	3855	rBV4	638	468	0.06%	0.007%
90	13.879	3990	3993	3995	rBV2	487	341	0.04%	0.005%
91	13.931	4006	4009	4011	rBV	644	410	0.05%	0.006%
92	14.088	4054	4058	4061	rBV3	683	484	0.06%	0.008%
93	14.124	4065	4069	4075	rBV5	748	593	0.08%	0.009%
94	14.156	4076	4079	4080	rBV2	507	282	0.04%	0.004%
95	14.326	4130	4132	4137	rVB2	640	528	0.07%	0.008%
96	14.644	4228	4231	4234	rBV3	815	524	0.07%	0.008%
97	14.667	4236	4238	4242	rVV5	652	430	0.06%	0.007%
98	14.966	4329	4331	4333	rBV2	768	389	0.05%	0.006%
99	15.333	4442	4445	4446	rBV3	1168	650	0.08%	0.010%
100	16.033	4661	4663	4668	rBV4	1209	961	0.12%	0.015%




Sum of corrected areas: 6339621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031614.D
Acq On : 29 Jun 2023 11:49
Operator : SY/MD
Sample : 03421-11ME
Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46G7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

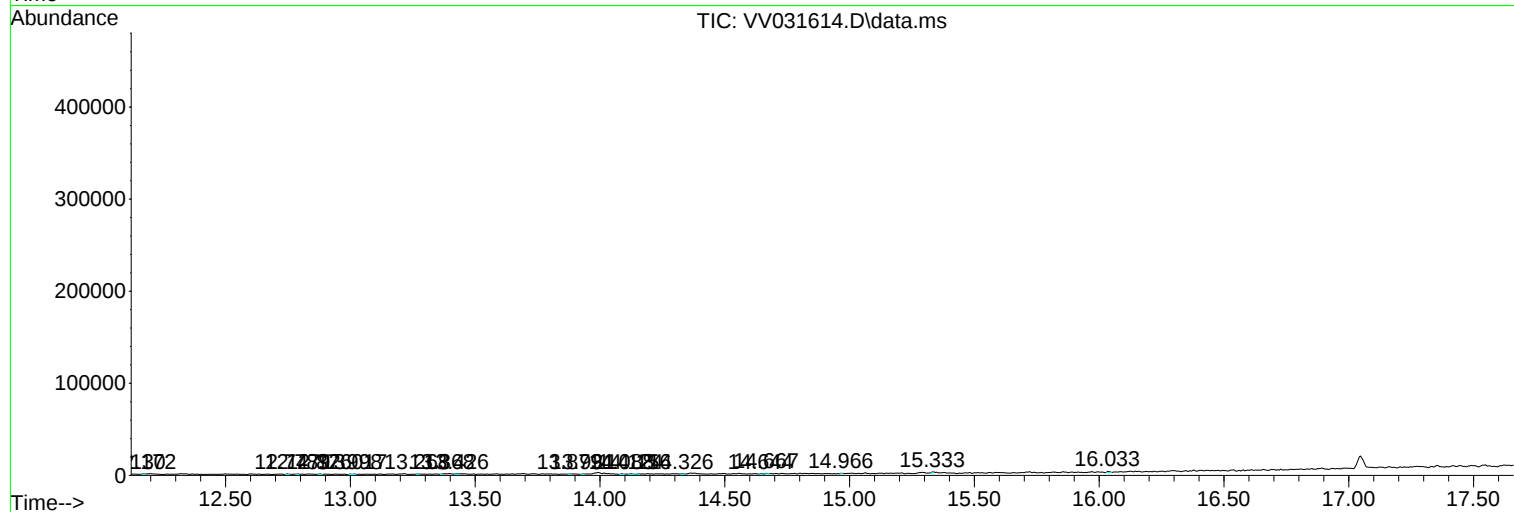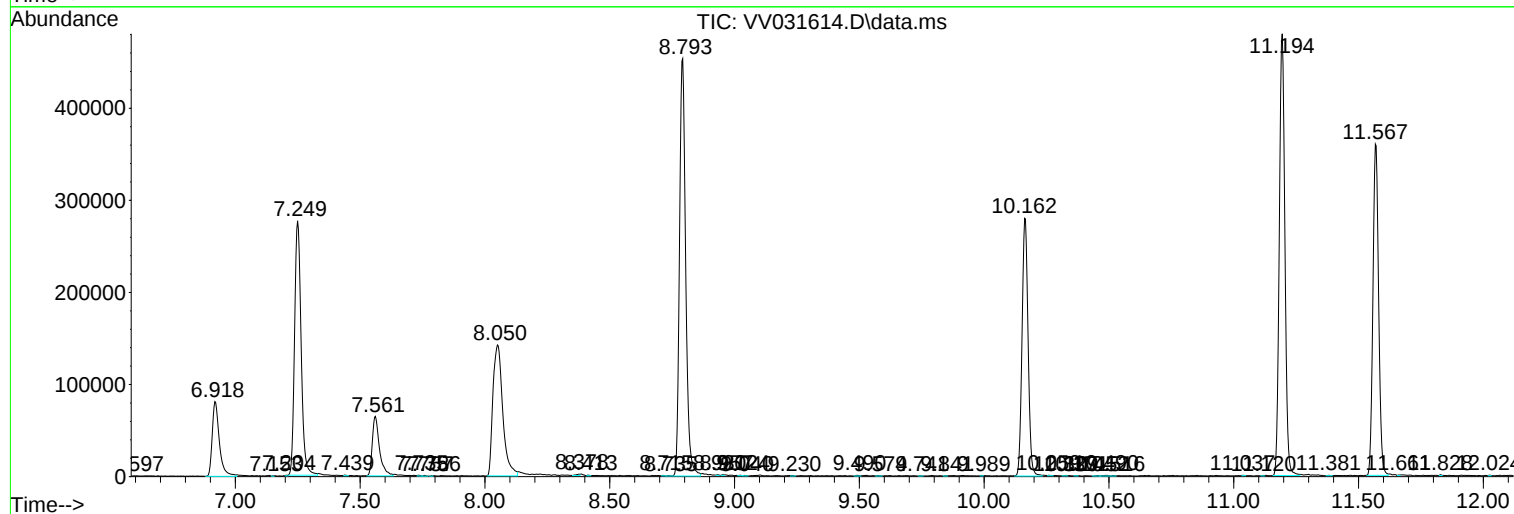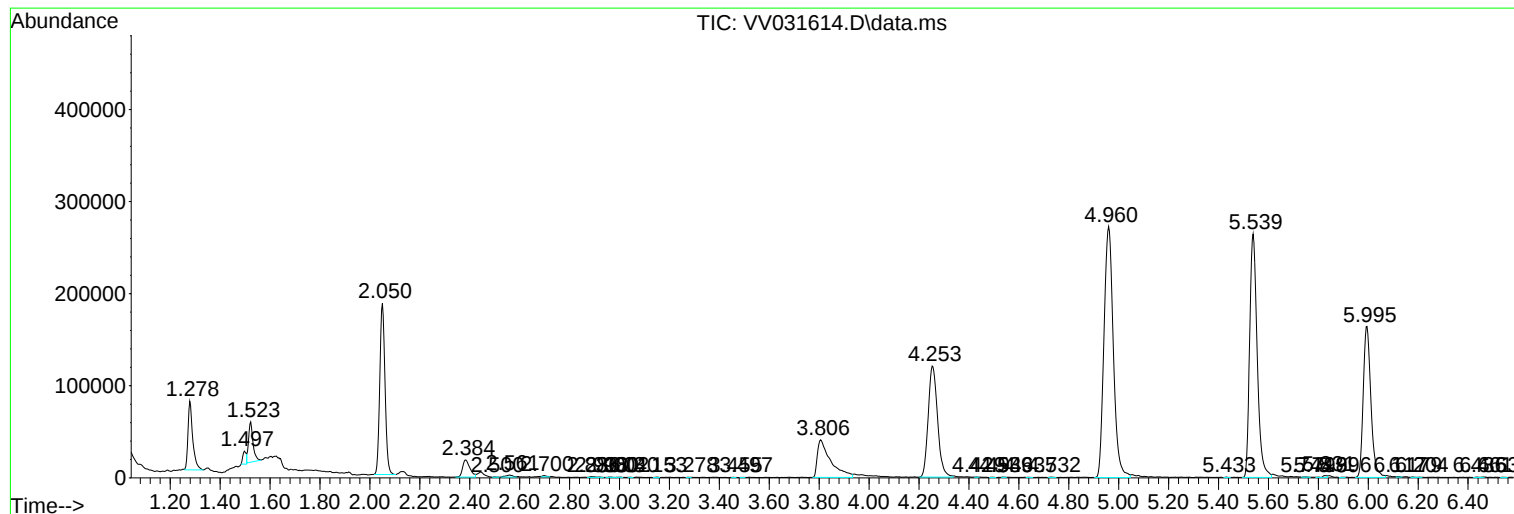

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031614.D
Acq On : 29 Jun 2023 11:49
Operator : SY/MD
Sample : 03421-11ME
Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46G7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031614.D
Acq On : 29 Jun 2023 11:49
Operator : SY/MD
Sample : 03421-11ME
Misc : 3.51g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46G7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------