

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031615.D
 Acq On : 29 Jun 2023 12:28
 Operator : SY/MD
 Sample : 03422-02ME
 Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46J1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	92	rVB	98155	128566	15.16%	1.903%
2	2.050	305	314	331	rVB	212677	302863	35.71%	4.482%
3	2.384	408	418	430	rBV	21593	42763	5.04%	0.633%
4	2.773	536	539	540	rBV	264	157	0.02%	0.002%
5	2.809	548	550	552	rBV2	473	201	0.02%	0.003%
6	2.957	592	596	600	rVB2	386	286	0.03%	0.004%
7	2.998	607	609	614	rVB2	278	207	0.02%	0.003%
8	3.146	653	655	657	rBV2	158	80	0.01%	0.001%
9	3.230	680	681	683	rVB	254	91	0.01%	0.001%
10	3.281	693	697	699	rBV2	397	312	0.04%	0.005%
11	3.330	710	712	717	rVB2	351	220	0.03%	0.003%
12	3.355	718	720	723	rBV2	327	182	0.02%	0.003%
13	3.436	742	745	747	rBV2	338	201	0.02%	0.003%
14	3.468	751	755	758	rBB2	291	192	0.02%	0.003%
15	3.487	758	761	764	rBV2	497	332	0.04%	0.005%
16	3.503	764	766	768	rBV2	186	54	0.01%	0.001%
17	3.571	784	787	794	rBV3	329	359	0.04%	0.005%
18	3.645	807	810	811	rBV	341	174	0.02%	0.003%
19	3.754	841	844	847	rBV2	373	313	0.04%	0.005%
20	3.802	849	859	898	rBV	45647	166635	19.65%	2.466%
21	4.249	981	998	1023	rBV	147502	378297	44.60%	5.599%
22	4.577	1097	1100	1103	rBV3	331	207	0.02%	0.003%
23	4.619	1110	1113	1117	rBV2	341	282	0.03%	0.004%
24	4.677	1129	1131	1134	rVB	349	165	0.02%	0.002%
25	4.693	1134	1136	1137	rVB	238	70	0.01%	0.001%
26	4.731	1145	1148	1150	rVB	277	110	0.01%	0.002%
27	4.751	1150	1154	1157	rVV2	333	223	0.03%	0.003%
28	4.767	1157	1159	1167	rVB2	542	478	0.06%	0.007%
29	4.831	1173	1179	1182	rBV	320	339	0.04%	0.005%
30	4.863	1186	1189	1192	rBV2	422	318	0.04%	0.005%
31	4.899	1198	1200	1201	rBV	357	143	0.02%	0.002%
32	4.957	1201	1218	1250	rVV2	323569	848221	100.00%	12.554%
33	5.272	1312	1316	1320	rVB2	589	475	0.06%	0.007%
34	5.291	1320	1322	1323	rBV2	314	139	0.02%	0.002%
35	5.323	1330	1332	1333	rBV2	282	143	0.02%	0.002%
36	5.436	1365	1367	1368	rBV2	367	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062923\
 Data File : VW031615.D
 Acq On : 29 Jun 2023 12:28
 Operator : SY/MD
 Sample : 03422-02ME
 Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46J1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.465	1374	1376	1378	rBV	352	184	0.02%	0.003%
38	5.490	1381	1384	1385	rBV2	382	243	0.03%	0.004%
39	5.535	1385	1398	1425	rBV	298357	624728	73.65%	9.246%
40	5.831	1481	1490	1501	rBV	2180	5157	0.61%	0.076%
41	5.992	1527	1540	1568	rBV	201091	422042	49.76%	6.246%
42	6.342	1648	1649	1651	rVB2	366	116	0.01%	0.002%
43	6.387	1662	1663	1664	rBV	85	24	0.00%	0.000%
44	6.397	1664	1666	1668	rVV	169	75	0.01%	0.001%
45	6.410	1668	1670	1671	rVV	152	52	0.01%	0.001%
46	6.432	1675	1677	1678	rBV	169	60	0.01%	0.001%
47	6.455	1682	1684	1685	rBV	262	86	0.01%	0.001%
48	6.519	1702	1704	1707	rVB	212	116	0.01%	0.002%
49	6.548	1711	1713	1717	rVB3	419	250	0.03%	0.004%
50	6.571	1717	1720	1721	rBV2	307	190	0.02%	0.003%
51	6.677	1752	1753	1756	rVB2	356	165	0.02%	0.002%
52	6.696	1756	1759	1761	rBV	387	241	0.03%	0.004%
53	6.728	1765	1769	1771	rBV2	347	311	0.04%	0.005%
54	6.770	1778	1782	1787	rBV2	461	478	0.06%	0.007%
55	6.796	1787	1790	1794	rBV2	469	280	0.03%	0.004%
56	6.844	1803	1805	1809	rBV	273	190	0.02%	0.003%
57	6.879	1814	1816	1817	rBV2	390	163	0.02%	0.002%
58	6.918	1817	1828	1848	rBV	94491	180102	21.23%	2.666%
59	7.185	1908	1911	1913	rVB2	613	334	0.04%	0.005%
60	7.246	1919	1930	1952	rBV	312265	552826	65.17%	8.182%
61	7.558	2017	2027	2056	rBV	68380	131808	15.54%	1.951%
62	7.744	2083	2085	2090	rVB2	478	236	0.03%	0.003%
63	7.863	2120	2122	2127	rBV4	407	310	0.04%	0.005%
64	7.918	2137	2139	2141	rBV	436	226	0.03%	0.003%
65	7.972	2154	2156	2158	rVB2	404	167	0.02%	0.002%
66	7.985	2158	2160	2166	rVB2	422	310	0.04%	0.005%
67	8.050	2166	2180	2207	rBV	136705	369764	43.59%	5.473%
68	8.548	2334	2335	2336	rBV	331	114	0.01%	0.002%
69	8.593	2347	2349	2351	rVB2	418	193	0.02%	0.003%
70	8.609	2351	2354	2355	rBV2	271	115	0.01%	0.002%
71	8.644	2362	2365	2368	rBV2	458	287	0.03%	0.004%
72	8.741	2393	2395	2397	rBV	270	175	0.02%	0.003%
73	8.789	2398	2410	2432	rBV	462465	773251	91.16%	11.444%
74	9.011	2477	2479	2480	rBV2	535	219	0.03%	0.003%
75	9.059	2491	2494	2500	rVB3	753	594	0.07%	0.009%
76	9.088	2500	2503	2504	rBV	585	297	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031615.D
 Acq On : 29 Jun 2023 12:28
 Operator : SY/MD
 Sample : 03422-02ME
 Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A46J1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

77	9.162	2520	2526	2528	rVB3	405	392	0.05%	0.006%
78	9.175	2528	2530	2532	rBV	397	217	0.03%	0.003%
79	9.963	2773	2775	2777	rBV2	440	217	0.03%	0.003%
80	10.162	2825	2837	2853	rBV	282749	463228	54.61%	6.856%
81	10.268	2868	2870	2874	rBV4	724	386	0.05%	0.006%
82	10.461	2928	2930	2932	rBV	541	273	0.03%	0.004%
83	10.686	2997	3000	3003	rBV3	321	234	0.03%	0.003%
84	10.705	3003	3006	3009	rVV3	364	311	0.04%	0.005%
85	10.815	3038	3040	3043	rBV	408	225	0.03%	0.003%
86	10.908	3067	3069	3072	rBV	362	236	0.03%	0.003%
87	11.014	3099	3102	3105	rBV3	378	295	0.03%	0.004%
88	11.130	3135	3138	3146	rVB4	611	810	0.10%	0.012%
89	11.194	3146	3158	3178	rBV	486874	755840	89.11%	11.187%
90	11.493	3248	3251	3257	rBV4	667	649	0.08%	0.010%
91	11.567	3263	3274	3290	rBV	373374	592925	69.90%	8.775%




Sum of corrected areas: 6756660

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031615.D
Acq On : 29 Jun 2023 12:28
Operator : SY/MD
Sample : 03422-02ME
Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46J1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

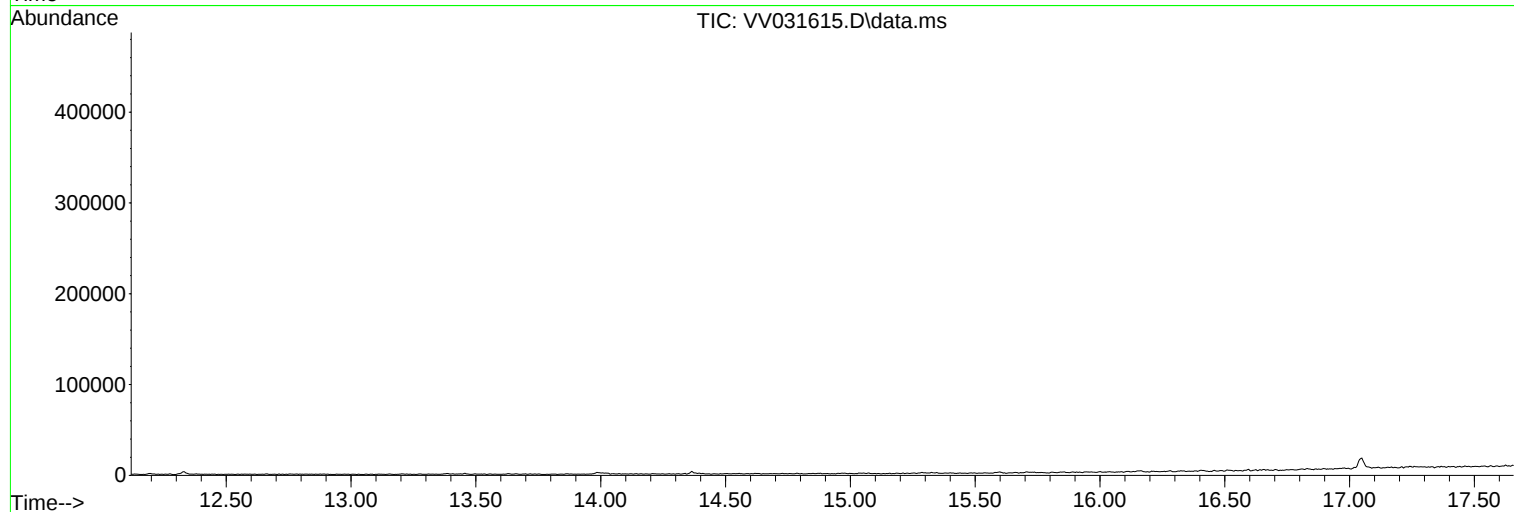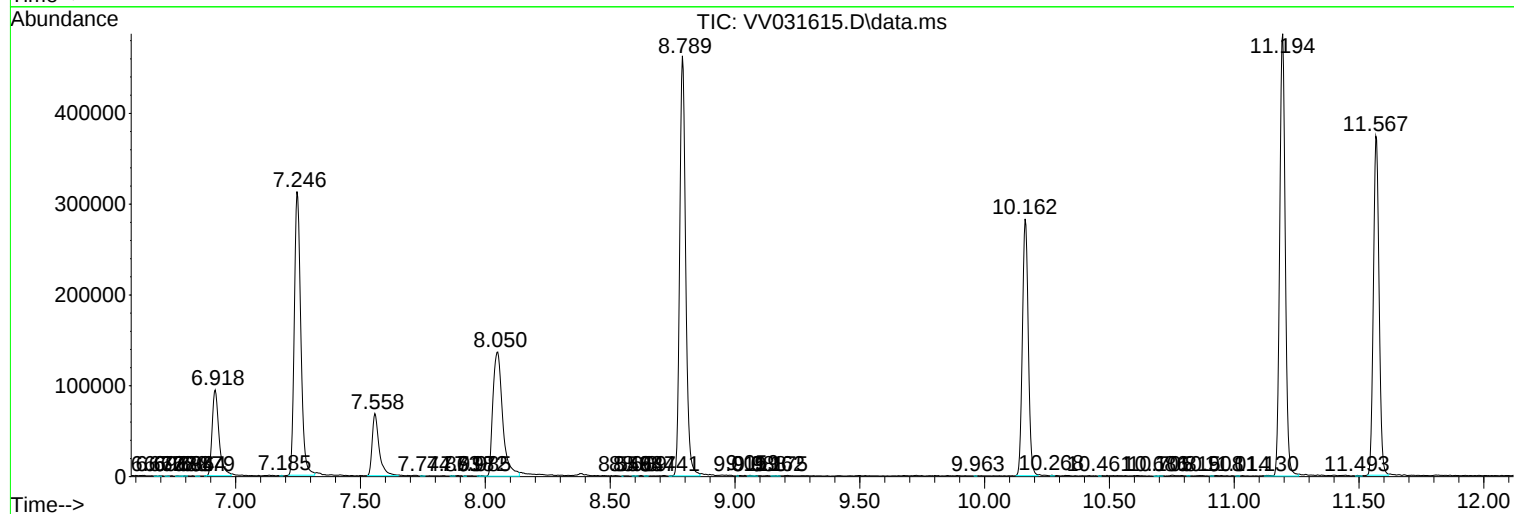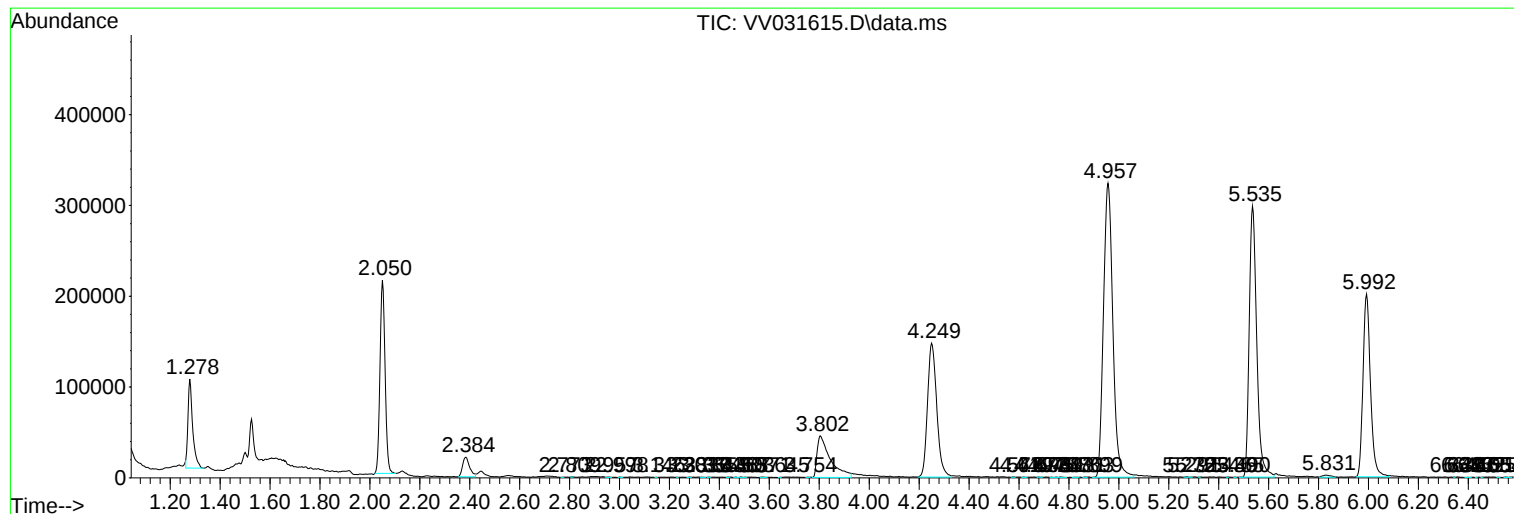

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031615.D
Acq On : 29 Jun 2023 12:28
Operator : SY/MD
Sample : 03422-02ME
Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46J1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031615.D
Acq On : 29 Jun 2023 12:28
Operator : SY/MD
Sample : 03422-02ME
Misc : 4.20g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A46J1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------