

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031616.D
 Acq On : 29 Jun 2023 12:51
 Operator : SY/MD
 Sample : 03420-06ME
 Misc : 5.17g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4645ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	91	rVB	86104	116070	14.57%	1.751%
2	2.047	304	313	329	rBV	195987	283371	35.58%	4.275%
3	2.378	408	416	432	rBV	52902	92460	11.61%	1.395%
4	2.773	535	539	541	rBV4	336	314	0.04%	0.005%
5	2.802	545	548	551	rBV2	325	303	0.04%	0.005%
6	2.831	555	557	558	rBV2	373	164	0.02%	0.002%
7	2.944	589	592	596	rBV2	371	320	0.04%	0.005%
8	2.966	596	599	600	rVV2	306	144	0.02%	0.002%
9	3.072	630	632	635	rVB2	300	137	0.02%	0.002%
10	3.105	640	642	643	rBV	315	118	0.01%	0.002%
11	3.159	657	659	663	rVB	299	133	0.02%	0.002%
12	3.185	665	667	670	rVB	520	189	0.02%	0.003%
13	3.246	682	686	689	rBV	354	377	0.05%	0.006%
14	3.320	707	709	713	rVB3	341	202	0.03%	0.003%
15	3.352	713	719	721	rBV2	448	494	0.06%	0.007%
16	3.365	721	723	724	rVV	477	198	0.02%	0.003%
17	3.384	727	729	733	rBV	395	321	0.04%	0.005%
18	3.416	738	739	742	rVV	336	139	0.02%	0.002%
19	3.433	742	744	747	rVB2	472	286	0.04%	0.004%
20	3.452	747	750	752	rBV	373	245	0.03%	0.004%
21	3.545	776	779	780	rBV	476	259	0.03%	0.004%
22	3.584	788	791	797	rVB2	505	385	0.05%	0.006%
23	3.638	806	808	811	rBV2	182	105	0.01%	0.002%
24	3.658	811	814	818	rVB2	363	235	0.03%	0.004%
25	3.680	818	821	824	rBV3	295	143	0.02%	0.002%
26	3.703	825	828	831	rVB2	358	203	0.03%	0.003%
27	3.719	831	833	837	rBV	363	259	0.03%	0.004%
28	3.764	846	847	849	rBV	277	115	0.01%	0.002%
29	3.802	849	859	889	rBV2	48606	162795	20.44%	2.456%
30	4.252	981	999	1026	rBV	135254	355497	44.63%	5.363%
31	4.555	1088	1093	1095	rBV3	437	316	0.04%	0.005%
32	4.571	1095	1098	1100	rBV2	402	251	0.03%	0.004%
33	4.828	1176	1178	1179	rBV2	349	154	0.02%	0.002%
34	4.960	1200	1219	1249	rBV2	302280	796474	100.00%	12.015%
35	5.127	1269	1271	1274	rVB2	678	310	0.04%	0.005%
36	5.214	1294	1298	1303	rBV2	607	559	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031616.D
 Acq On : 29 Jun 2023 12:51
 Operator : SY/MD
 Sample : 03420-06ME
 Misc : 5.17g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4645ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.352	1338	1341	1342	rBV2	354	166	0.02%	0.003%
38	5.378	1347	1349	1351	rBV2	327	151	0.02%	0.002%
39	5.410	1357	1359	1361	rBV3	790	381	0.05%	0.006%
40	5.461	1373	1375	1376	rBV3	239	105	0.01%	0.002%
41	5.477	1377	1380	1385	rVB5	636	380	0.05%	0.006%
42	5.539	1385	1399	1427	rBV	283048	604976	75.96%	9.126%
43	5.947	1523	1526	1527	rBV	450	289	0.04%	0.004%
44	5.992	1527	1540	1563	rVV	186285	395128	49.61%	5.961%
45	6.194	1600	1603	1607	rBV5	645	468	0.06%	0.007%
46	6.233	1613	1615	1620	rBV4	575	355	0.04%	0.005%
47	6.275	1626	1628	1630	rBV4	443	206	0.03%	0.003%
48	6.310	1637	1639	1641	rBV4	316	205	0.03%	0.003%
49	6.333	1644	1646	1649	rVV	386	241	0.03%	0.004%
50	6.358	1653	1654	1657	rVV	371	155	0.02%	0.002%
51	6.420	1670	1673	1680	rBV3	382	297	0.04%	0.004%
52	6.490	1693	1695	1699	rVB2	409	235	0.03%	0.004%
53	6.510	1699	1701	1709	rBV3	399	360	0.05%	0.005%
54	6.580	1720	1723	1725	rBV2	651	410	0.05%	0.006%
55	6.635	1739	1740	1744	rVB2	516	263	0.03%	0.004%
56	6.712	1762	1764	1772	rVB3	418	359	0.05%	0.005%
57	6.754	1774	1777	1783	rVB3	367	314	0.04%	0.005%
58	6.821	1796	1798	1801	rVB2	460	190	0.02%	0.003%
59	6.847	1804	1806	1808	rBV3	310	201	0.03%	0.003%
60	6.918	1817	1828	1852	rBV	84382	168721	21.18%	2.545%
61	7.085	1878	1880	1883	rBV2	447	308	0.04%	0.005%
62	7.249	1920	1931	1950	rBV	287158	511495	64.22%	7.716%
63	7.522	2014	2016	2018	rBV2	566	284	0.04%	0.004%
64	7.558	2018	2027	2049	rVV	64635	125061	15.70%	1.887%
65	7.731	2079	2081	2086	rVB3	527	390	0.05%	0.006%
66	7.805	2102	2104	2109	rVB2	370	166	0.02%	0.003%
67	7.831	2110	2112	2119	rBV3	416	341	0.04%	0.005%
68	7.866	2120	2123	2124	rBV2	705	334	0.04%	0.005%
69	8.043	2166	2178	2208	rBV	170406	396874	49.83%	5.987%
70	8.378	2277	2282	2285	rBV4	1426	1530	0.19%	0.023%
71	8.432	2298	2299	2300	rBV	322	105	0.01%	0.002%
72	8.513	2322	2324	2328	rBV4	357	225	0.03%	0.003%
73	8.635	2360	2362	2364	rVB4	662	181	0.02%	0.003%
74	8.792	2399	2411	2432	rBV	442748	749893	94.15%	11.313%
75	9.046	2488	2490	2491	rBV	315	145	0.02%	0.002%
76	9.191	2533	2535	2536	rBV2	368	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031616.D
 Acq On : 29 Jun 2023 12:51
 Operator : SY/MD
 Sample : 03420-06ME
 Misc : 5.17g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4645ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.323	2572	2576	2577	rBV2	391	289	0.04%	0.004%
78	9.468	2619	2621	2624	rBV2	384	174	0.02%	0.003%
79	9.484	2624	2626	2629	rBV	312	194	0.02%	0.003%
80	9.516	2633	2636	2639	rVB2	424	272	0.03%	0.004%
81	9.535	2639	2642	2643	rBV2	423	243	0.03%	0.004%
82	9.657	2677	2680	2682	rBV	424	264	0.03%	0.004%
83	9.693	2688	2691	2696	rBV2	613	551	0.07%	0.008%
84	9.738	2701	2705	2707	rBV	354	298	0.04%	0.004%
85	9.796	2718	2723	2727	rBV5	596	554	0.07%	0.008%
86	9.866	2743	2745	2747	rBV	261	134	0.02%	0.002%
87	10.162	2825	2837	2857	rBV	301183	483951	60.76%	7.301%
88	10.490	2934	2939	2941	rBV4	738	709	0.09%	0.011%
89	10.593	2969	2971	2972	rBV	287	112	0.01%	0.002%
90	10.841	3046	3048	3051	rVB	434	200	0.03%	0.003%
91	10.863	3053	3055	3059	rVV2	522	346	0.04%	0.005%
92	10.947	3079	3081	3084	rBV	353	212	0.03%	0.003%
93	11.024	3102	3105	3107	rBV3	559	325	0.04%	0.005%
94	11.120	3132	3135	3136	rBV	669	358	0.04%	0.005%
95	11.191	3146	3157	3182	rBV	485664	764388	95.97%	11.531%
96	11.567	3262	3274	3291	rBV	379794	589685	74.04%	8.896%
97	12.323	3503	3509	3520	rBV6	4677	7108	0.89%	0.107%
98	12.384	3526	3528	3533	rVB4	805	520	0.07%	0.008%
99	13.985	4020	4026	4027	rBV3	1721	1576	0.20%	0.024%
100	14.660	4234	4236	4237	rBV	654	254	0.03%	0.004%




Sum of corrected areas: 6628829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031616.D
Acq On : 29 Jun 2023 12:51
Operator : SY/MD
Sample : 03420-06ME
Misc : 5.17g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4645ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

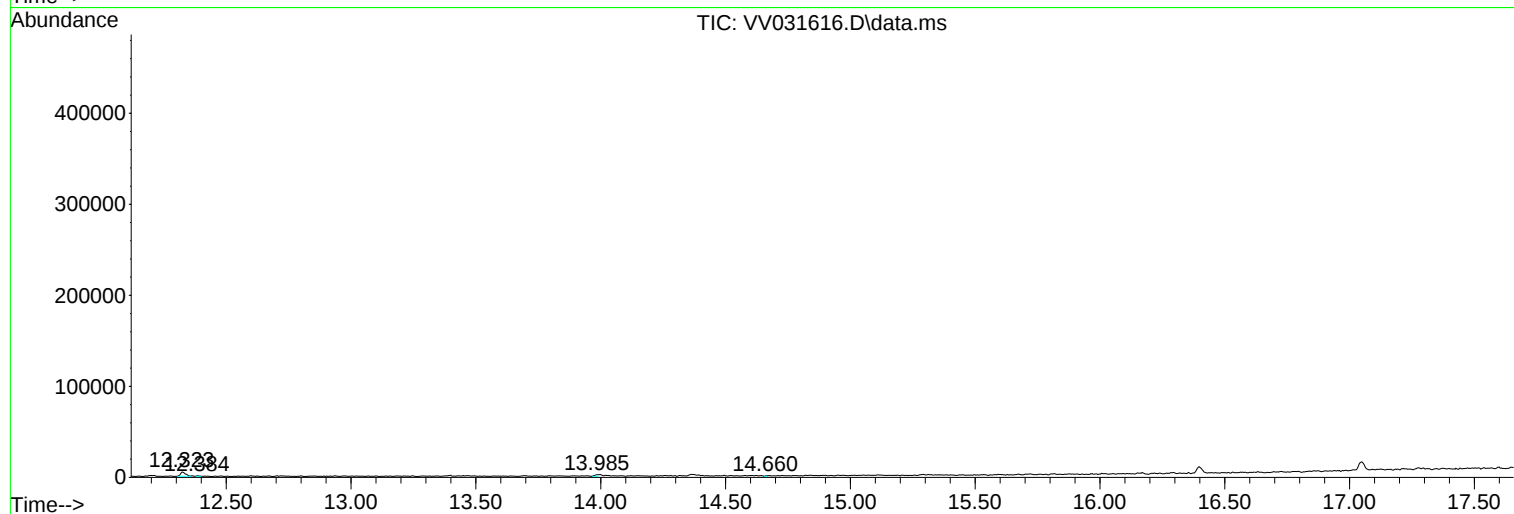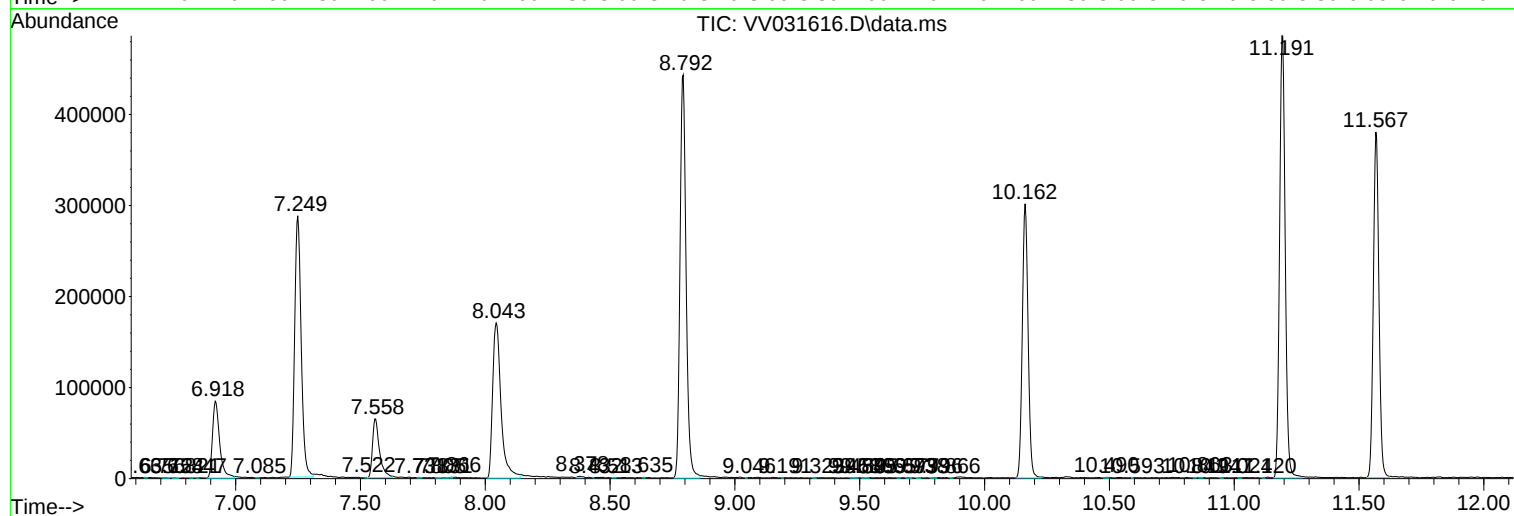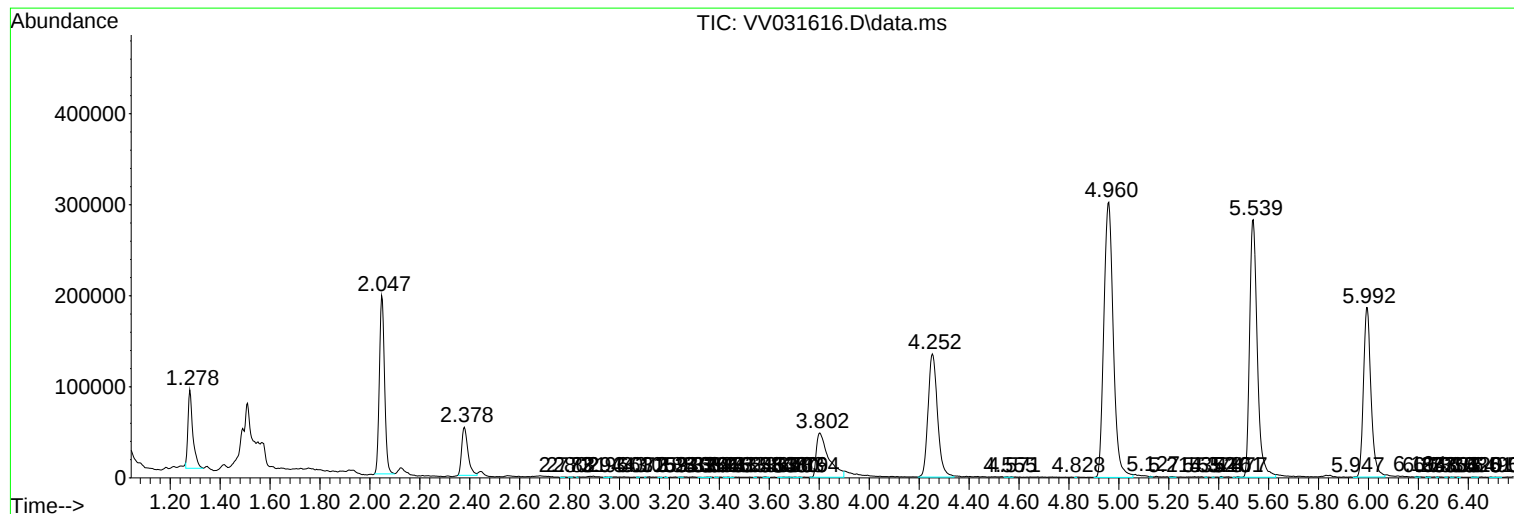

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031616.D
Acq On : 29 Jun 2023 12:51
Operator : SY/MD
Sample : 03420-06ME
Misc : 5.17g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4645ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031616.D
Acq On : 29 Jun 2023 12:51
Operator : SY/MD
Sample : 03420-06ME
Misc : 5.17g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4645ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc