

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031625.D
 Acq On : 29 Jun 2023 16:57
 Operator : SY/MD
 Sample : VIBLK219
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	86482	97171	11.89%	1.519%
2	1.532	148	153	166	rVB	92540	108852	13.32%	1.702%
3	2.063	309	318	331	rBV	163726	234480	28.68%	3.665%
4	2.452	430	439	452	rVB2	11942	20414	2.50%	0.319%
5	2.545	465	468	469	rBV2	437	229	0.03%	0.004%
6	2.696	511	515	516	rBV4	1087	753	0.09%	0.012%
7	2.931	586	588	589	rBV2	230	76	0.01%	0.001%
8	2.992	604	607	612	rVB2	598	416	0.05%	0.007%
9	3.217	671	677	680	rBV2	421	517	0.06%	0.008%
10	3.249	685	687	691	rBV3	270	189	0.02%	0.003%
11	3.317	706	708	712	rBV3	305	221	0.03%	0.003%
12	3.339	712	715	719	rVB3	325	197	0.02%	0.003%
13	3.465	753	754	755	rVB3	98	19	0.00%	0.000%
14	3.478	755	758	760	rBV2	345	183	0.02%	0.003%
15	3.500	761	765	767	rVV2	382	274	0.03%	0.004%
16	3.606	786	798	799	rBV3	600	799	0.10%	0.012%
17	3.667	813	817	821	rVB3	254	197	0.02%	0.003%
18	3.793	847	856	882	rBV	80212	222952	27.27%	3.485%
19	4.259	983	1001	1029	rBV	140995	357419	43.72%	5.587%
20	4.744	1149	1152	1159	rVB3	844	612	0.07%	0.010%
21	4.776	1159	1162	1168	rBV3	534	442	0.05%	0.007%
22	4.809	1169	1172	1174	rBV3	294	174	0.02%	0.003%
23	4.963	1203	1220	1245	rBV2	305212	817500	100.00%	12.779%
24	5.542	1387	1400	1421	rBV	244257	502950	61.52%	7.862%
25	5.838	1482	1492	1505	rBV10	3858	8046	0.98%	0.126%
26	5.899	1509	1511	1514	rBV3	396	206	0.03%	0.003%
27	5.995	1527	1541	1562	rBV	193252	408599	49.98%	6.387%
28	6.397	1662	1666	1674	rBV2	295	489	0.06%	0.008%
29	6.429	1674	1676	1680	rBV3	331	268	0.03%	0.004%
30	6.448	1680	1682	1683	rBV	339	111	0.01%	0.002%
31	6.558	1713	1716	1718	rBV2	417	294	0.04%	0.005%
32	6.574	1718	1721	1723	rVV	646	437	0.05%	0.007%
33	6.625	1732	1737	1740	rVB3	701	569	0.07%	0.009%
34	6.645	1740	1743	1745	rBV2	630	334	0.04%	0.005%
35	6.657	1745	1747	1750	rVB	498	151	0.02%	0.002%
36	6.674	1750	1752	1753	rBV2	316	130	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
 Data File : VV031625.D
 Acq On : 29 Jun 2023 16:57
 Operator : SY/MD
 Sample : VIBLK219
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.696	1758	1759	1760	rBV	243	58	0.01%	0.001%
38	6.754	1774	1777	1779	rBV2	260	177	0.02%	0.003%
39	6.767	1779	1781	1784	rVB	252	100	0.01%	0.002%
40	6.786	1784	1787	1790	rBV2	294	207	0.03%	0.003%
41	6.805	1790	1793	1794	rBV2	321	149	0.02%	0.002%
42	6.918	1817	1828	1852	rBV	92216	176554	21.60%	2.760%
43	7.249	1920	1931	1964	rBV	280406	507905	62.13%	7.939%
44	7.558	2017	2027	2049	rBV	70537	131240	16.05%	2.051%
45	7.744	2081	2085	2089	rBV5	581	643	0.08%	0.010%
46	7.809	2103	2105	2107	rBB	222	65	0.01%	0.001%
47	7.915	2135	2138	2145	rVB4	1391	1218	0.15%	0.019%
48	8.030	2164	2174	2203	rBV	255377	464712	56.85%	7.264%
49	8.365	2271	2278	2285	rBV5	3048	5364	0.66%	0.084%
50	8.503	2320	2321	2324	rVB	554	170	0.02%	0.003%
51	8.522	2324	2327	2331	rBV4	556	557	0.07%	0.009%
52	8.561	2338	2339	2341	rBV2	258	96	0.01%	0.002%
53	8.677	2372	2375	2376	rBV2	513	285	0.03%	0.004%
54	8.792	2398	2411	2434	rBV	372855	627075	76.71%	9.802%
55	9.030	2483	2485	2489	rBV4	426	217	0.03%	0.003%
56	9.140	2516	2519	2521	rBV2	426	309	0.04%	0.005%
57	9.255	2551	2555	2557	rBV3	634	482	0.06%	0.008%
58	9.284	2562	2564	2565	rBV	304	88	0.01%	0.001%
59	9.384	2593	2595	2598	rBV2	267	139	0.02%	0.002%
60	9.445	2612	2614	2619	rBV3	349	234	0.03%	0.004%
61	9.493	2623	2629	2633	rBV6	1185	1735	0.21%	0.027%
62	9.792	2719	2722	2725	rBV3	444	325	0.04%	0.005%
63	10.014	2789	2791	2792	rBV	297	134	0.02%	0.002%
64	10.159	2823	2836	2858	rBV	311788	500105	61.17%	7.817%
65	10.487	2933	2938	2944	rVB6	1673	1856	0.23%	0.029%
66	10.615	2976	2978	2980	rBV	345	194	0.02%	0.003%
67	10.734	3011	3015	3016	rBV3	563	384	0.05%	0.006%
68	11.133	3132	3139	3146	rVB6	2659	3740	0.46%	0.058%
69	11.191	3146	3157	3176	rBV	369644	578963	70.82%	9.050%
70	11.567	3262	3274	3296	rBV	340029	542902	66.41%	8.486%
71	12.377	3519	3526	3534	rBV7	1613	2290	0.28%	0.036%
72	12.590	3585	3592	3601	rBV4	4311	6234	0.76%	0.097%
73	12.795	3654	3656	3659	rVB3	758	363	0.04%	0.006%
74	13.207	3778	3784	3798	rVB5	6919	11229	1.37%	0.176%
75	13.448	3852	3859	3871	rVB2	16672	26669	3.26%	0.417%
76	13.689	3927	3934	3945	rVB5	9812	14784	1.81%	0.231%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031625.D
Acq On : 29 Jun 2023 16:57
Operator : SY/MD
Sample : VIBLK219
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK219

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis

77	13.972	4019	4022	4023	rBV2	1010	658	0.08%	0.010%
----	--------	------	------	------	------	------	-----	-------	--------




Sum of corrected areas: 6397279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031625.D
Acq On : 29 Jun 2023 16:57
Operator : SY/MD
Sample : VIBLK219
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

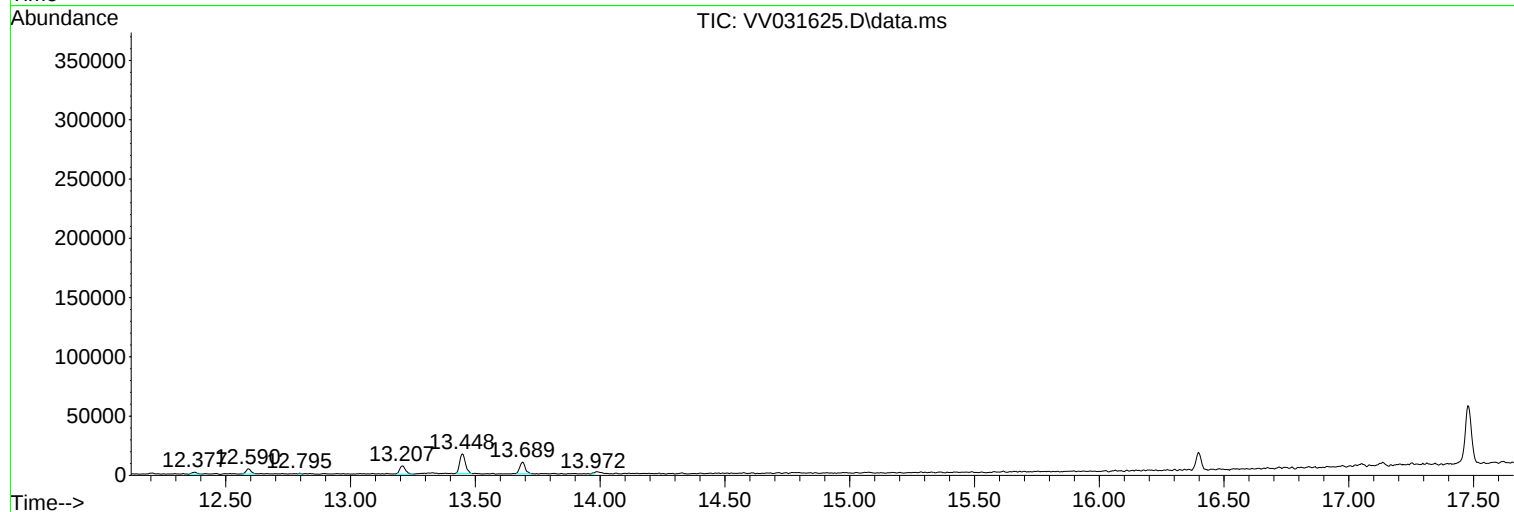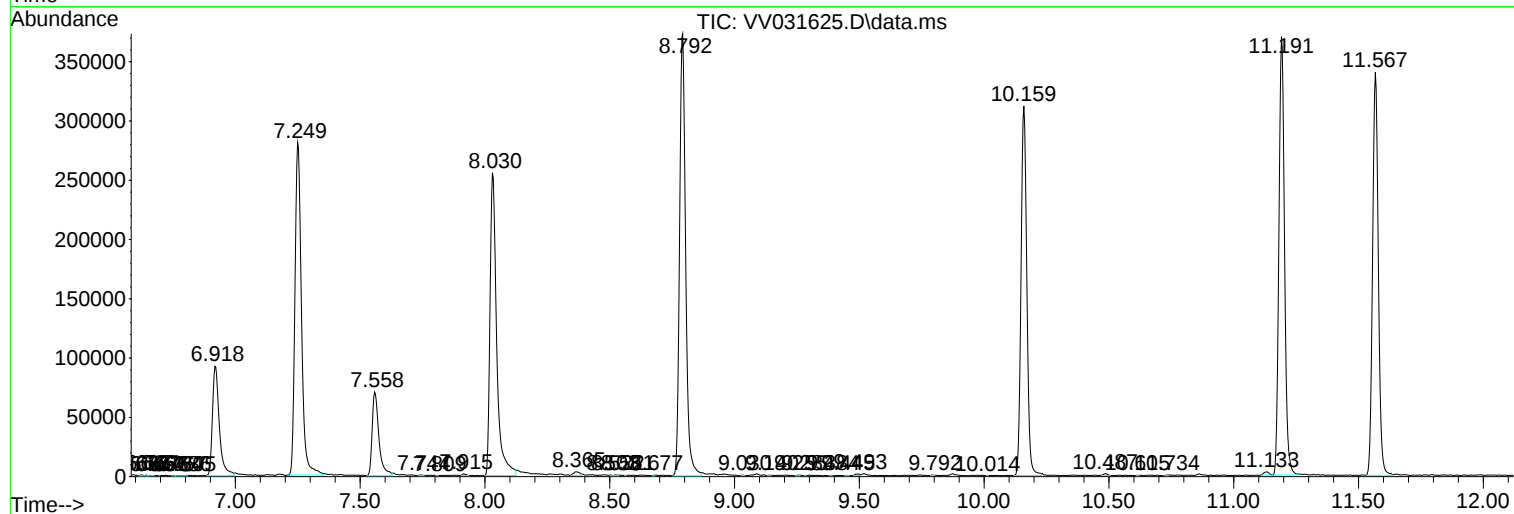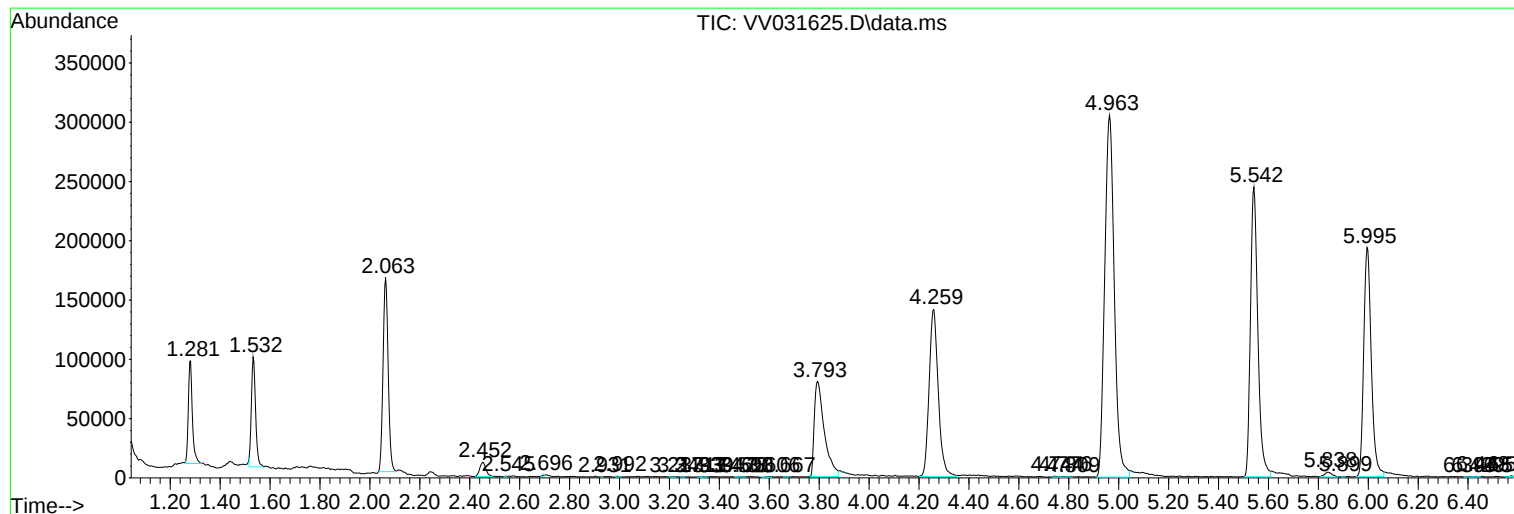

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031625.D
Acq On : 29 Jun 2023 16:57
Operator : SY/MD
Sample : VIBLK219
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031625.D
Acq On : 29 Jun 2023 16:57
Operator : SY/MD
Sample : VIBLK219
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------