


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062923\
Data File : VV031609.D
Acq On : 29 Jun 2023 09:42
Operator : SY/MD
Sample : BFB392
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB392

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Fri Jun 30 04:25:13 2023

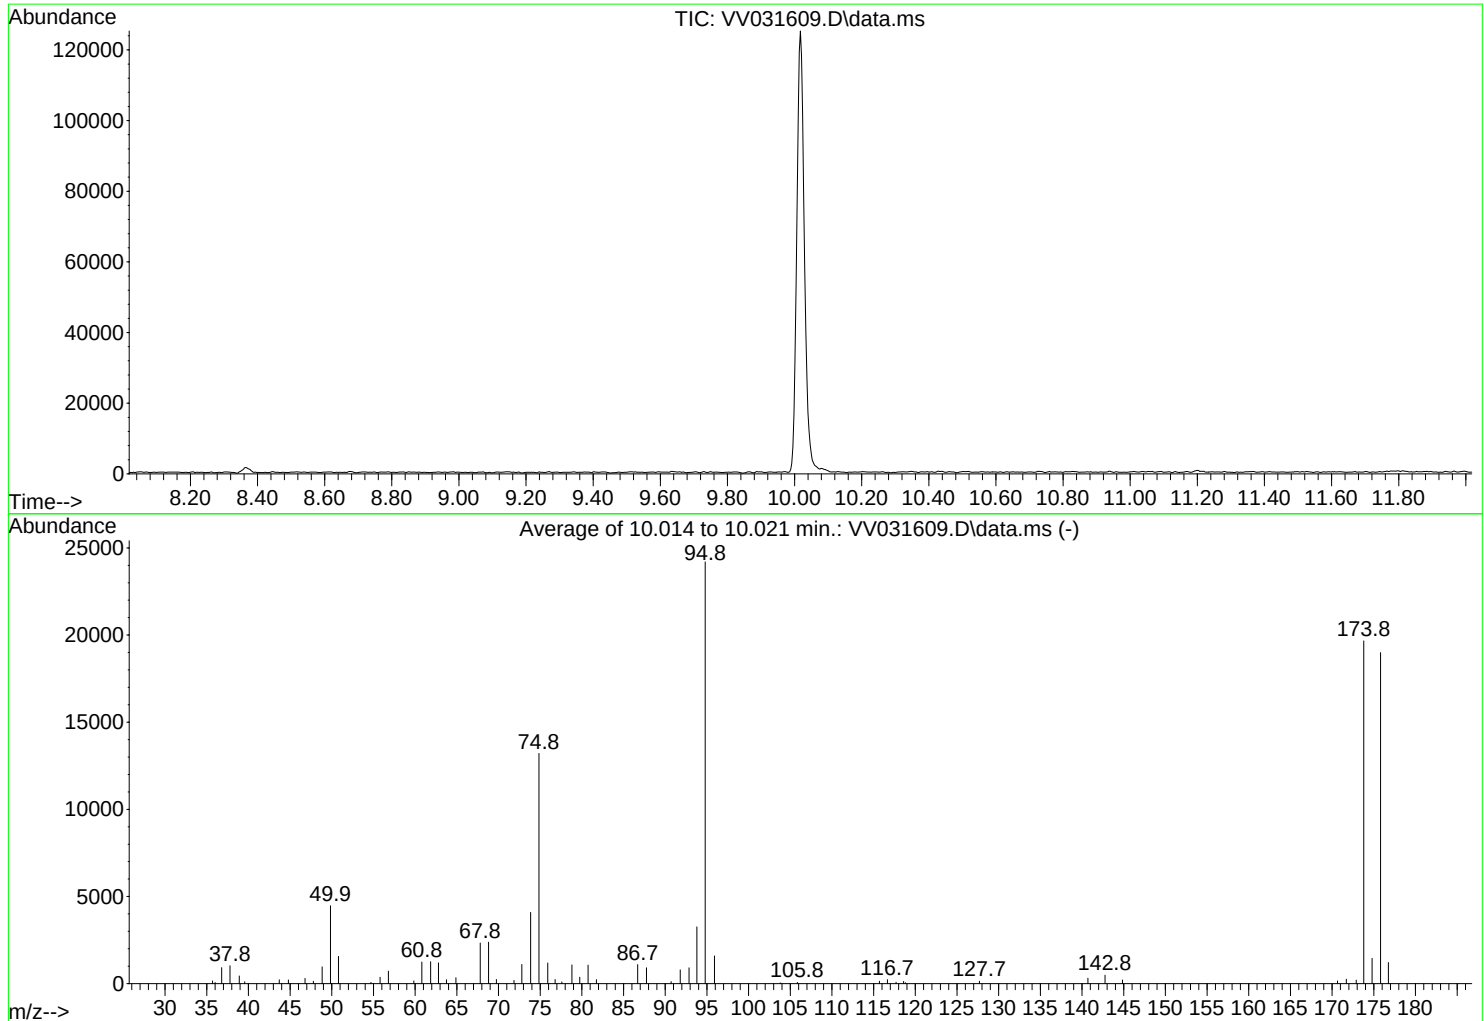

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	4471	PASS
75	95	30	80	54.6	13209	PASS
95	95	100	100	100.0	24200	PASS
96	95	5	9	6.6	1588	PASS
173	174	0.00	2	1.0	203	PASS
174	95	50	120	81.3	19664	PASS
175	174	5	9	7.4	1455	PASS
176	174	95	105	96.6	18995	PASS
177	176	5	10	6.4	1213	PASS

m/z	Abundance
39.80	158.0
43.70	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
35.70	246.0
36.80	925.0
37.80	1181.0
38.90	445.0
39.50	162.0
43.80	494.0
44.80	171.0
46.80	339.0
47.80	134.0
48.80	933.0
49.80	4357.0
50.80	1651.0
54.70	130.0
55.80	314.0
56.80	754.0
59.90	162.0
60.80	1268.0
61.80	1232.0
62.80	1162.0
63.70	247.0
64.90	251.0
67.80	2272.0
68.80	2623.0
69.70	240.0
71.80	187.0
72.80	1189.0
73.80	4046.0
74.80	13129.0
75.90	1265.0
76.80	247.0
77.60	149.0
78.80	1037.0
79.70	427.0
80.80	993.0
81.70	227.0
86.70	1057.0
87.70	1006.0
90.70	122.0
91.80	840.0
92.80	918.0
93.80	3050.0
94.80	23912.0
95.90	1628.0
105.80	116.0
115.70	144.0
116.70	221.0
118.60	203.0
127.70	143.0
140.70	344.0
142.70	404.0
144.90	208.0
170.70	150.0
171.70	262.0
173.80	18752.0
174.80	1465.0
175.80	18704.0
176.80	1186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
35.70	213.0
36.80	927.0
37.80	1067.0
38.90	467.0
39.60	155.0
43.80	526.0
44.80	214.0
46.80	315.0
47.80	137.0
48.90	974.0
49.90	4631.0
50.80	1634.0
54.70	105.0
55.80	370.0
56.80	743.0
59.90	145.0
60.80	1292.0
61.90	1302.0
62.80	1210.0
63.80	224.0
64.90	341.0
67.80	2383.0
68.80	2458.0
69.80	258.0
71.90	193.0
72.80	1114.0
73.90	4191.0
74.80	13822.0
75.90	1248.0
76.80	250.0
77.60	144.0
78.80	1112.0
79.70	377.0
80.70	1091.0
81.80	241.0
86.70	1156.0
87.80	957.0
90.70	120.0
91.80	821.0
92.80	923.0
93.80	3395.0
94.80	25080.0
95.90	1659.0
105.90	107.0
115.70	142.0
116.60	244.0
117.70	112.0
118.60	195.0
127.70	137.0
140.70	316.0
142.80	486.0
144.90	218.0
170.60	169.0
171.70	268.0
172.90	312.0
173.80	20288.0
174.80	1503.0
175.80	19616.0
176.80	1260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
36.00	181.0
36.80	902.0
37.80	852.0
38.90	424.0
39.80	175.0
43.70	555.0
44.80	259.0
46.80	260.0
47.80	130.0
48.90	975.0
49.90	4424.0
50.80	1403.0
55.80	404.0
56.80	652.0
59.80	174.0
60.80	1151.0
61.90	1239.0
62.80	1207.0
63.80	199.0
64.90	434.0
67.80	2335.0
68.80	2046.0
69.80	218.0
71.80	176.0
72.80	991.0
73.90	4020.0
74.90	12677.0
75.90	1041.0
76.80	209.0
78.80	1073.0
79.80	288.0
80.70	1119.0
81.80	232.0
86.70	1057.0
87.80	771.0
90.70	112.0
91.80	717.0
92.90	893.0
93.80	3345.0
94.80	23608.0
95.90	1476.0
103.80	138.0
115.70	123.0
116.60	221.0
117.70	126.0
118.80	176.0
127.70	140.0
140.70	278.0
142.80	565.0
144.80	218.0
170.60	152.0
171.70	237.0
172.90	296.0
173.80	19952.0
174.80	1397.0
175.80	18664.0
176.70	1192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392