


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV063020\
 Data File : VV017254.D
 Acq On : 30 Jun 2020 12:17
 Operator : SY/MD
 Sample : BFB44
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 01 21:41:10 2020

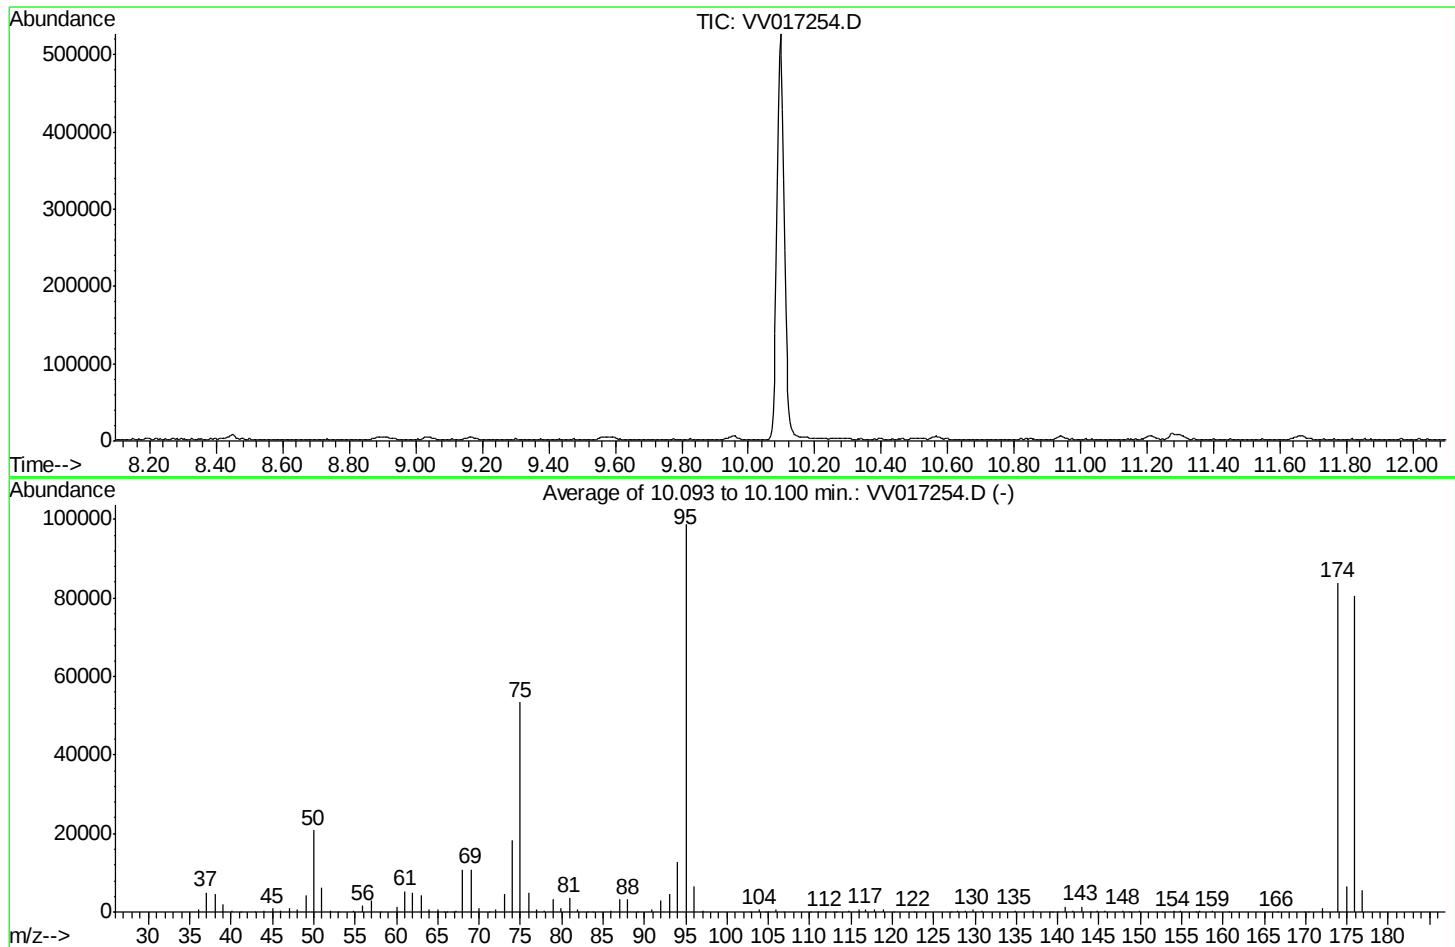

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	20733	PASS
75	95	30	80	54.1	53477	PASS
95	95	100	100	100.0	98770	PASS
96	95	5	9	6.5	6381	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.0	83928	PASS
175	174	5	9	7.6	6376	PASS
176	174	95	101	95.9	80466	PASS
177	176	5	9	6.8	5509	PASS

m/z	Abundance
36.10	204.0
36.80	164.0
38.80	134.0
39.80	261.0
41.10	137.0
41.80	114.0
43.90	303.0
50.90	111.0
51.40	142.0
55.20	108.0
71.50	122.0
76.20	113.0
182.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	1078.0
37.00	5059.0
38.00	4190.0
39.00	1902.0
40.10	463.0
41.30	111.0
44.00	736.0
45.00	867.0
46.00	154.0
47.10	865.0
48.00	567.0
49.00	4226.0
50.00	19840.0
51.00	6214.0
52.00	456.0
54.90	274.0
56.00	1458.0
57.00	2869.0
57.90	155.0
60.00	1122.0
61.00	4854.0
62.00	4960.0
63.00	3974.0
64.00	525.0
65.00	632.0
65.80	121.0
67.10	250.0
68.00	10469.0
69.00	10510.0
70.00	743.0
71.20	161.0
72.00	633.0
73.00	4514.0
74.00	18152.0
75.00	51384.0
76.00	4802.0
77.00	662.0
78.00	445.0
78.90	3260.0
79.90	1167.0
81.00	3550.0
81.90	706.0
86.00	271.0
87.00	3228.0
87.90	3234.0
90.90	445.0
92.00	3117.0
93.00	4264.0
94.00	12595.0
95.00	97368.0
96.00	6101.0
97.20	164.0
102.80	102.0
103.90	610.0
104.90	216.0
105.80	578.0
106.80	155.0
110.10	129.0
111.00	107.0
111.90	184.0
112.80	121.0
114.80	171.0
115.90	619.0
116.80	719.0
117.90	548.0
118.90	712.0
127.90	393.0
128.90	262.0
129.80	548.0
130.80	228.0
134.90	295.0
136.90	195.0
140.00	122.0
140.80	1208.0
141.90	260.0
142.90	1393.0
144.00	167.0
144.80	296.0
145.80	234.0
147.90	341.0
149.90	185.0
152.70	141.0
154.00	225.0
154.80	248.0
156.60	142.0
157.10	182.0
158.80	313.0
160.70	159.0
166.60	119.0
170.30	119.0
172.00	944.0
173.90	84392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

175.00	6277.0
175.90	79536.0
176.90	5353.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	1065.0
37.00	5481.0
38.00	4550.0
39.00	2087.0
40.10	463.0
41.30	168.0
42.90	118.0
44.00	816.0
45.00	943.0
46.00	184.0
47.10	992.0
47.90	634.0
49.00	4464.0
50.00	21448.0
51.00	6594.0
52.00	438.0
52.90	106.0
54.90	345.0
55.90	1633.0
57.00	3091.0
58.00	138.0
60.00	1231.0
61.00	5392.0
62.00	5200.0
63.00	4295.0
64.00	653.0
65.00	797.0
66.10	109.0
66.90	230.0
67.20	278.0
68.00	11144.0
69.00	11253.0
70.00	837.0
71.20	138.0
72.00	636.0
73.00	4902.0
74.00	18776.0
75.00	55456.0
76.00	5292.0
77.00	690.0
78.00	449.0
78.90	3542.0
79.90	1171.0
80.90	3747.0
81.90	806.0
86.00	303.0
87.00	3249.0
88.00	3321.0
89.10	128.0
90.90	550.0
92.00	3201.0
93.00	4664.0
94.00	13416.0
95.00	102144.0
96.00	6611.0
97.10	173.0
102.90	100.0
103.90	640.0
104.90	220.0
105.80	596.0
106.80	169.0
110.10	102.0
111.90	181.0
112.80	110.0
114.80	215.0
115.90	690.0
116.80	755.0
117.90	557.0
118.90	748.0
122.60	112.0
127.90	435.0
128.80	228.0
129.80	641.0
130.90	221.0
134.80	358.0
137.00	204.0
140.00	116.0
140.90	1185.0
141.90	290.0
142.90	1433.0
144.00	124.0
144.80	279.0
145.70	258.0
147.90	361.0
150.00	191.0
152.70	167.0
154.00	229.0
154.80	294.0
156.70	149.0
157.10	194.0
158.80	264.0
160.70	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

172.00	1013.0
173.90	87104.0
175.00	6440.0
175.90	83320.0
176.90	5753.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	890.0
37.00	5140.0
38.00	4518.0
39.00	1932.0
40.00	407.0
41.30	166.0
42.00	109.0
42.90	105.0
44.00	789.0
45.00	921.0
46.00	216.0
47.00	929.0
47.90	712.0
49.00	4219.0
50.00	20912.0
51.00	6324.0
52.00	352.0
52.90	166.0
54.80	347.0
55.90	1671.0
57.00	2926.0
58.20	130.0
60.00	1147.0
61.00	5439.0
62.00	5001.0
63.00	4253.0
64.00	722.0
65.00	896.0
66.10	133.0
66.80	238.0
68.00	10472.0
69.00	10974.0
70.00	907.0
72.00	598.0
73.00	4783.0
74.00	17904.0
75.00	53592.0
76.00	5249.0
77.00	676.0
77.90	407.0
78.90	3455.0
79.90	1056.0
80.90	3565.0
81.90	880.0
83.10	101.0
83.70	105.0
85.90	257.0
87.00	3045.0
88.00	3064.0
89.20	104.0
90.80	551.0
92.00	2915.0
93.00	4755.0
94.00	12488.0
95.00	96800.0
96.00	6433.0
97.00	206.0
103.90	559.0
104.60	177.0
105.90	529.0
106.80	159.0
111.90	139.0
112.80	101.0
113.20	115.0
114.80	196.0
115.90	634.0
116.80	784.0
117.90	465.0
118.90	739.0
120.10	110.0
127.10	142.0
127.90	407.0
128.80	227.0
129.70	591.0
130.90	209.0
134.80	378.0
137.10	210.0
139.10	122.0
139.40	123.0
140.90	1087.0
141.80	298.0
142.90	1384.0
144.80	236.0
145.70	219.0
147.90	310.0
148.70	108.0
149.90	168.0
152.70	169.0
154.00	152.0
154.80	236.0
157.10	177.0
158.70	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

160.70	108.0
169.90	106.0
172.00	991.0
173.90	80288.0
175.00	6411.0
175.90	78544.0
176.90	5422.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44