

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063021\
 Data File : VV021585.D
 Acq On : 30 Jun 2021 11:12
 Operator : SY/MD
 Sample : M2877-05ME
 Misc : 4.37g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE06ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

Signal : TIC: VV021585.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	104	rVB	158165	210689	13.27%	1.675%
2	2.082	314	324	334	rBV	327884	472847	29.79%	3.759%
3	2.609	474	488	504	rBV2	20534	50945	3.21%	0.405%
4	3.011	610	613	614	rBV	557	282	0.02%	0.002%
5	3.117	642	646	648	rBV	480	378	0.02%	0.003%
6	3.224	674	679	680	rBV3	413	344	0.02%	0.003%
7	3.256	685	689	691	rBV2	432	283	0.02%	0.002%
8	3.285	695	698	703	rVB3	671	604	0.04%	0.005%
9	3.326	707	711	712	rBV	350	162	0.01%	0.001%
10	3.359	717	721	724	rBV3	339	207	0.01%	0.002%
11	3.381	724	728	731	rBV2	416	370	0.02%	0.003%
12	3.416	736	739	743	rVB3	506	286	0.02%	0.002%
13	3.439	744	746	752	rBV3	333	282	0.02%	0.002%
14	3.523	767	772	775	rBV4	757	767	0.05%	0.006%
15	3.548	778	780	784	rVB2	731	370	0.02%	0.003%
16	3.577	784	789	791	rBV2	545	355	0.02%	0.003%
17	3.597	791	795	797	rBV3	370	324	0.02%	0.003%
18	3.619	800	802	804	rVV2	343	157	0.01%	0.001%
19	3.632	804	806	812	rVB2	701	492	0.03%	0.004%
20	3.661	812	815	818	rBV2	404	259	0.02%	0.002%
21	3.780	851	852	855	rVB2	596	210	0.01%	0.002%
22	3.806	855	860	861	rBV2	362	295	0.02%	0.002%
23	3.825	864	866	870	rBV	425	236	0.01%	0.002%
24	3.883	874	884	912	rBV2	82203	301404	18.99%	2.396%
25	4.339	1008	1026	1053	rBV	242728	619369	39.02%	4.924%
26	4.632	1112	1117	1121	rBV6	944	1055	0.07%	0.008%
27	4.690	1132	1135	1136	rBV3	567	267	0.02%	0.002%
28	4.722	1142	1145	1148	rBV	528	339	0.02%	0.003%
29	4.751	1152	1154	1156	rVB3	524	241	0.02%	0.002%
30	4.777	1156	1162	1164	rBV3	321	355	0.02%	0.003%
31	4.860	1185	1188	1190	rBV2	309	169	0.01%	0.001%
32	4.924	1207	1208	1213	rVB	287	180	0.01%	0.001%
33	4.950	1213	1216	1218	rBV	454	292	0.02%	0.002%
34	5.037	1224	1243	1288	rBV2	628115	1587429	100.00%	12.621%
35	5.516	1390	1392	1397	rVB2	607	387	0.02%	0.003%
36	5.551	1397	1403	1406	rBV3	514	467	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063021\
 Data File : VV021585.D
 Acq On : 30 Jun 2021 11:12
 Operator : SY/MD
 Sample : M2877-05ME
 Misc : 4.37g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE06ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.609	1406	1421	1456	rBV	490295	1022742	64.43%	8.131%
38	5.902	1501	1512	1526	rBV4	21666	48389	3.05%	0.385%
39	6.066	1549	1563	1597	rBV	330578	702400	44.25%	5.584%
40	6.378	1657	1660	1663	rBV2	309	264	0.02%	0.002%
41	6.400	1663	1667	1669	rBV3	322	249	0.02%	0.002%
42	6.452	1679	1683	1685	rVV	224	204	0.01%	0.002%
43	6.519	1701	1704	1708	rVB2	422	297	0.02%	0.002%
44	6.551	1711	1714	1716	rBV2	317	169	0.01%	0.001%
45	6.629	1724	1738	1740	rBV4	3717	5411	0.34%	0.043%
46	6.860	1808	1810	1813	rVB2	372	167	0.01%	0.001%
47	6.876	1813	1815	1818	rVB	456	154	0.01%	0.001%
48	6.908	1822	1825	1826	rBV2	546	262	0.02%	0.002%
49	6.944	1831	1836	1837	rBV2	236	175	0.01%	0.001%
50	6.985	1837	1849	1877	rBV	192934	375970	23.68%	2.989%
51	7.313	1939	1951	1976	rBV	735875	1325944	83.53%	10.542%
52	7.622	2037	2047	2073	rBV	132367	254816	16.05%	2.026%
53	7.854	2115	2119	2124	rBV2	834	789	0.05%	0.006%
54	7.889	2126	2130	2131	rBV3	518	224	0.01%	0.002%
55	7.908	2134	2136	2138	rBV3	299	138	0.01%	0.001%
56	7.985	2155	2160	2163	rVB3	1021	664	0.04%	0.005%
57	8.001	2163	2165	2167	rBV	289	154	0.01%	0.001%
58	8.098	2183	2195	2238	rVV	355153	818690	51.57%	6.509%
59	8.526	2326	2328	2331	rVB2	590	264	0.02%	0.002%
60	8.567	2339	2341	2343	rBV2	406	173	0.01%	0.001%
61	8.616	2352	2356	2359	rVB2	408	295	0.02%	0.002%
62	8.654	2365	2368	2370	rBV2	372	262	0.02%	0.002%
63	8.667	2370	2372	2374	rVV3	396	236	0.01%	0.002%
64	8.699	2379	2382	2383	rBV3	296	144	0.01%	0.001%
65	8.712	2384	2386	2390	rVV2	474	366	0.02%	0.003%
66	8.741	2392	2395	2397	rVB2	418	246	0.02%	0.002%
67	8.854	2418	2430	2456	rBV	745690	1261482	79.47%	10.029%
68	9.233	2546	2548	2550	rBV	283	147	0.01%	0.001%
69	9.246	2550	2552	2555	rVV	232	135	0.01%	0.001%
70	9.265	2555	2558	2563	rVV3	305	261	0.02%	0.002%
71	9.310	2570	2572	2574	rBV	461	156	0.01%	0.001%
72	9.349	2581	2584	2588	rVB3	418	331	0.02%	0.003%
73	9.390	2591	2597	2599	rBV2	468	454	0.03%	0.004%
74	9.445	2612	2614	2618	rVB	394	266	0.02%	0.002%
75	9.464	2618	2620	2623	rBV	265	149	0.01%	0.001%
76	9.484	2623	2626	2628	rBV2	380	265	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063021\
 Data File : VW021585.D
 Acq On : 30 Jun 2021 11:12
 Operator : SY/MD
 Sample : M2877-05ME
 Misc : 4.37g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE06ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.609	2663	2665	2667	rBV	413	203	0.01%	0.002%
78	9.715	2697	2698	2702	rBV2	386	174	0.01%	0.001%
79	9.741	2703	2706	2708	rVB	322	156	0.01%	0.001%
80	9.773	2713	2716	2718	rVV2	275	178	0.01%	0.001%
81	9.841	2733	2737	2738	rBV2	579	344	0.02%	0.003%
82	9.934	2764	2766	2771	rBV4	319	255	0.02%	0.002%
83	10.008	2787	2789	2792	rVV2	378	216	0.01%	0.002%
84	10.027	2792	2795	2800	rVB2	379	311	0.02%	0.002%
85	10.127	2818	2826	2840	rVB2	4273	6551	0.41%	0.052%
86	10.220	2843	2855	2875	rBV	488592	790282	49.78%	6.283%
87	10.448	2924	2926	2927	rBV	304	149	0.01%	0.001%
88	10.516	2944	2947	2950	rBV	300	224	0.01%	0.002%
89	10.548	2950	2957	2958	rBV3	675	695	0.04%	0.006%
90	10.757	3021	3022	3024	rBV	360	163	0.01%	0.001%
91	10.796	3029	3034	3035	rBV3	431	400	0.03%	0.003%
92	10.992	3094	3095	3100	rVB2	418	289	0.02%	0.002%
93	11.034	3101	3108	3115	rVV5	1303	2121	0.13%	0.017%
94	11.149	3134	3144	3152	rBV3	5681	8979	0.57%	0.071%
95	11.252	3164	3176	3195	rBV	883015	1374096	86.56%	10.925%
96	11.538	3260	3265	3267	rBV3	594	536	0.03%	0.004%
97	11.554	3267	3270	3272	rBV2	1047	667	0.04%	0.005%
98	11.628	3281	3293	3318	rBV	831107	1312933	82.71%	10.438%
99	12.837	3666	3669	3670	rBV	546	281	0.02%	0.002%
100	13.069	3737	3741	3744	rBV5	792	771	0.05%	0.006%




Sum of corrected areas: 12577976

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063021\
Data File : VV021585.D
Acq On : 30 Jun 2021 11:12
Operator : SY/MD
Sample : M2877-05ME
Misc : 4.37g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE06ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

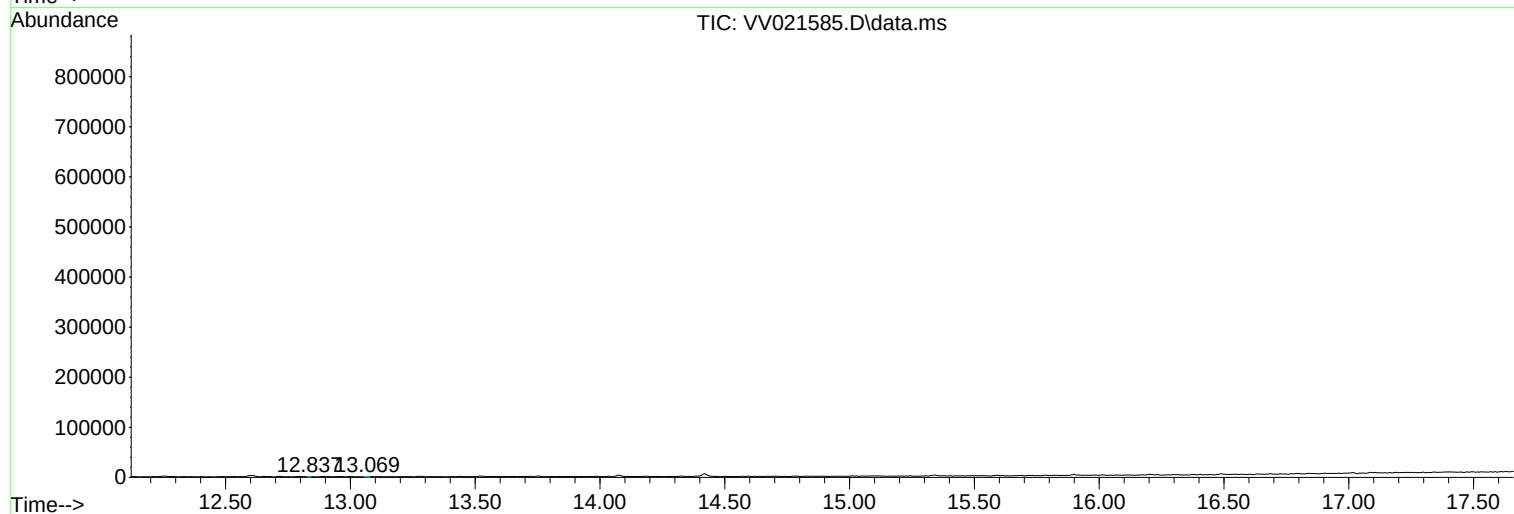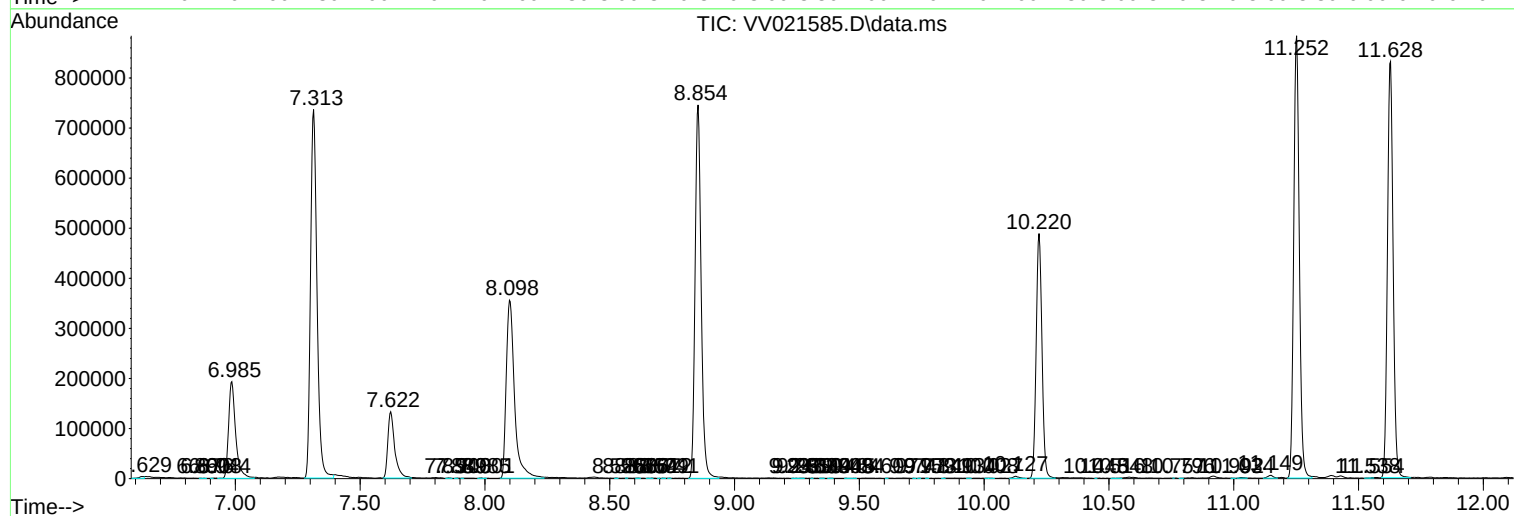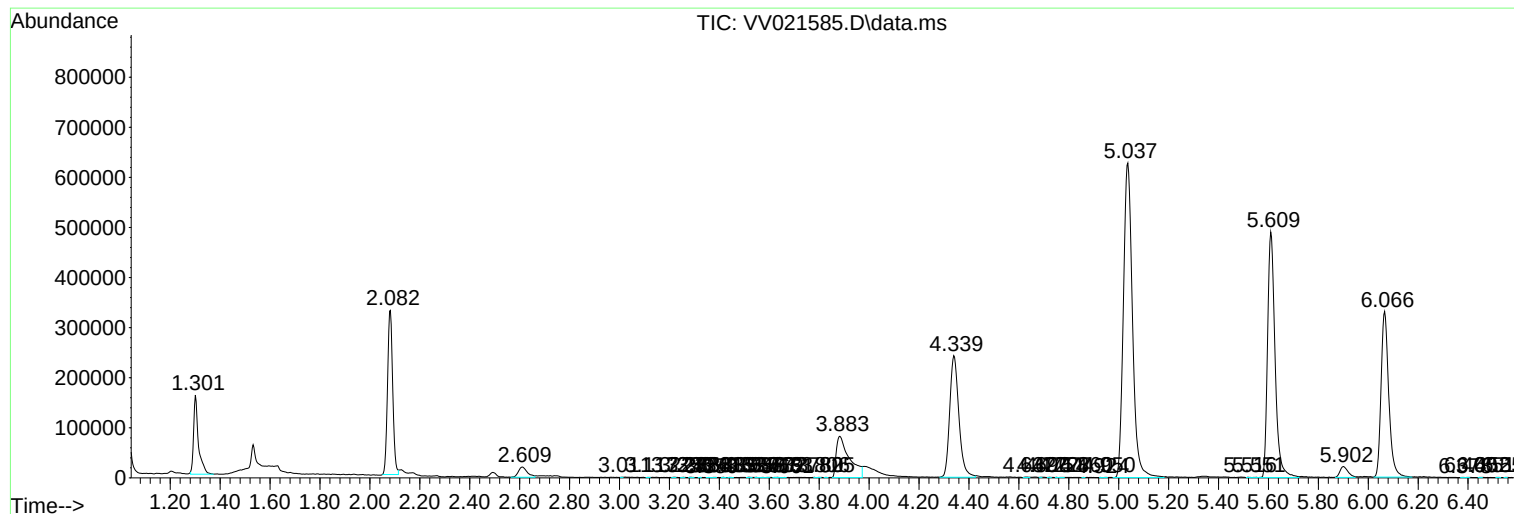

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063021\
Data File : VV021585.D
Acq On : 30 Jun 2021 11:12
Operator : SY/MD
Sample : M2877-05ME
Misc : 4.37g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE06ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063021\
Data File : VV021585.D
Acq On : 30 Jun 2021 11:12
Operator : SY/MD
Sample : M2877-05ME
Misc : 4.37g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE06ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
