
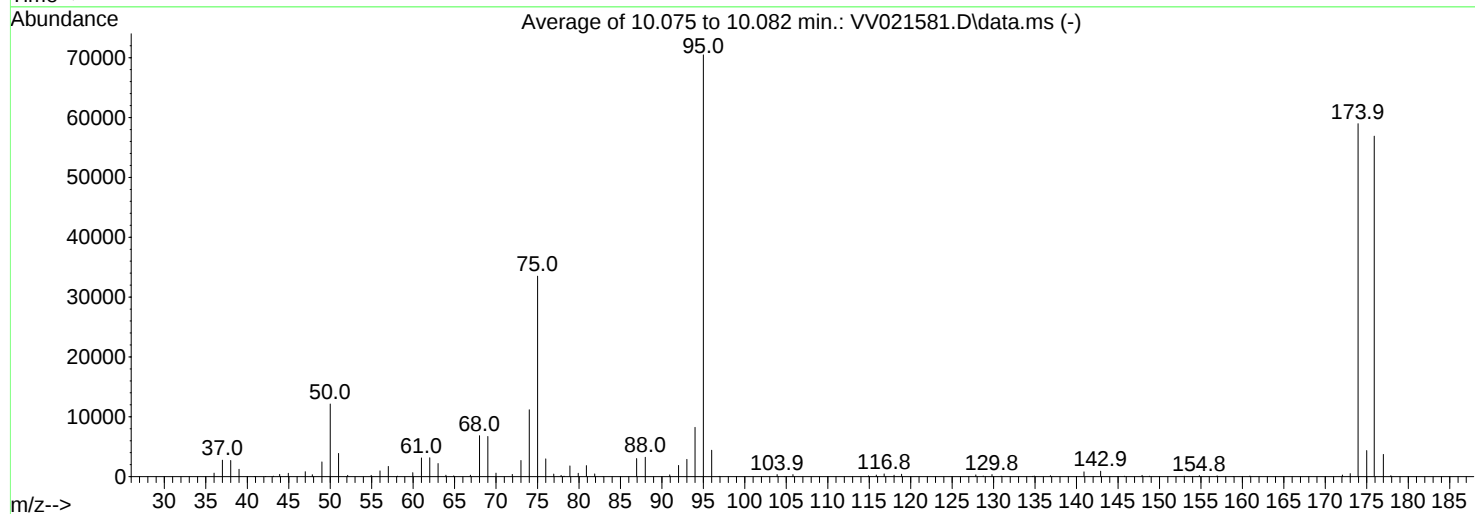


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063021\
Data File : VV021581.D
Acq On : 30 Jun 2021 09:10
Operator : SY/MD
Sample : BFB75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB175

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Title : VOC Analysis
Last Update : Sat Jul 03 00:01:46 2021

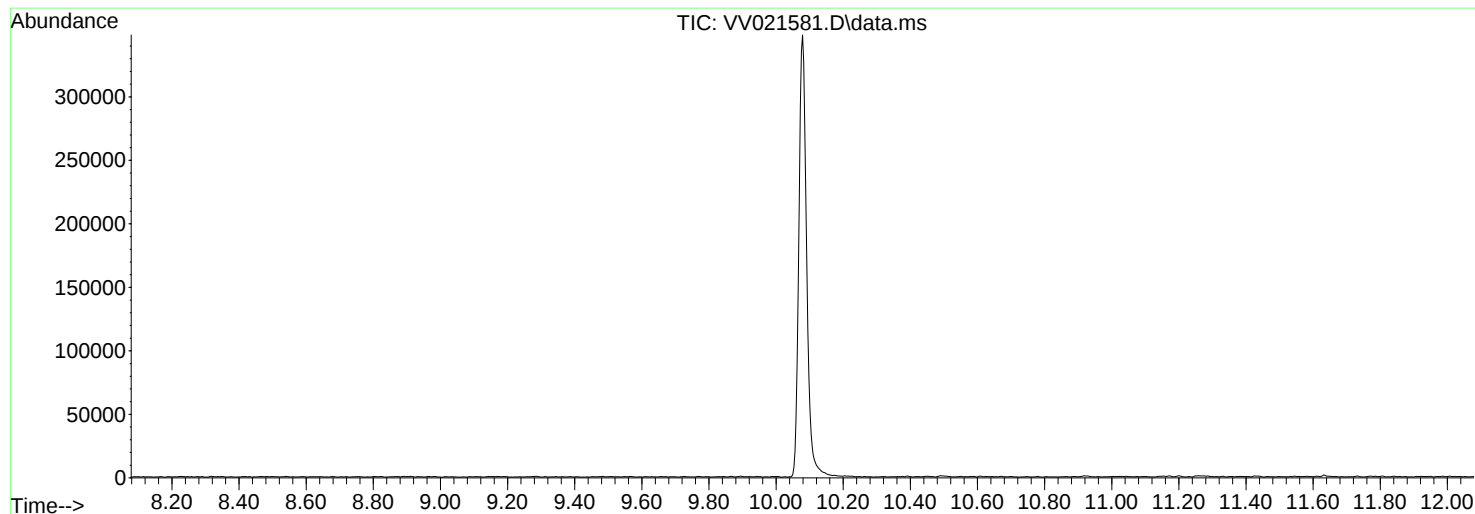

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	12133	PASS
75	95	30	80	47.5	33507	PASS
95	95	100	100	100.0	70477	PASS
96	95	5	9	6.2	4400	PASS
173	174	0.00	2	0.9	511	PASS
174	95	50	120	83.7	58973	PASS
175	174	5	9	7.4	4352	PASS
176	174	95	105	96.5	56899	PASS
177	176	5	10	6.5	3704	PASS

m/z	Abundance
38.60	113.0
40.00	247.0
43.90	475.0

Instrument :
MSVOA_V
ClientSampleId :
BFB175

m/z	Abundance
36.00	569.0
37.00	2878.0
38.00	2736.0
39.00	1247.0
39.90	248.0
40.90	103.0
43.90	843.0
45.00	579.0
47.00	824.0
47.80	331.0
49.00	2564.0
50.00	12251.0
51.00	3911.0
52.10	216.0
54.90	252.0
56.00	980.0
57.00	1782.0
58.10	123.0
60.00	695.0
61.00	3270.0
62.00	3183.0
63.00	2174.0
64.00	219.0
64.90	123.0
66.90	255.0
68.00	6767.0
69.00	6824.0
70.00	529.0
71.90	422.0
73.00	2801.0
74.00	11028.0
75.00	33976.0
76.00	3010.0
77.00	450.0
77.80	217.0
78.90	1830.0
79.90	565.0
80.90	1935.0
81.90	502.0
86.90	3021.0
88.00	3147.0
91.00	261.0
92.00	1855.0
93.00	2966.0
94.00	8314.0
95.00	70848.0
96.00	4515.0
96.90	138.0
103.90	367.0
104.80	110.0
105.80	356.0
114.90	149.0
115.80	289.0
116.80	448.0
118.00	253.0
118.90	451.0
127.90	257.0
128.80	109.0
129.80	331.0
130.90	111.0
134.70	135.0
136.80	175.0
140.90	828.0
142.10	107.0
142.90	860.0
145.80	121.0
147.90	271.0
154.80	208.0
157.00	125.0
160.90	104.0
172.00	230.0
173.00	465.0
174.00	57280.0
175.00	4503.0
175.90	55256.0
177.00	3591.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB175

m/z	Abundance
36.00	607.0
37.00	2601.0
38.00	2571.0
39.00	1131.0
40.00	245.0
43.10	121.0
43.90	832.0
44.90	548.0
47.00	800.0
47.90	316.0
49.00	2318.0
50.00	11715.0
51.00	3739.0
52.10	228.0
55.00	192.0
56.00	921.0
57.00	1601.0
59.90	610.0
61.00	2927.0
62.00	3013.0
63.00	2183.0
63.90	270.0
64.90	167.0
66.90	235.0
68.00	6744.0
69.00	6376.0
70.00	619.0
72.00	352.0
73.00	2567.0
74.00	10910.0
75.00	32048.0
76.00	2818.0
76.80	398.0
77.90	227.0
78.90	1714.0
79.90	576.0
80.90	1742.0
81.90	409.0
82.90	103.0
87.00	2943.0
88.00	3190.0
90.90	313.0
92.00	1839.0
93.00	2724.0
94.00	7896.0
95.00	67808.0
96.00	4150.0
103.90	332.0
105.80	306.0
114.90	111.0
115.90	261.0
116.80	474.0
118.00	230.0
118.90	354.0
127.80	312.0
128.70	112.0
129.80	322.0
134.90	157.0
136.90	172.0
140.90	760.0
142.90	931.0
147.90	175.0
148.80	104.0
153.00	105.0
154.80	177.0
156.90	156.0
160.90	114.0
172.10	307.0
173.00	542.0
173.90	58496.0
175.00	4024.0
175.90	56752.0
177.00	3684.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB175

m/z	Abundance
36.00	628.0
37.00	2781.0
38.00	2806.0
39.00	1302.0
39.90	238.0
42.20	109.0
43.20	102.0
43.90	876.0
45.00	582.0
47.00	846.0
47.90	347.0
49.00	2526.0
50.00	12434.0
51.00	4012.0
52.10	244.0
54.90	204.0
56.00	993.0
57.00	1782.0
58.10	117.0
59.90	664.0
61.00	3197.0
62.00	3275.0
63.00	2253.0
64.00	272.0
64.90	146.0
66.90	251.0
68.00	7062.0
69.00	6934.0
70.00	650.0
71.90	398.0
73.00	2764.0
74.00	11564.0
75.00	34496.0
76.00	3092.0
77.00	455.0
77.80	209.0
78.20	223.0
78.90	1853.0
79.90	555.0
80.90	1863.0
81.90	455.0
87.00	3078.0
88.00	3335.0
90.90	290.0
92.00	1917.0
93.00	2995.0
94.00	8526.0
95.00	72776.0
96.00	4536.0
103.90	375.0
105.80	353.0
114.90	135.0
115.90	297.0
116.80	489.0
118.00	261.0
118.90	419.0
127.80	309.0
128.70	111.0
129.80	356.0
130.90	111.0
134.90	153.0
136.80	172.0
140.90	840.0
142.90	928.0
145.80	118.0
147.90	231.0
148.80	100.0
153.00	117.0
154.80	207.0
156.90	156.0
158.90	106.0
160.90	118.0
172.10	285.0
173.00	527.0
174.00	61144.0
175.00	4529.0
175.90	58688.0
177.00	3836.0
177.90	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB175