

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026600.D
 Acq On : 30 Jun 2022 12:18
 Operator : SY/MD
 Sample : N3534-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

Quant Time: Jul 01 00:20:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	421346	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	410997	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	212407	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	149594	43.554	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.100%
7) Chloroethane-d5	1.580	69	128791	43.722	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.440%
11) 1,1-Dichloroethene-d2	2.121	63	314331	48.583	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.160%
21) 2-Butanone-d5	3.915	46	170025	98.874	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.870%
24) Chloroform-d	4.455	84	640	0.097	ug/L	0.10
Spiked Amount	50.000	Range	70 - 125	Recovery	=	0.200%#
26) 1,2-Dichloroethane-d4	5.037	65	173623	46.009	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.020%
32) Benzene-d6	5.053	84	580594	46.457	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.920%
36) 1,2-Dichloropropane-d6	6.072	67	189386	48.111	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.220%
41) Toluene-d8	7.316	98	508838	46.354	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.700%
43) trans-1,3-Dichloroprop...	7.622	79	75854	47.995	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.980%
47) 2-Hexanone-d5	8.091	63	124645	91.553	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.550%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	259464	45.651	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.300%
66) 1,2-Dichlorobenzene-d4	11.622	152	196214	47.201	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.400%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.146	85	111789	36.898	ug/L	100
3) Chloromethane	1.256	50	121955	32.465	ug/L	100
5) Vinyl chloride	1.326	62	239652	60.392	ug/L	100
6) Bromomethane	1.535	94	44833	17.947	ug/L	99
8) Chloroethane	1.600	64	77118	28.961	ug/L	99
9) Trichlorofluoromethane	1.764	101	290703	52.212	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.127	101	83325	25.493	ug/L	99
12) 1,1-Dichloroethene	2.127	96	185693	57.665	ug/L	95
13) Acetone	2.191	43	29155	23.286	ug/L	46
14) Carbon disulfide	2.304	76	5146	0.576	ug/L	96
15) Methyl Acetate	2.461	43	2109	0.802	ug/L #	69
16) Methylene chloride	2.519	84	169507	44.839	ug/L	99
17) trans-1,2-Dichloroethene	2.770	96	70405	21.192	ug/L	100
19) 1,1-Dichloroethane	3.201	63	416262	69.212	ug/L	100
20) cis-1,2-Dichloroethene	3.921	96	161651	45.541	ug/L	100
23) Bromochloromethane	4.259	128	83892	41.786	ug/L	98
25) Chloroform	4.381	83	388471	61.033	ug/L	100
27) 1,2-Dichloroethane	5.133	62	330453	76.821	ug/L	100
30) 1,1,1-Trichloroethane	4.616	97	120870	22.511	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026600.D
 Acq On : 30 Jun 2022 12:18
 Operator : SY/MD
 Sample : N3534-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1


Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0

Quant Time: Jul 01 00:20:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

31) Carbon tetrachloride	4.834	117	287358	63.738	ug/L	100
33) Benzene	5.104	78	672769	50.486	ug/L	100
34) Trichloroethene	5.915	95	299166	88.948	ug/L	99
37) 1,2-Dichloropropane	6.175	63	144968	41.764	ug/L	99
38) Bromodichloromethane	6.513	83	91991	20.624	ug/L	99
39) cis-1,3-Dichloropropene	7.027	75	122447	26.197	ug/L	98
44) trans-1,3-Dichloropropene	7.651	75	197993	45.935	ug/L	99
45) 1,1,2-Trichloroethane	7.837	97	94583	26.845	ug/L	99
46) Tetrachloroethene	7.976	164	213010	78.367	ug/L	99
49) Dibromochloromethane	8.246	129	126077	37.175	ug/L	99
50) 1,2-Dibromoethane	8.352	107	111217	31.105	ug/L	96
57) 1,1,2,2-Tetrachloroethane	10.239	83	209054	38.124	ug/L	100
59) Bromoform	9.731	173	82348	44.044	ug/L	99
63) 1,2,4-Trimethylbenzene	10.914	105	522112	49.974	ug/L	100
68) 1,2-Dibromo-3-chloropr...	12.426	75	34201	40.261	ug/L	95





(#) = qualifier out of range (m) = manual integration (+) = signals summed

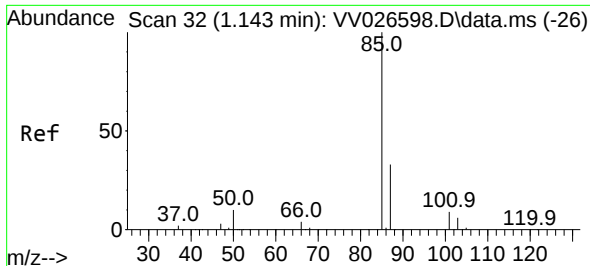

#2
 Dichlorodifluoromethane
 Concen: 36.898 ug/L
 RT: 1.146 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18




Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0


Tgt Ion: 85 Resp: 111789
 Ion Ratio Lower Upper
 85 100
 87 32.5 25.8 38.8

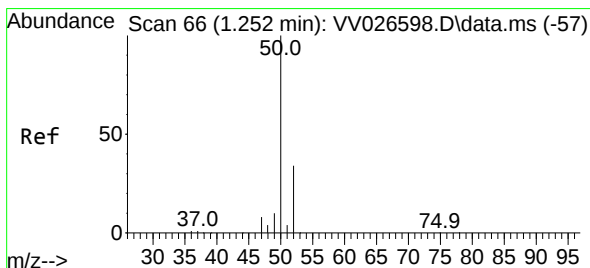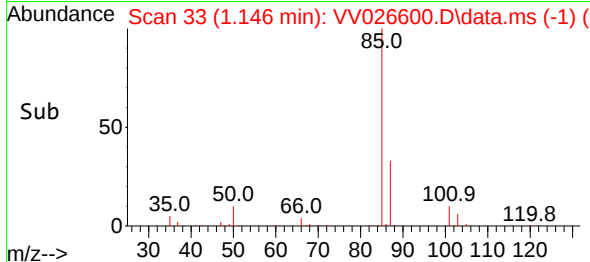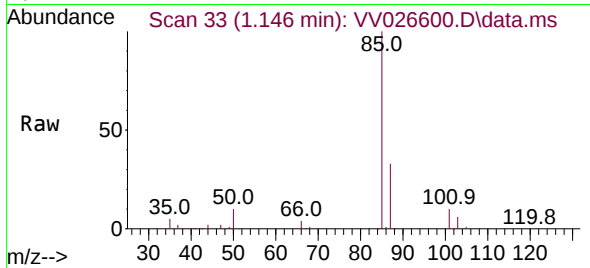

#3
 Chloromethane
 Concen: 32.465 ug/L
 RT: 1.256 min Scan# 67
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Tgt Ion: 50 Resp: 121955
 Ion Ratio Lower Upper
 50 100
 52 32.8 23.1 42.9


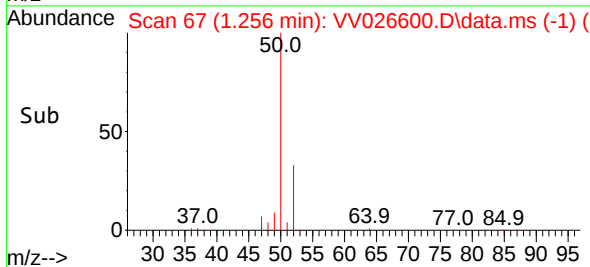

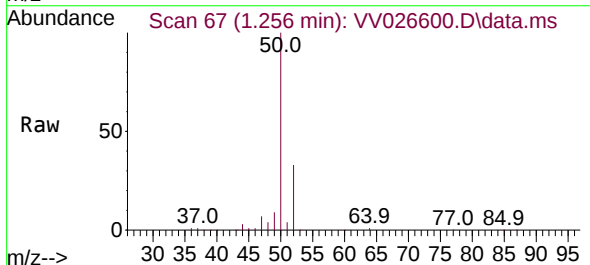


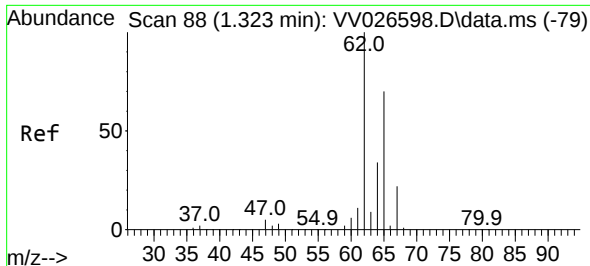

#5
 Vinyl chloride
 Concen: 60.392 ug/L
 RT: 1.326 min Scan# 89
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18




Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0


Tgt Ion: 62 Resp: 239652
 Ion Ratio Lower Upper
 62 100
 64 33.9 23.7 44.1

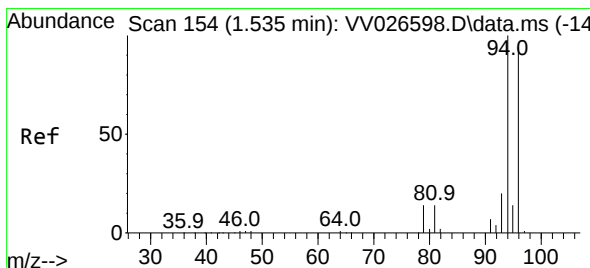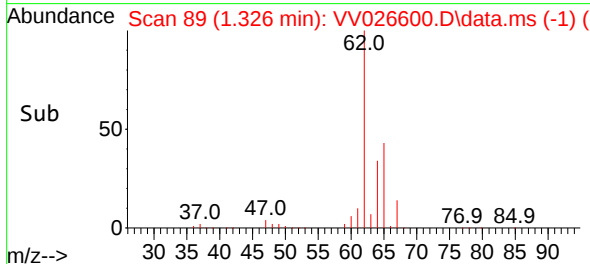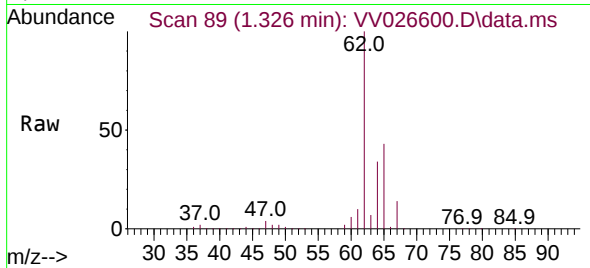

#6
 Bromomethane
 Concen: 17.947 ug/L
 RT: 1.535 min Scan# 154
 Delta R.T. -0.000 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Tgt Ion: 94 Resp: 44833
 Ion Ratio Lower Upper
 94 100
 96 94.2 65.6 121.8


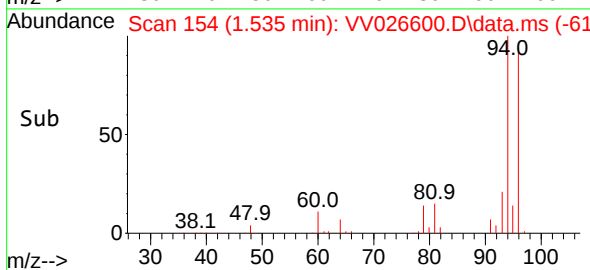

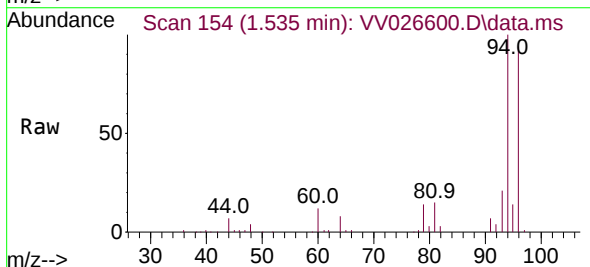


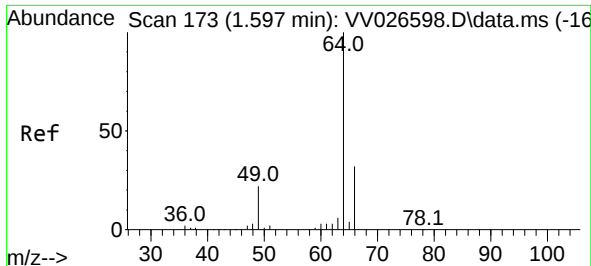

#8
Chloroethane
Concen: 28.961 ug/L
RT: 1.600 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0


Tgt Ion: 64 Resp: 77118
Ion Ratio Lower Upper
64 100
66 31.4 21.6 40.0

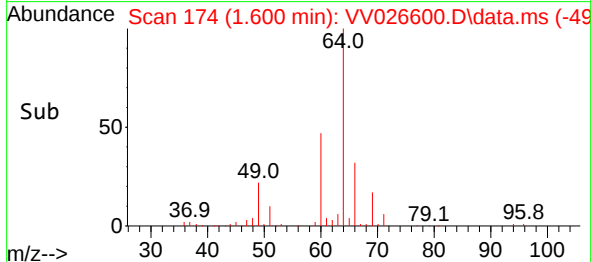

#9
Trichlorofluoromethane
Concen: 52.212 ug/L
RT: 1.764 min Scan# 225
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion:101 Resp: 290703
Ion Ratio Lower Upper
101 100
103 64.3 51.8 77.6


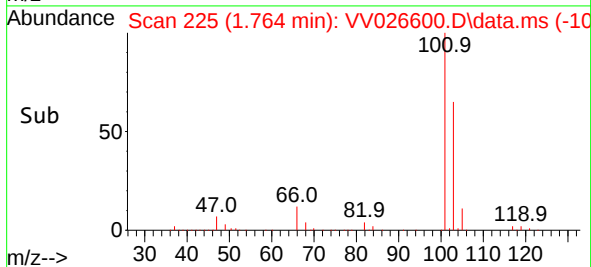

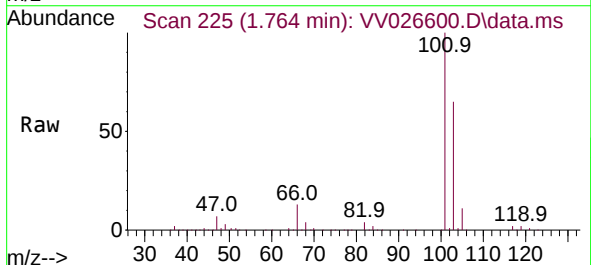


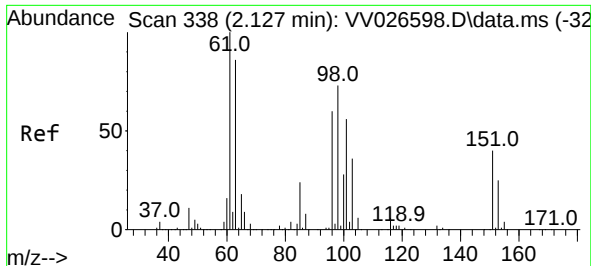

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 25.493 ug/L
 RT: 2.127 min Scan# 338
 Delta R.T. -0.000 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18




Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0


Tgt Ion:101 Resp: 83325
 Ion Ratio Lower Upper
 101 100
 85 43.3 34.5 51.7
 151 69.6 56.9 85.3

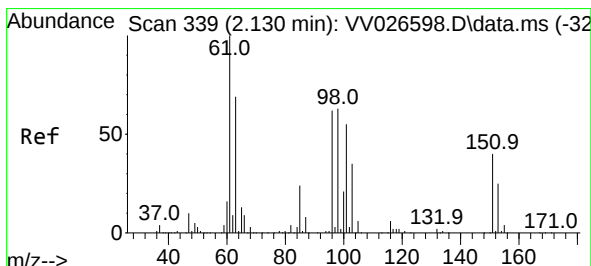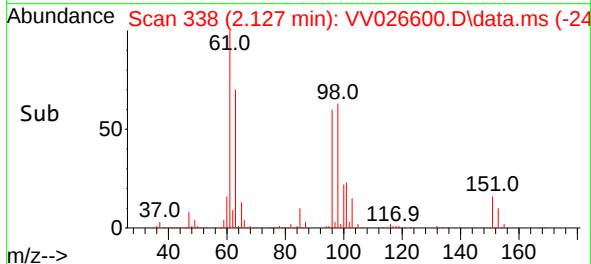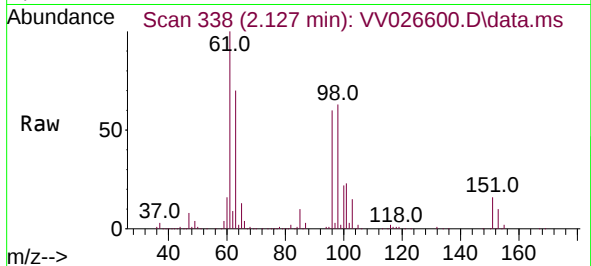

#12
 1,1-Dichloroethene
 Concen: 57.665 ug/L
 RT: 2.127 min Scan# 338
 Delta R.T. -0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Tgt Ion: 96 Resp: 185693
 Ion Ratio Lower Upper
 96 100
 61 165.5 114.9 213.5
 63 115.9 88.8 164.8



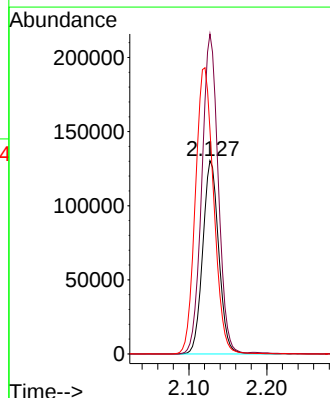
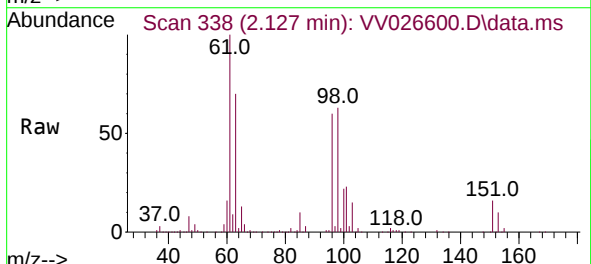




#13
Acetone
Concen: 23.286 ug/L
RT: 2.191 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0


Tgt Ion: 43 Resp: 29155
Ion Ratio Lower Upper
43 100
58 2.0 0.0 65.0

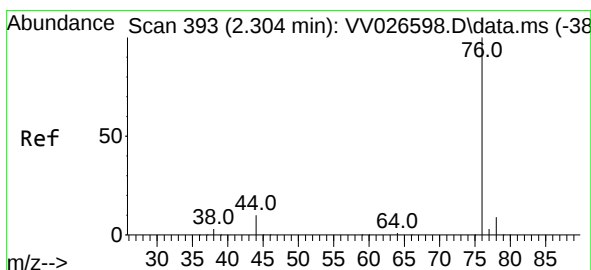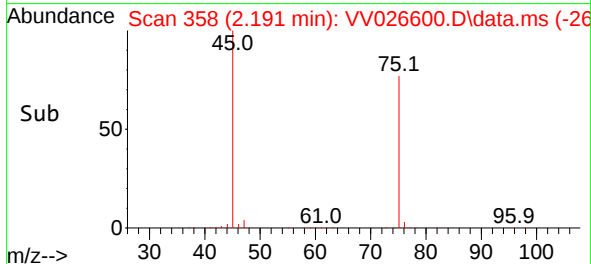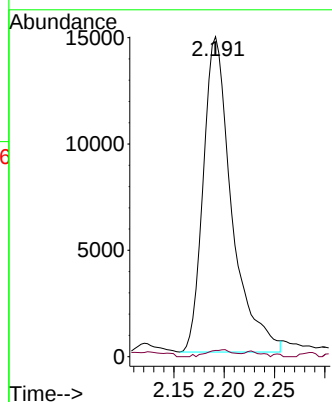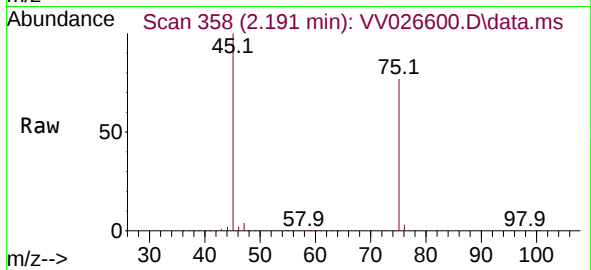

#14
Carbon disulfide
Concen: 0.576 ug/L
RT: 2.304 min Scan# 393
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion: 76 Resp: 5146
Ion Ratio Lower Upper
76 100
78 10.5 7.1 10.7


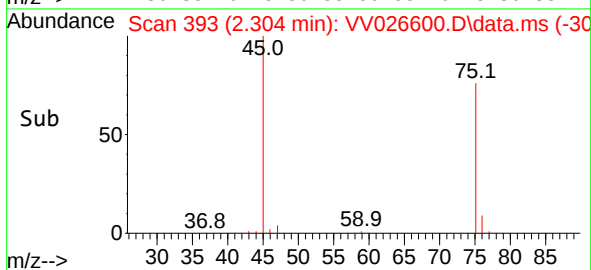
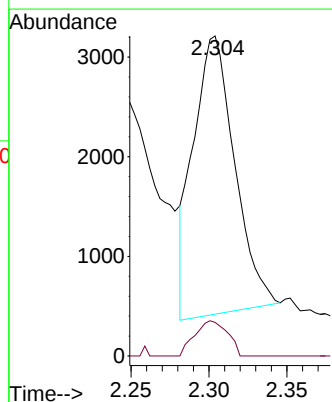
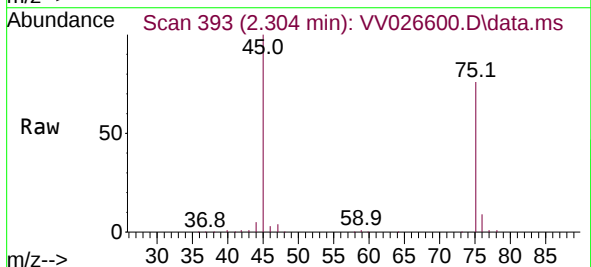




#15
Methyl Acetate
Concen: 0.802 ug/L
RT: 2.461 min Scan# 441
Delta R.T. 0.010 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0


Tgt Ion: 43 Resp: 2109
Ion Ratio Lower Upper
43 100
74 11.3 22.2 33.4#

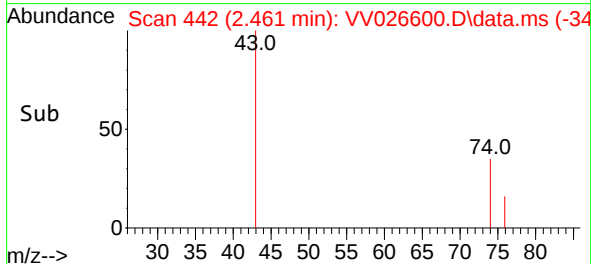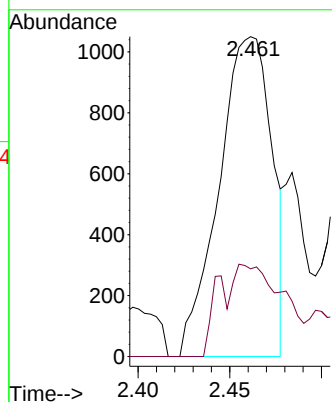

#16
Methylene chloride
Concen: 44.839 ug/L
RT: 2.519 min Scan# 460
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18


Tgt Ion: 84 Resp: 169507
Ion Ratio Lower Upper
84 100
86 64.5 45.4 84.2
49 107.9 76.5 142.1

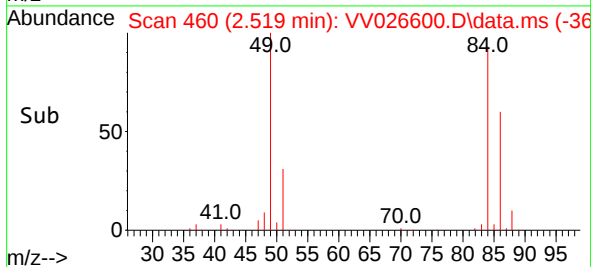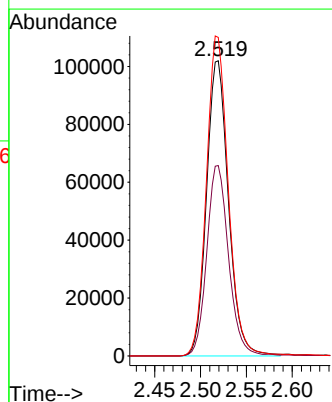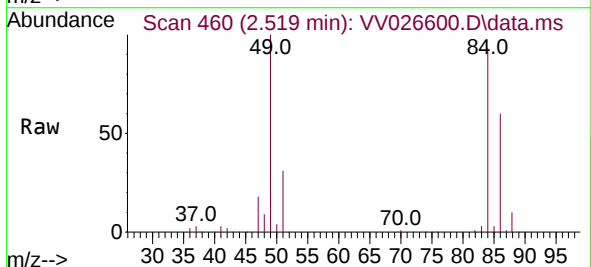



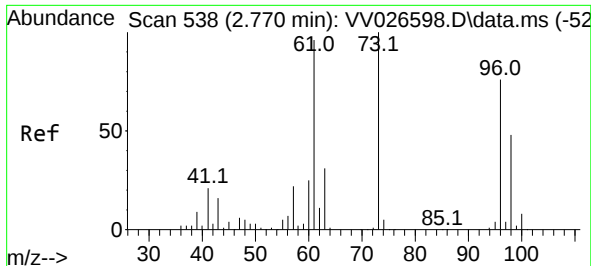


#17
trans-1,2-Dichloroethene
Concen: 21.192 ug/L
RT: 2.770 min Scan# 51
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0



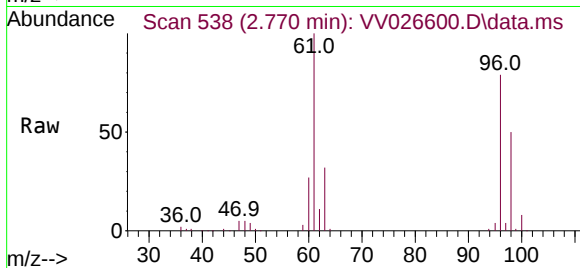



Tgt Ion: 96	Resp: 70405
Ion Ratio	Lower Upper
96 100	
61 125.8	88.4 164.2
98 63.5	44.2 82.0

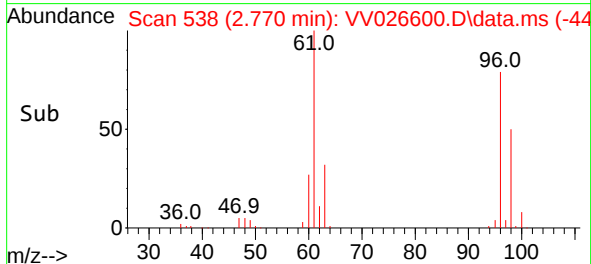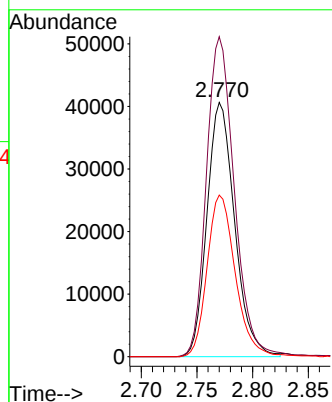

#19
1,1-Dichloroethane
Concen: 69.212 ug/L
RT: 3.201 min Scan# 672
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion: 63	Resp: 416262
Ion Ratio	Lower Upper
63 100	
65 31.7	22.2 41.2
83 13.4	9.5 17.7


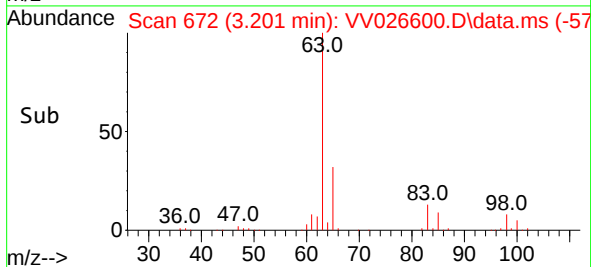

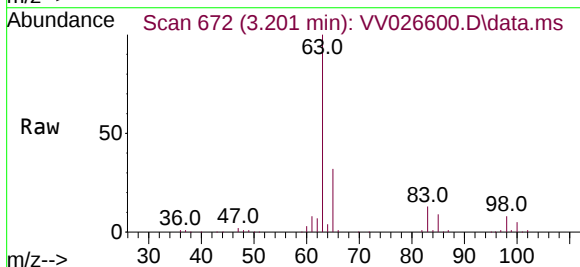


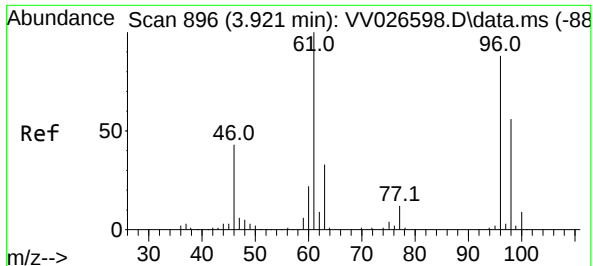

#20
cis-1,2-Dichloroethene
Concen: 45.541 ug/L
RT: 3.921 min Scan# 896
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0


Tgt Ion: 96 Resp: 161651
Ion Ratio Lower Upper
96 100
61 117.5 82.6 153.4
68 0.0 0.0 0.0

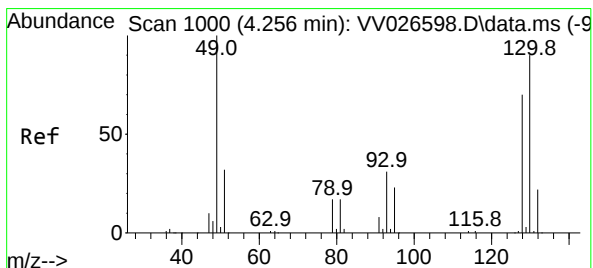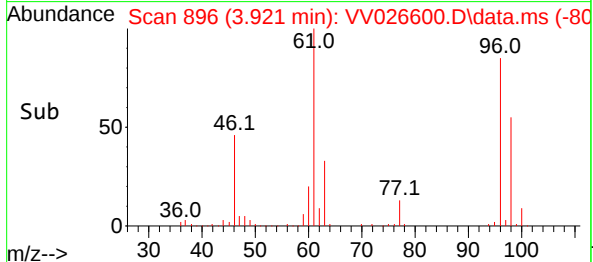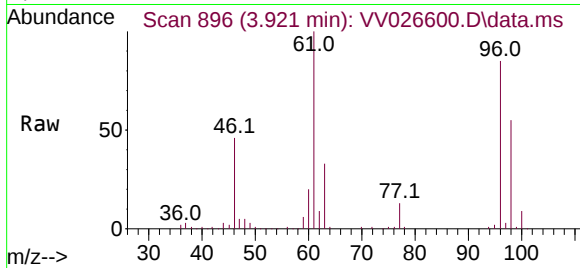

#23
Bromochloromethane
Concen: 41.786 ug/L
RT: 4.259 min Scan# 1001
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion:128 Resp: 83892
Ion Ratio Lower Upper
128 100
49 141.5 102.3 190.1
130 128.0 90.2 167.6
51 45.9 36.2 54.4

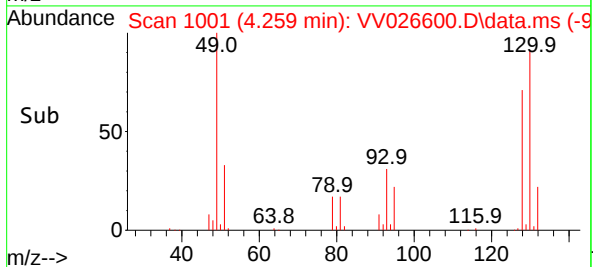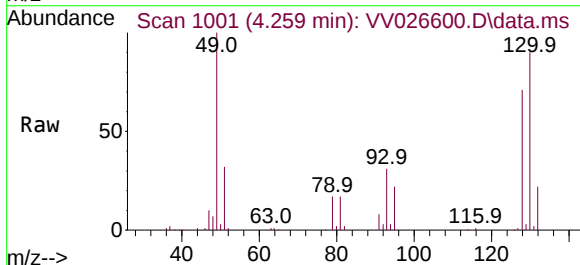

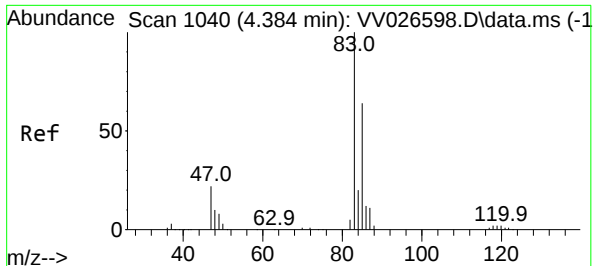

#25

Chloroform

Concen: 61.033 ug/L

RT: 4.381 min Scan# 1040

Delta R.T. -0.003 min

Lab File: VV026600.D

Acq: 30 Jun 2022 12:18

Instrument :

MSVOA_V

ClientSampleId :





A0AH0

Tgt Ion: 83 Resp: 388471

Ion Ratio Lower Upper

83 100

85 65.1 45.4 84.4

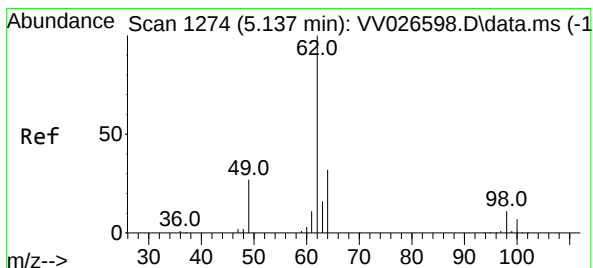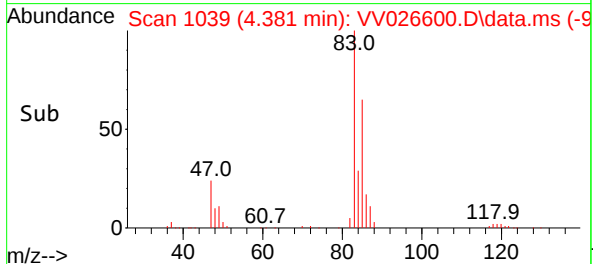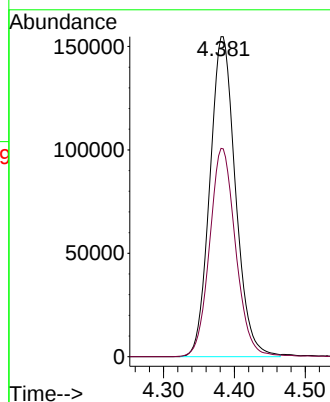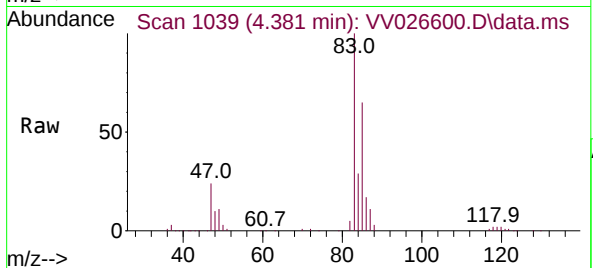

#27

1,2-Dichloroethane

Concen: 76.821 ug/L

RT: 5.133 min Scan# 1273

Delta R.T. -0.003 min

Lab File: VV026600.D




Acq: 30 Jun 2022 12:18


Tgt Ion: 62 Resp: 330453

Ion Ratio Lower Upper

62 100

98 10.9 8.8 13.2


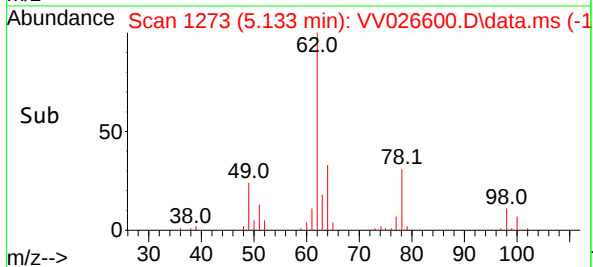

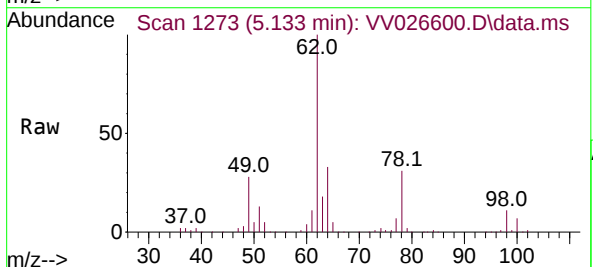


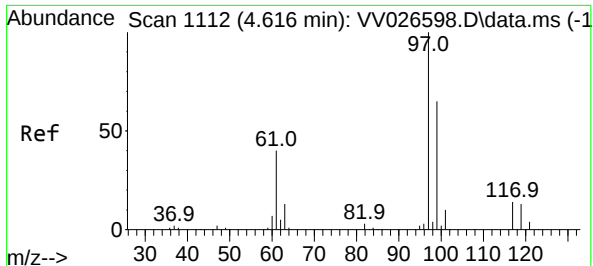

#30
1,1,1-Trichloroethane
Concen: 22.511 ug/L
RT: 4.616 min Scan# 1112
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0


Tgt Ion: 97 Resp: 120870
Ion Ratio Lower Upper
97 100
99 63.9 52.1 78.1
61 40.1 31.8 47.6

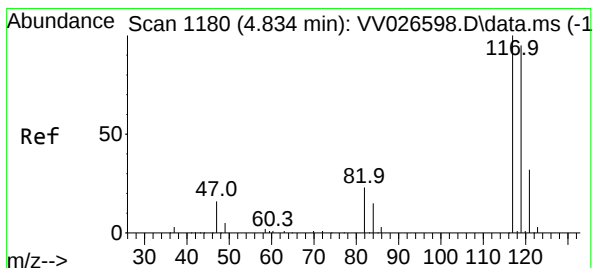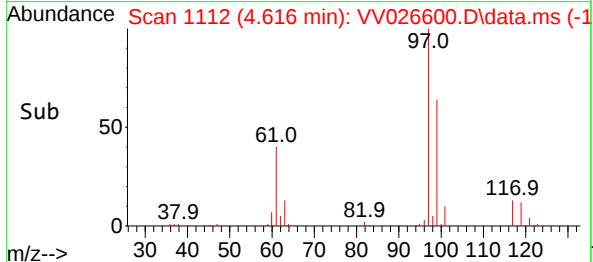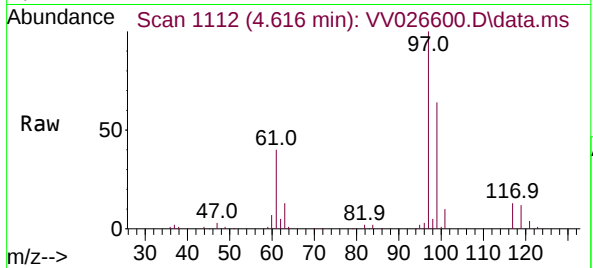

#31
Carbon tetrachloride
Concen: 63.738 ug/L
RT: 4.834 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion: 117 Resp: 287358
Ion Ratio Lower Upper
117 100
119 95.9 77.0 115.4


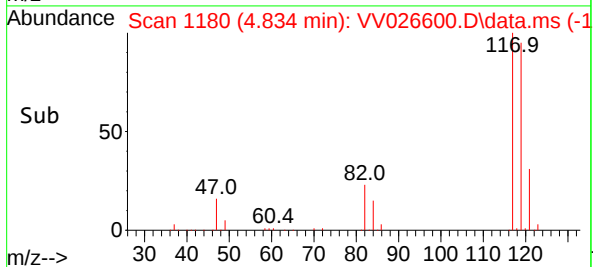

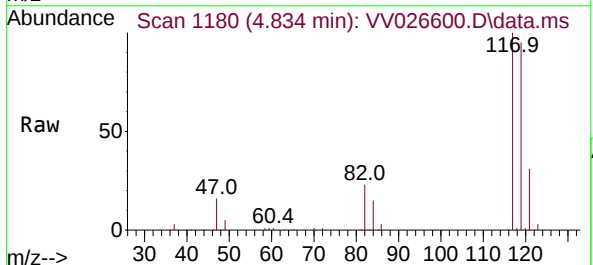


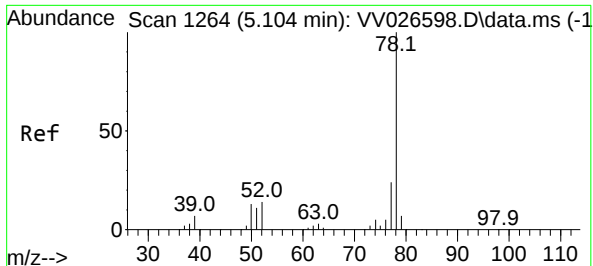

#33
Benzene
Concen: 50.486 ug/L
RT: 5.104 min Scan# 11
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0




Tgt Ion: 78 Resp: 672769

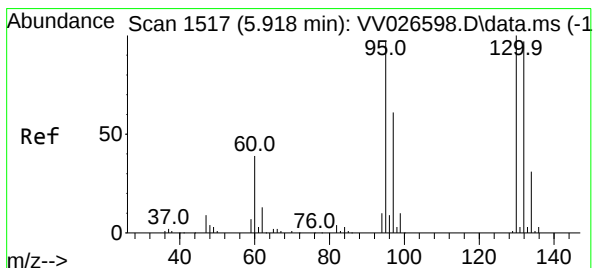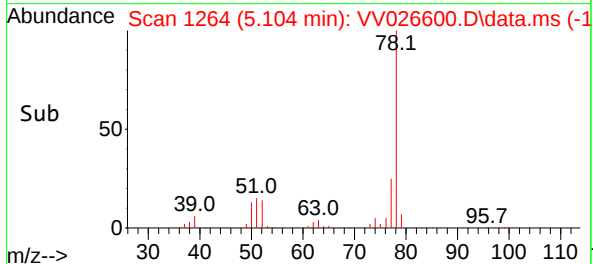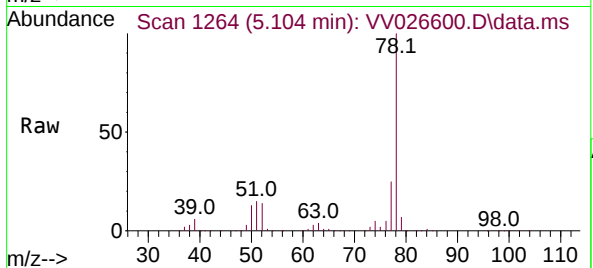


#34
Trichloroethene
Concen: 88.948 ug/L
RT: 5.915 min Scan# 1516
Delta R.T. -0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion: 95 Resp: 299166

Ion	Ratio	Lower	Upper
95	100		
97	63.7	45.0	83.6
132	99.5	69.0	128.2
130	105.0	73.1	135.8

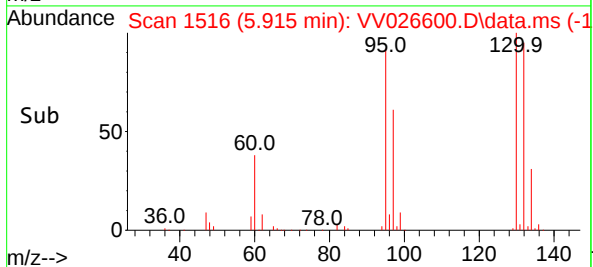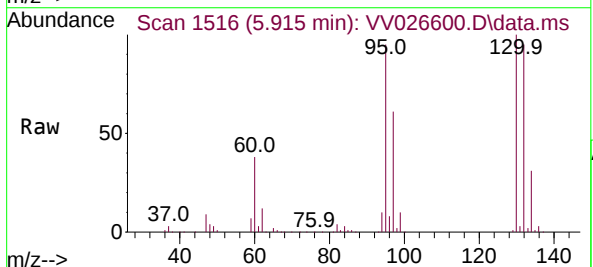

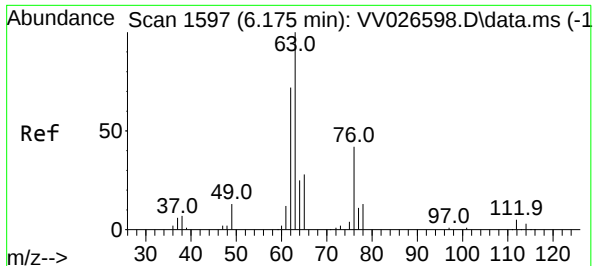

#37

1,2-Dichloropropane

Concen: 41.764 ug/L

RT: 6.175 min Scan# 11

Delta R.T. -0.000 min

Lab File: VV026600.D

Acq: 30 Jun 2022 12:18

Instrument :

MSVOA_V

ClientSampleId :





A0AH0

Tgt Ion: 63 Resp: 144968

Ion Ratio Lower Upper

63 100

112 4.9 4.2 6.2

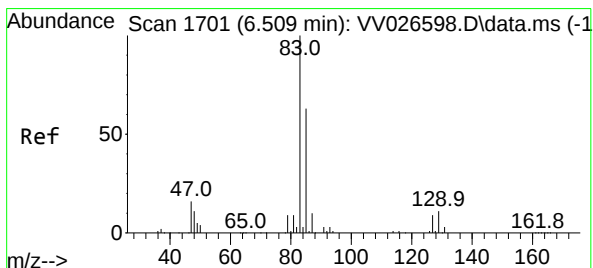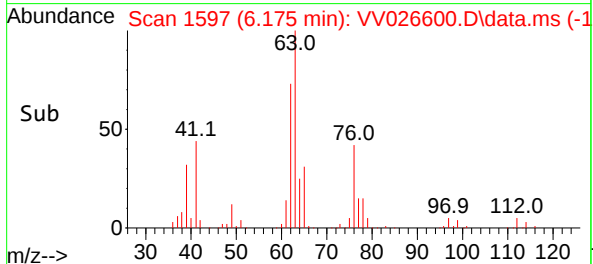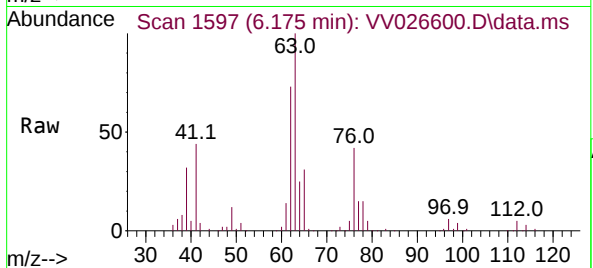

#38

Bromodichloromethane

Concen: 20.624 ug/L

RT: 6.513 min Scan# 1702

Delta R.T. 0.003 min

Lab File: VV026600.D

Acq: 30 Jun 2022 12:18




Tgt Ion: 83 Resp: 91991


Ion Ratio Lower Upper

83 100

85 64.2 44.6 82.8

127 8.3 7.3 10.9

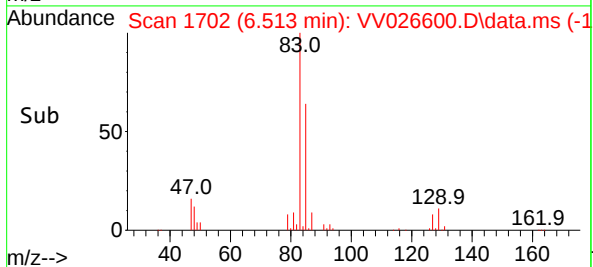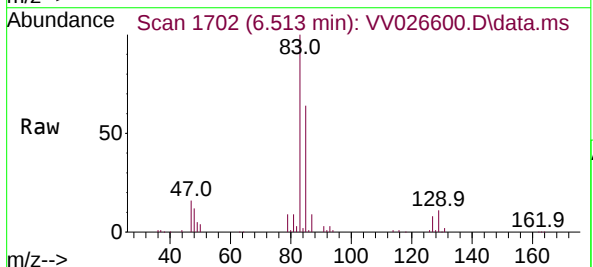



#39

cis-1,3-Dichloropropene

Concen: 26.197 ug/L

RT: 7.027 min Scan# 11

Delta R.T. -0.000 min

Lab File: VV026600.D

Acq: 30 Jun 2022 12:18

Instrument :

MSVOA_V

ClientSampleId :





A0AH0

Tgt Ion: 75 Resp: 122447

Ion Ratio Lower Upper

75 100

77 30.7 22.4 41.6

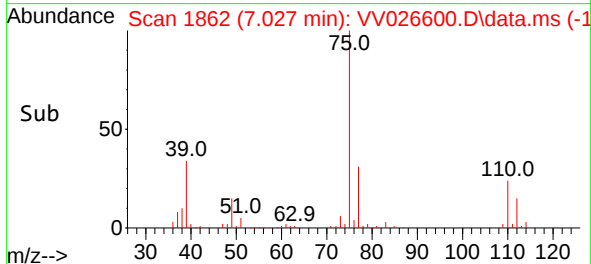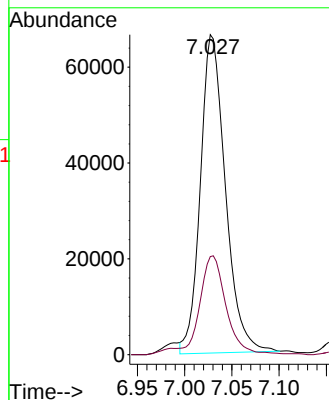

#44

trans-1,3-Dichloropropene

Concen: 45.935 ug/L

RT: 7.651 min Scan# 2056

Delta R.T. -0.000 min

Lab File: VV026600.D




Acq: 30 Jun 2022 12:18


Tgt Ion: 75 Resp: 197993

Ion Ratio Lower Upper

75 100

77 31.7 22.6 42.0



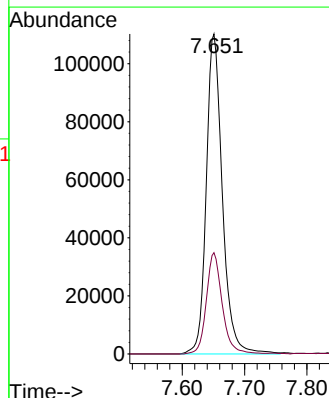
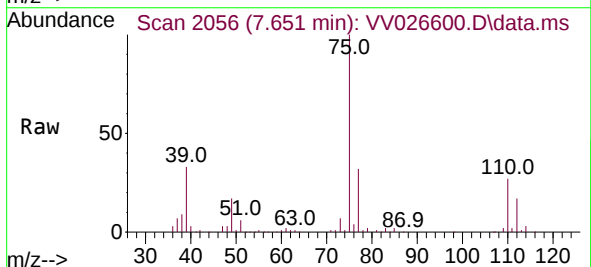


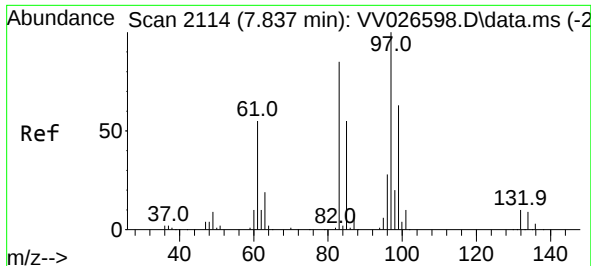

#45
1,1,2-Trichloroethane
Concen: 26.845 ug/L
RT: 7.837 min Scan# 2114
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18




Instrument :
MSVOA_V
ClientSampleId :
A0AH0


Tgt Ion:	97	Resp:	94583
Ion	Ratio	Lower	Upper
97	100		
99	63.2	42.8	79.6
83	84.1	59.1	109.7
85	54.5	37.7	70.1

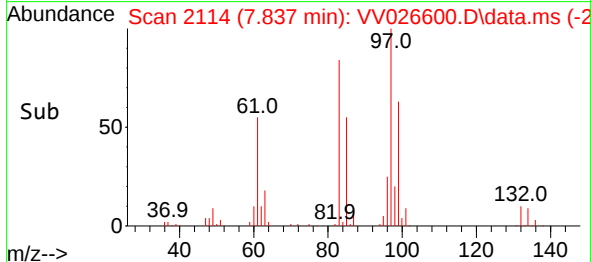

#46
Tetrachloroethene
Concen: 78.367 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion:	164	Resp:	213010
Ion	Ratio	Lower	Upper
164	100		
129	95.9	66.1	122.8
131	91.9	64.2	119.2
166	126.9	88.1	163.7


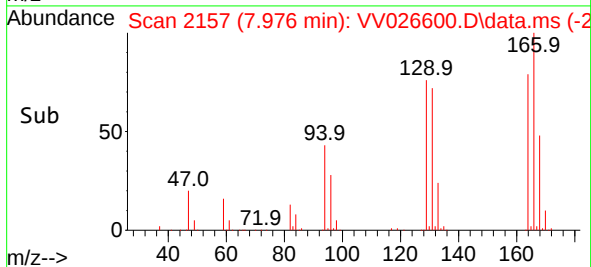
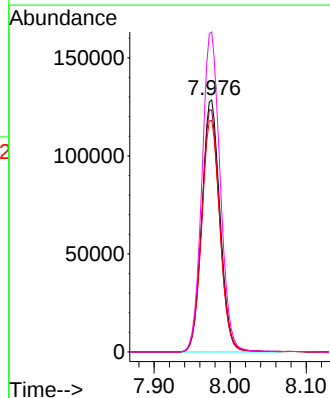
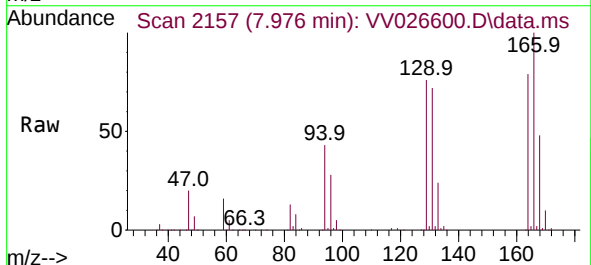


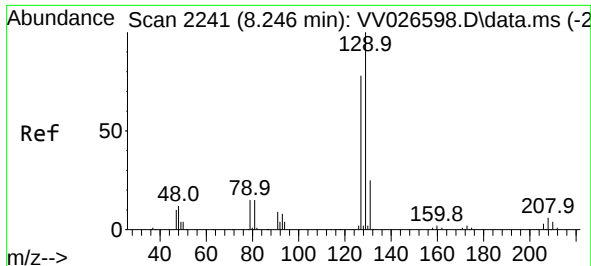

#49
 Dibromochloromethane
 Concen: 37.175 ug/L
 RT: 8.246 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18




Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0


Tgt Ion:129 Resp: 126077
 Ion Ratio Lower Upper
 129 100
 127 77.9 54.1 100.5

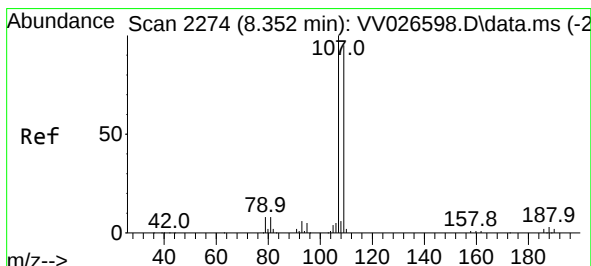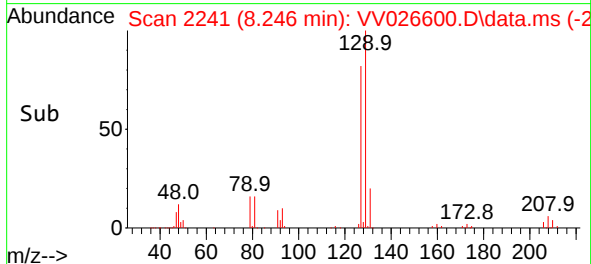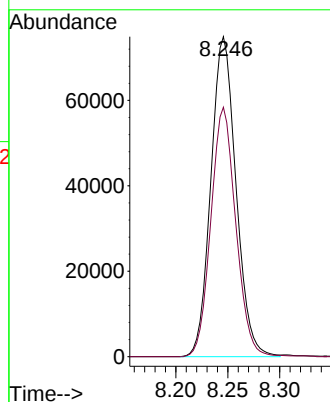

#50
 1,2-Dibromoethane
 Concen: 31.105 ug/L
 RT: 8.352 min Scan# 2274
 Delta R.T. -0.000 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Tgt Ion:107 Resp: 111217
 Ion Ratio Lower Upper
 107 100
 109 92.0 67.3 125.1
 188 3.4 2.7 4.1


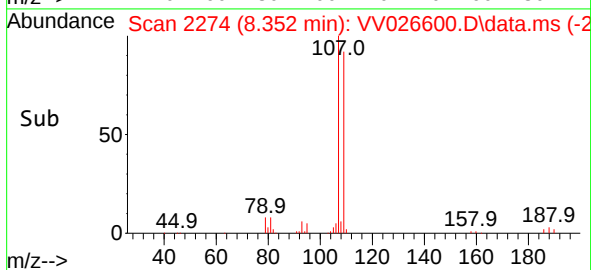
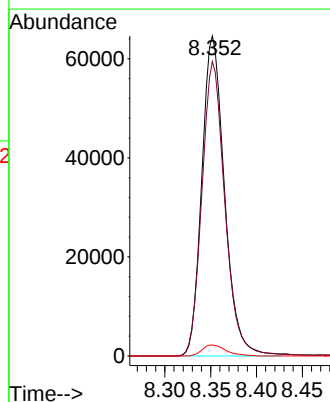
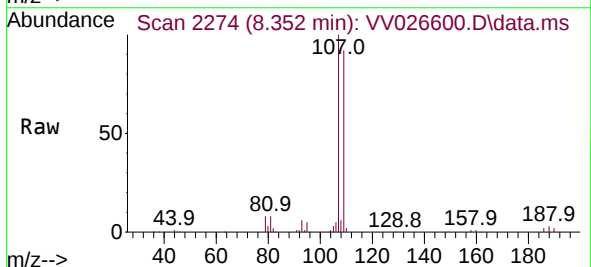




#57
 1,1,2,2-Tetrachloroethane
 Concen: 38.124 ug/L
 RT: 10.239 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18




Instrument :
 MSVOA_V
 ClientSampleId :
 A0AH0


Tgt Ion: 83 Resp: 209054
 Ion Ratio Lower Upper
 83 100
 85 63.9 44.6 82.8
 131 9.9 7.6 11.4

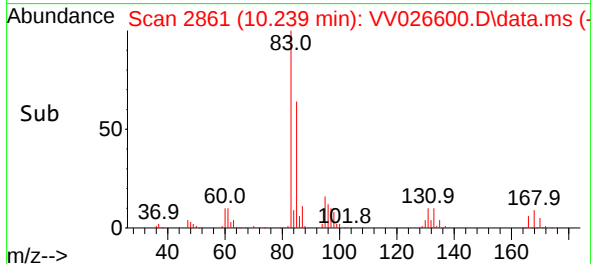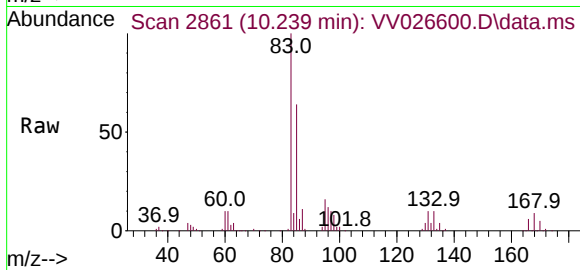

#59
 Bromoform
 Concen: 44.044 ug/L
 RT: 9.731 min Scan# 2703
 Delta R.T. 0.003 min
 Lab File: VV026600.D
 Acq: 30 Jun 2022 12:18

Tgt Ion: 173 Resp: 82348
 Ion Ratio Lower Upper
 173 100
 175 49.5 39.1 58.7
 254 8.8 7.1 10.7


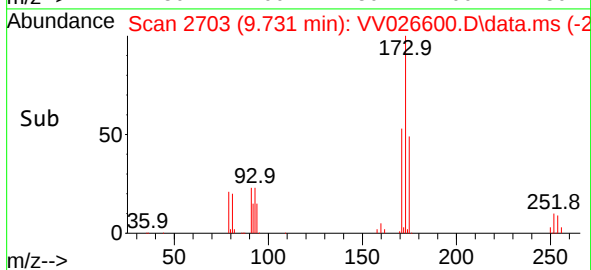

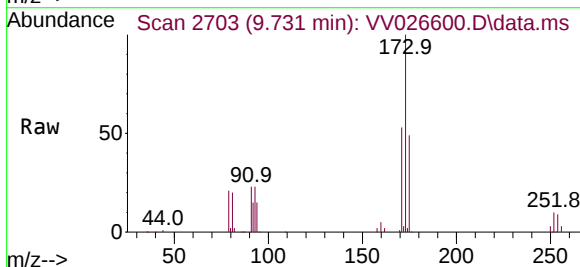




#63
1,2,4-Trimethylbenzene
Concen: 49.974 ug/L
RT: 10.914 min Scan# 3070
Delta R.T. 0.003 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
A0AH0

Tgt Ion:105 Resp: 522112
Ion Ratio Lower Upper
105 100
120 47.1 37.5 56.3

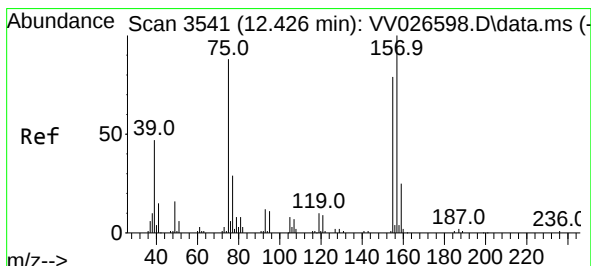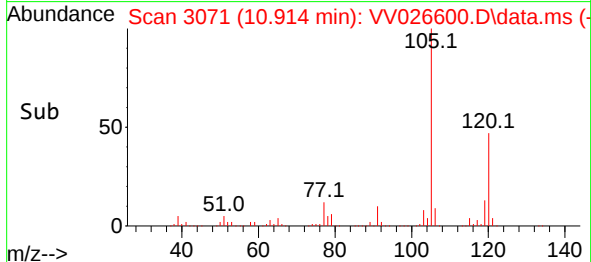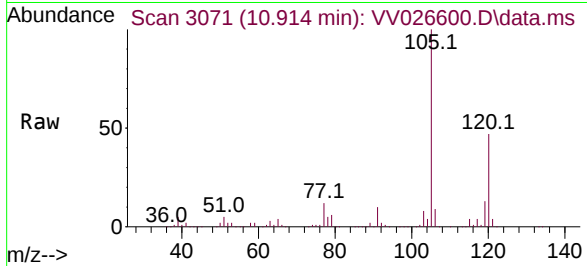

#68
1,2-Dibromo-3-chloropropane
Concen: 40.261 ug/L
RT: 12.426 min Scan# 3541
Delta R.T. -0.000 min
Lab File: VV026600.D
Acq: 30 Jun 2022 12:18

Tgt Ion: 75 Resp: 34201
Ion Ratio Lower Upper
75 100
155 92.8 71.0 106.4
157 119.8 91.3 136.9

