

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW063022\
 Data File : VW026603.D
 Acq On : 30 Jun 2022 13:32
 Operator : SY/MD
 Sample : N3521-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JW6

Quant Time: Jul 01 00:21:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 01 00:19:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	382904	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	379125	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	164514	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	135521	43.418	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.840%
7) Chloroethane-d5	1.581	69	123583	46.167	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.340%
11) 1,1-Dichloroethene-d2	2.121	63	198815	33.814	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.620%
21) 2-Butanone-d5	3.918	46	153909	98.488	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.490%
24) Chloroform-d	4.362	84	272521	45.217	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.440%
26) 1,2-Dichloroethane-d4	5.040	65	164064	47.841	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.680%
32) Benzene-d6	5.060	84	531914	46.139	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.280%
36) 1,2-Dichloropropane-d6	6.076	67	172042	47.379	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.760%
41) Toluene-d8	7.317	98	441402	43.591	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.180%
43) trans-1,3-Dichloroprop...	7.625	79	60698	41.634	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.260%
47) 2-Hexanone-d5	8.092	63	112627	89.680	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.680%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	242082	46.173	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.340%
66) 1,2-Dichlorobenzene-d4	11.622	152	169339	52.594	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.180%
Target Compounds						Qvalue
3) Chloromethane	1.253	50	7441	2.180	ug/L	94
61) 1,2,3-Trichloropropane	11.246	75	18502	6.280	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV063022\
Data File : VV026603.D
Acq On : 30 Jun 2022 13:32
Operator : SY/MD
Sample : N3521-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JW6

Quant Time: Jul 01 00:21:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 01 00:19:36 2022
Response via : Initial Calibration

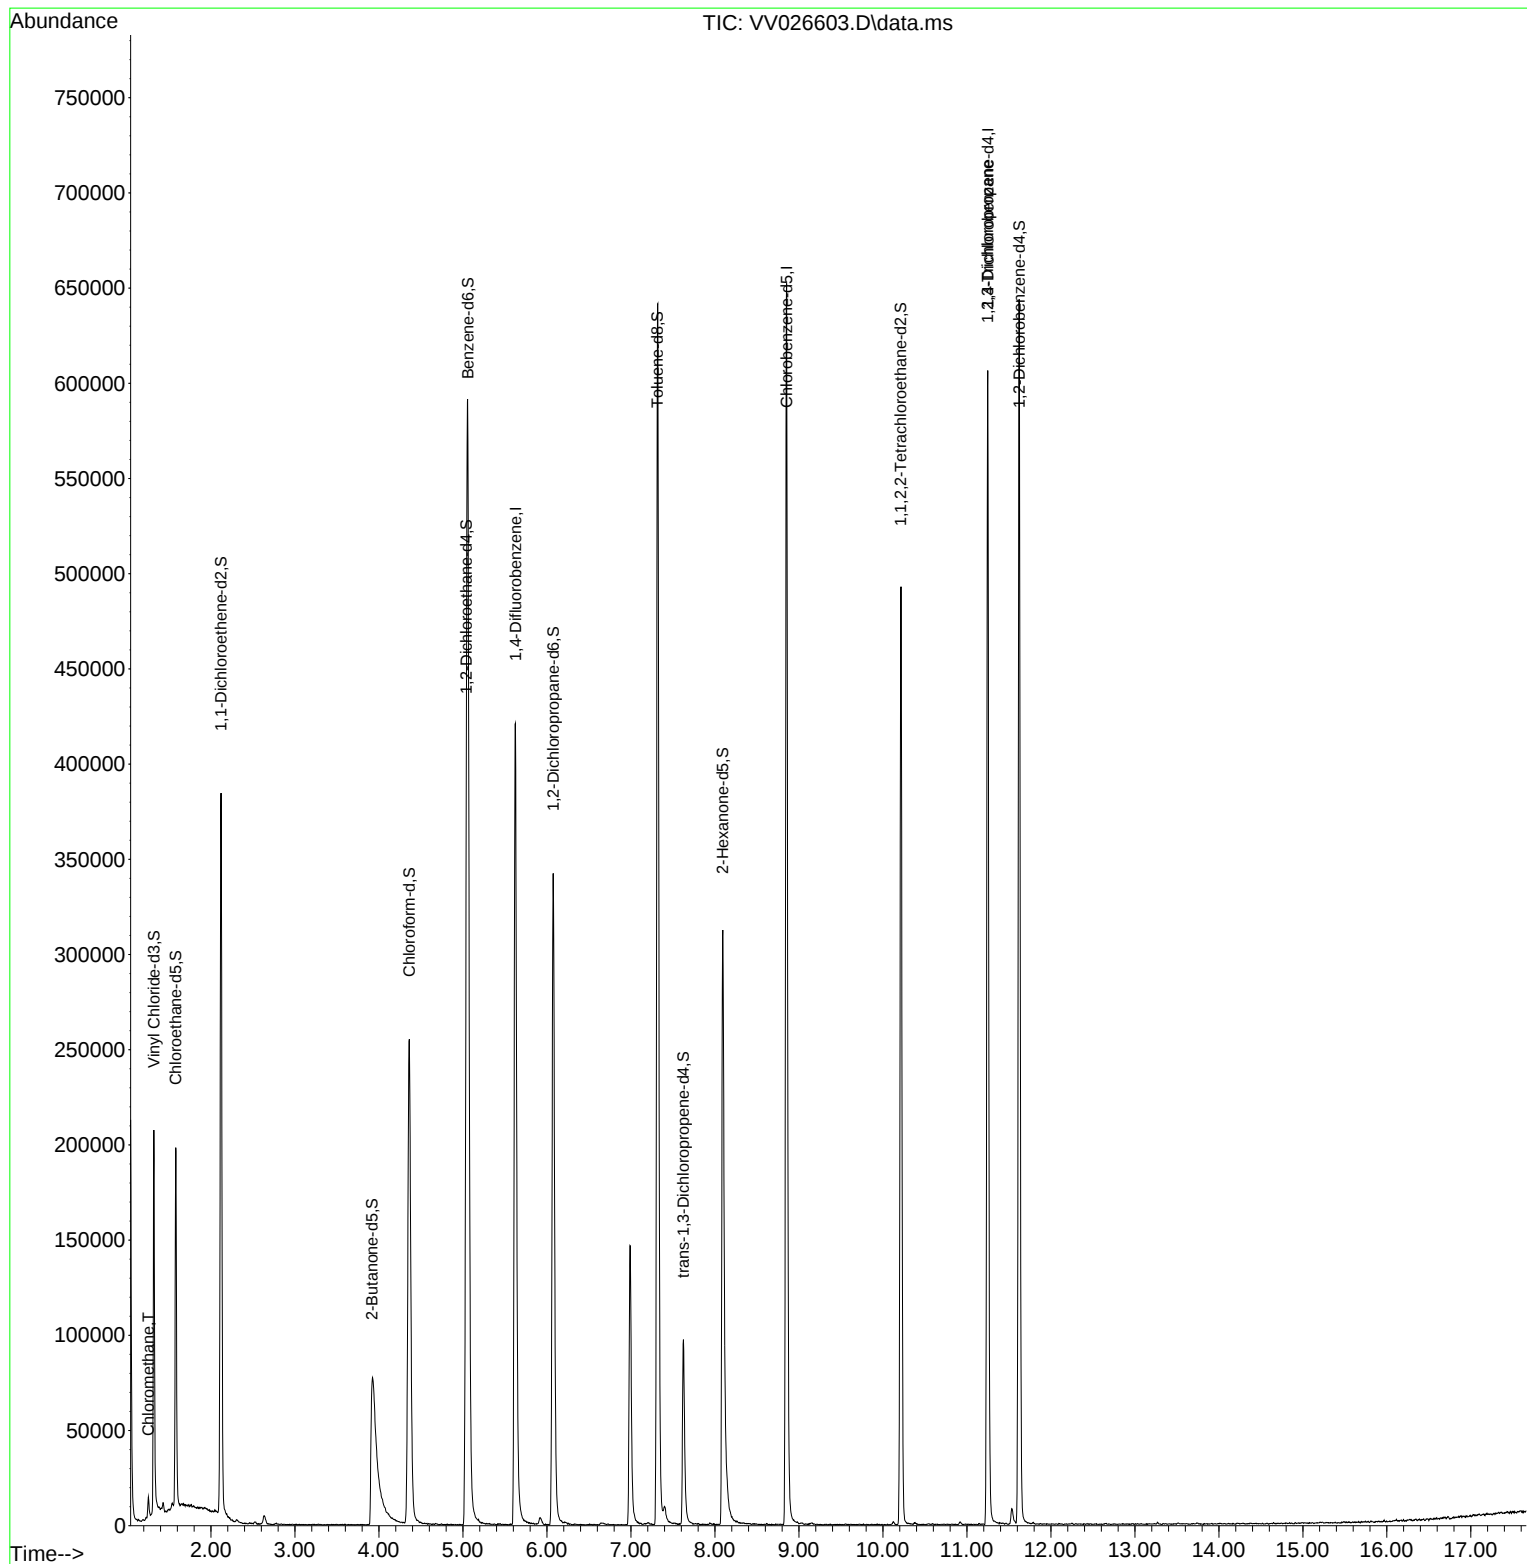

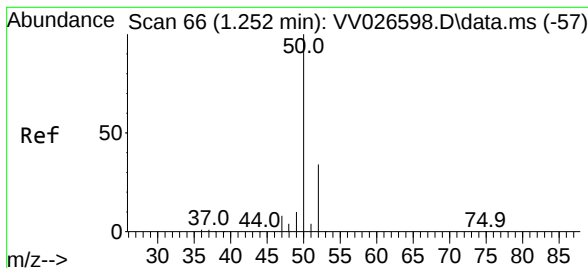

#3

Chloromethane

Concen: 2.180 ug/L

RT: 1.253 min Scan# 60

Delta R.T. 0.000 min

Lab File: VV026603.D

Acq: 30 Jun 2022 13:32

Instrument :

MSVOA_V

ClientSampleId :





C0JW6

Tgt Ion: 50 Resp: 7441

Ion Ratio Lower Upper

50 100

52 36.3 23.1 42.9

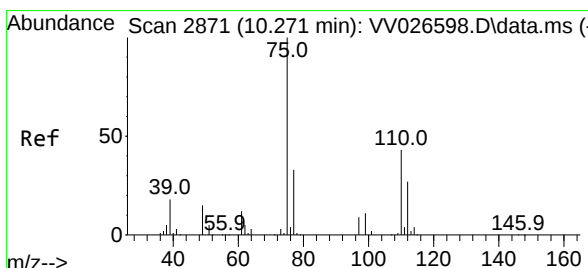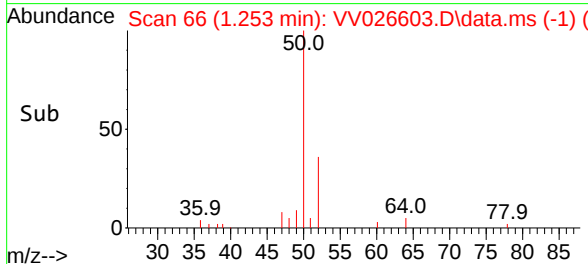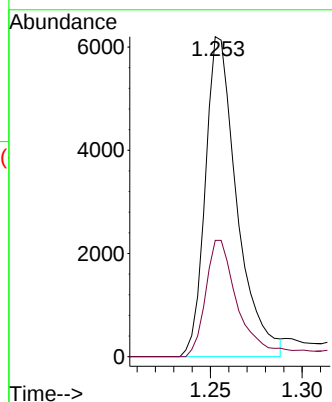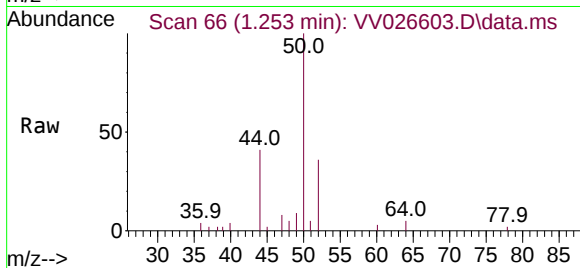

#61

1,2,3-Trichloropropane

Concen: 6.280 ug/L

RT: 11.246 min Scan# 3174

Delta R.T. 0.974 min

Lab File: VV026603.D

Acq: 30 Jun 2022 13:32

Tgt Ion: 75 Resp: 18502

Ion Ratio Lower Upper

75 100

77 32.5 25.8 38.6

110 1.4 32.8 49.2#

